

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082119\
 Data File : FB022053.D
 Signal(s) : FID2B.CH
 Acq On : 21 Aug 2019 10:30
 Operator : DD/AJ
 Sample : BSF0821S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 21 15:48:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.984	431380	20.310 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	1169695	29.226 ng/ml
2) t 2,2,4-Trimethylpentane	7.604	1142561	28.367 ng/ml
3) t n-Heptane	7.943	360995	9.450 ng/ml
4) t Benzene	8.079	432343	9.630 ng/ml
6) t Toluene	10.825	883451	28.737 ng/ml
7) t Ethylbenzene	13.270	203741	9.984 ng/ml
8) t m-Xylene	13.403	426652	20.258 ng/ml
9) t O-Xylene	14.132	447447	20.006 ng/ml
10) t 1,2,4-Trimethylbenzene	16.412	497506	19.399 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082119\
Data File : FB022053.D
Signal(s) : FID2B.CH
Acq On : 21 Aug 2019 10:30
Operator : DD/AJ
Sample : BSF0821S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 21 15:48:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

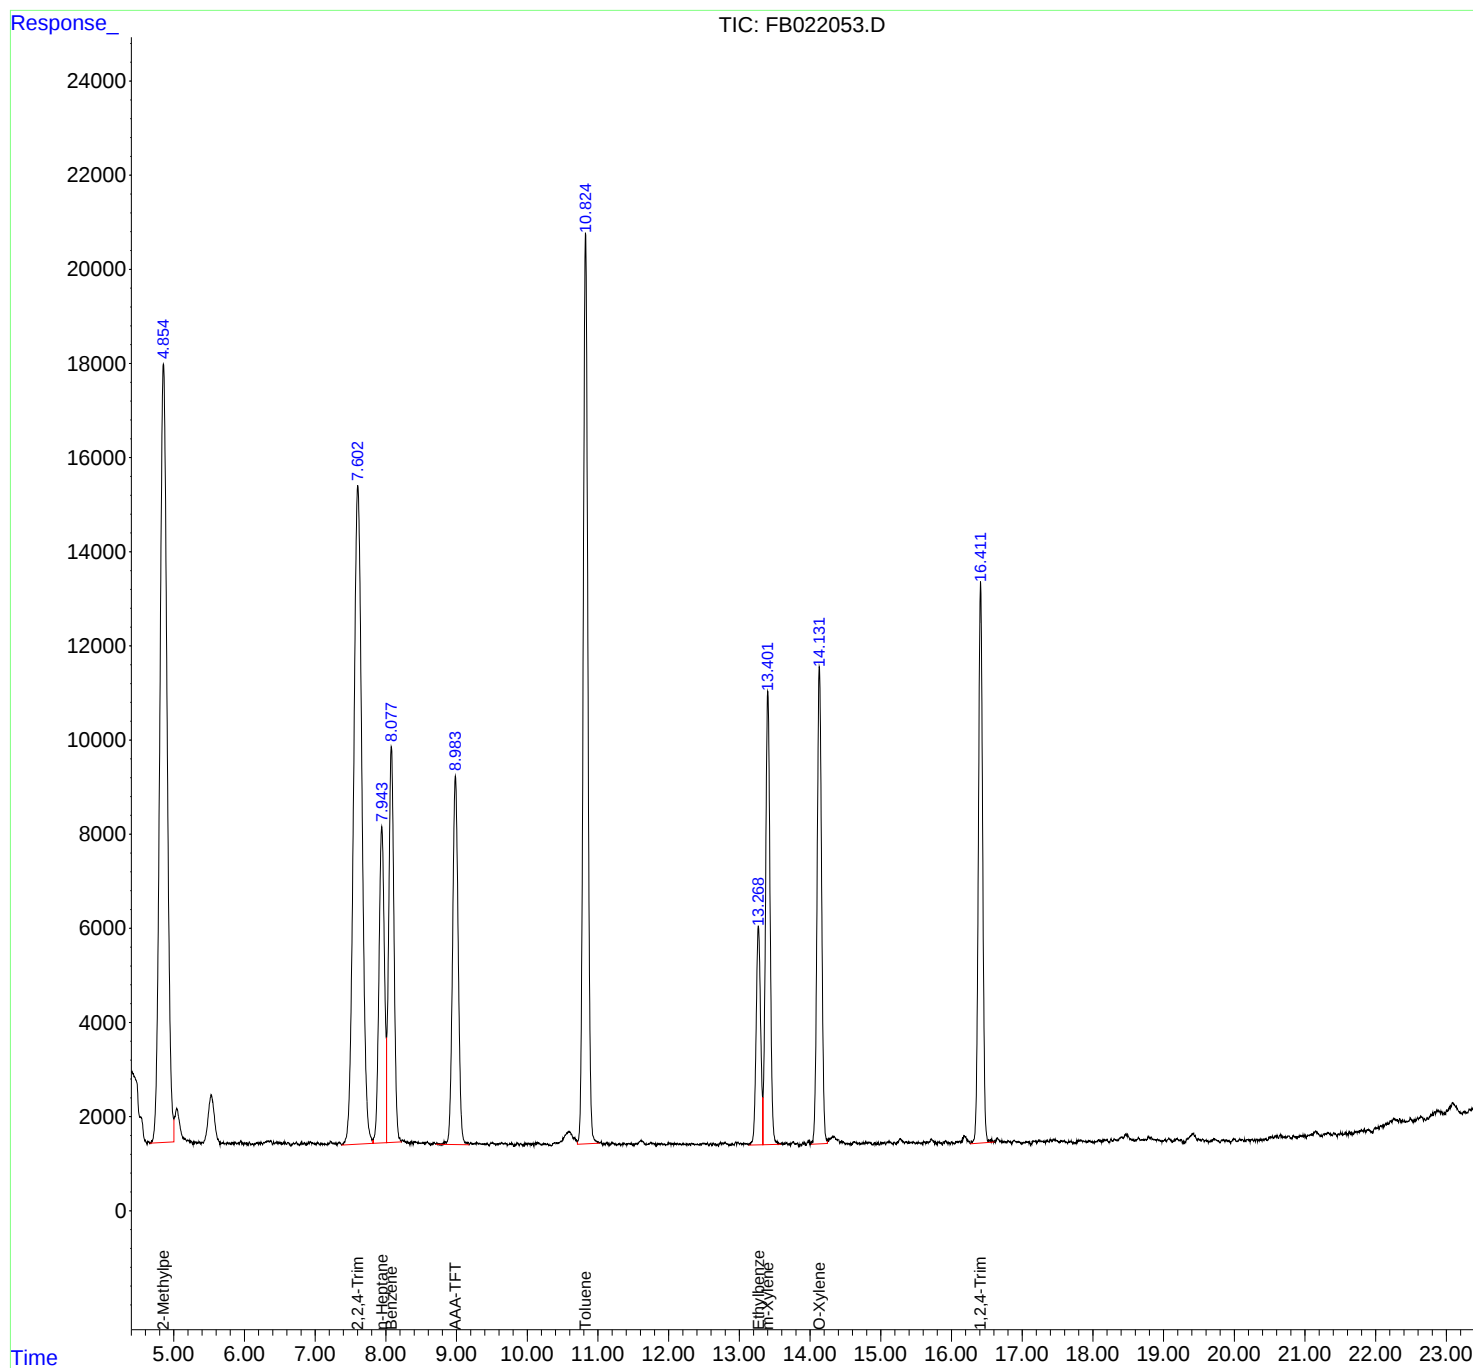

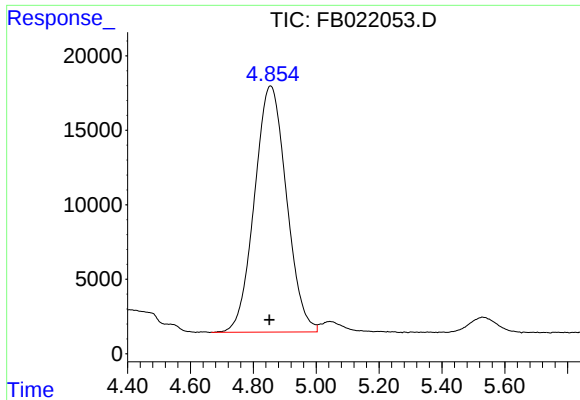


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: 0.003 min
Response: 1169695
Conc: 29.23 ng/ml

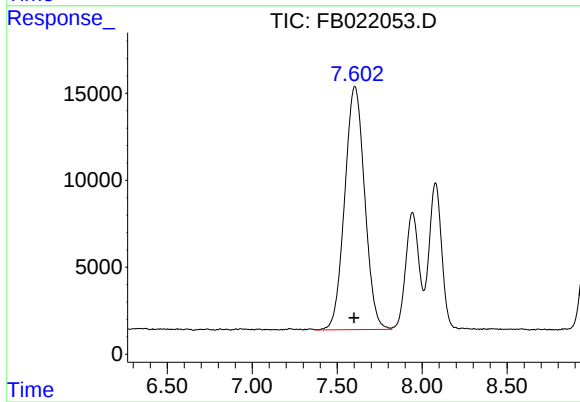


#2 2,2,4-Trimethylpentane

R.T.: 7.604 min
Delta R.T.: 0.005 min
Response: 1142561
Conc: 28.37 ng/ml

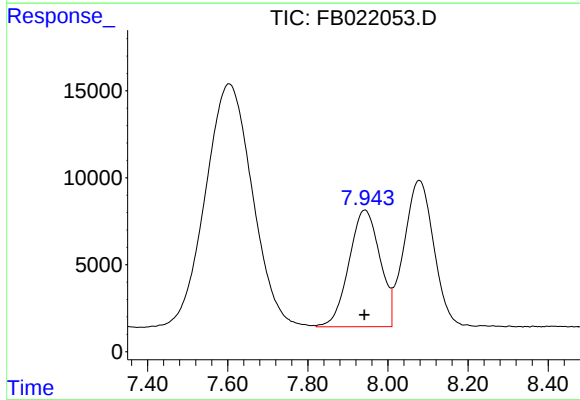


#3 n-Heptane

R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 360995
Conc: 9.45 ng/ml

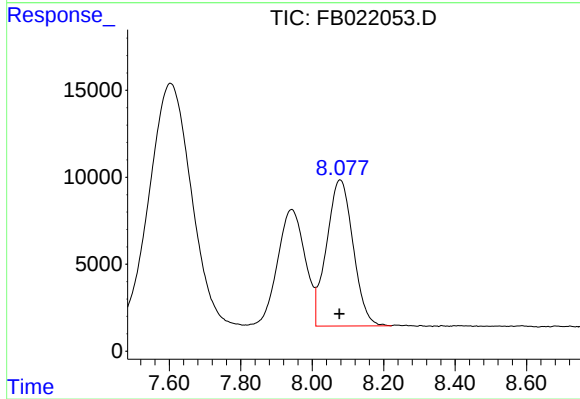


#4 Benzene

R.T.: 8.079 min
Delta R.T.: 0.002 min
Response: 432343
Conc: 9.63 ng/ml

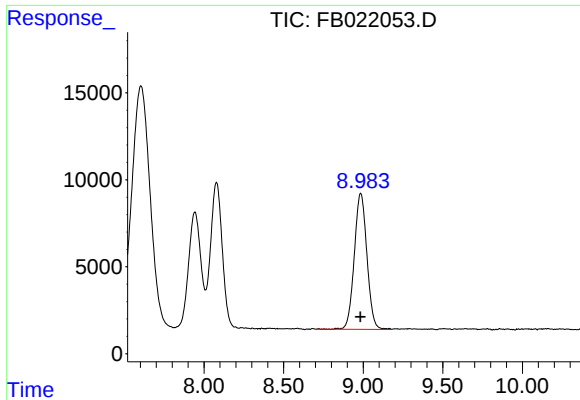


#5 AAA-TFT

R.T.: 8.984 min
 Delta R.T.: 0.002 min
 Response: 431380
 Conc: 20.31 ng/ml

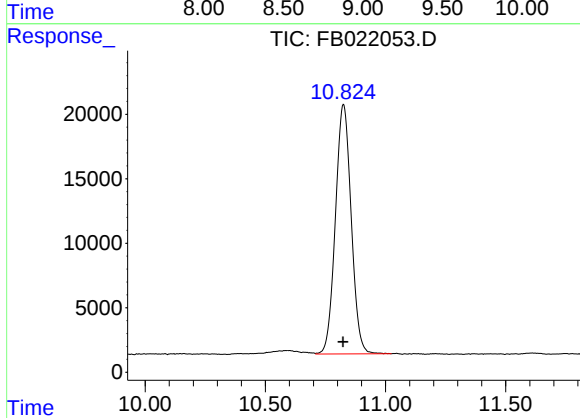


#6 Toluene

R.T.: 10.825 min
 Delta R.T.: 0.003 min
 Response: 883451
 Conc: 28.74 ng/ml

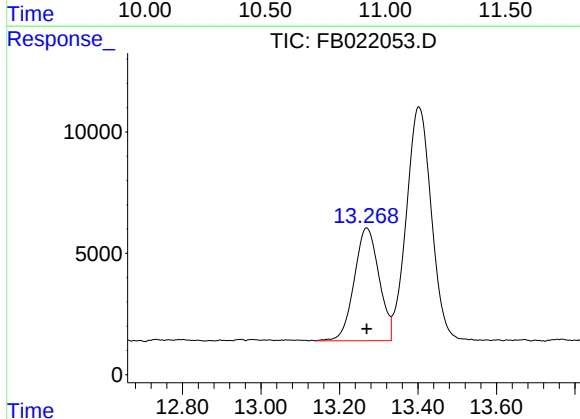


#7 Ethylbenzene

R.T.: 13.270 min
 Delta R.T.: 0.000 min
 Response: 203741
 Conc: 9.98 ng/ml

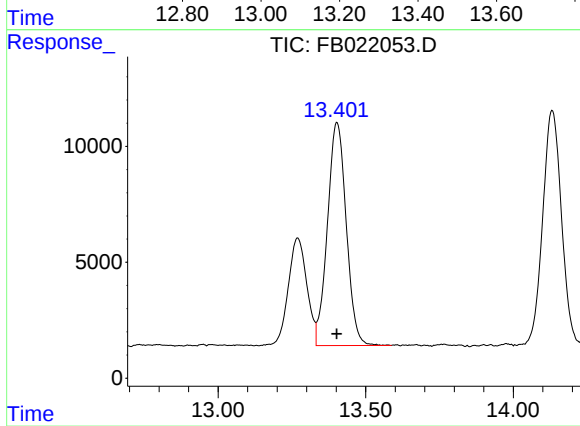


#8 m-Xylene

R.T.: 13.403 min
 Delta R.T.: 0.001 min
 Response: 426652
 Conc: 20.26 ng/ml

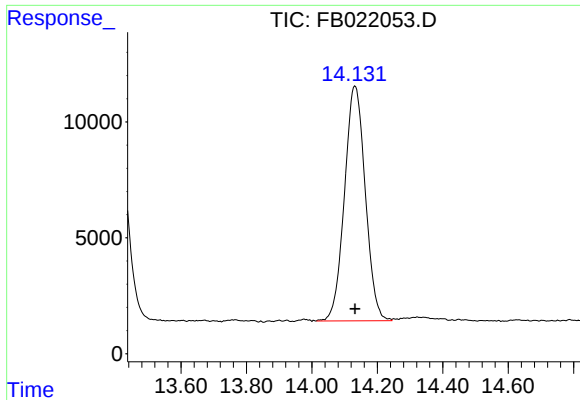

#9 O-Xylene

R.T.: 14.132 min
Delta R.T.: 0.000 min
Response: 447447
Conc: 20.01 ng/ml

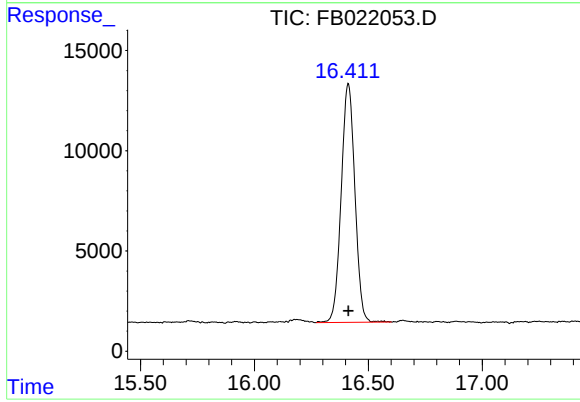

#10 1,2,4-Trimethylbenzene

R.T.: 16.412 min
Delta R.T.: 0.000 min
Response: 497506
Conc: 19.40 ng/ml