

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082119\
 Data File : FB022057.D
 Signal(s) : FID2B.CH
 Acq On : 21 Aug 2019 13:15
 Operator : DD/AJ
 Sample : K4095-10MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 21 15:48:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.982	436650	20.558 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.852	1096042	27.386 ng/ml
2) t 2,2,4-Trimethylpentane	7.602	1026115	25.476 ng/ml
3) t n-Heptane	7.941	171992	4.502 ng/ml
4) t Benzene	8.075	465797	10.376 ng/ml
6) t Toluene	10.823	942078	30.644 ng/ml
7) t Ethylbenzene	13.269	200126	9.807 ng/ml
8) t m-Xylene	13.402	369415	17.541 ng/ml
9) t O-Xylene	14.131	421872	18.863 ng/ml
10) t 1,2,4-Trimethylbenzene	16.411	337266	13.151 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082119\
Data File : FB022057.D
Signal(s) : FID2B.CH
Acq On : 21 Aug 2019 13:15
Operator : DD/AJ
Sample : K4095-10MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 21 15:48:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

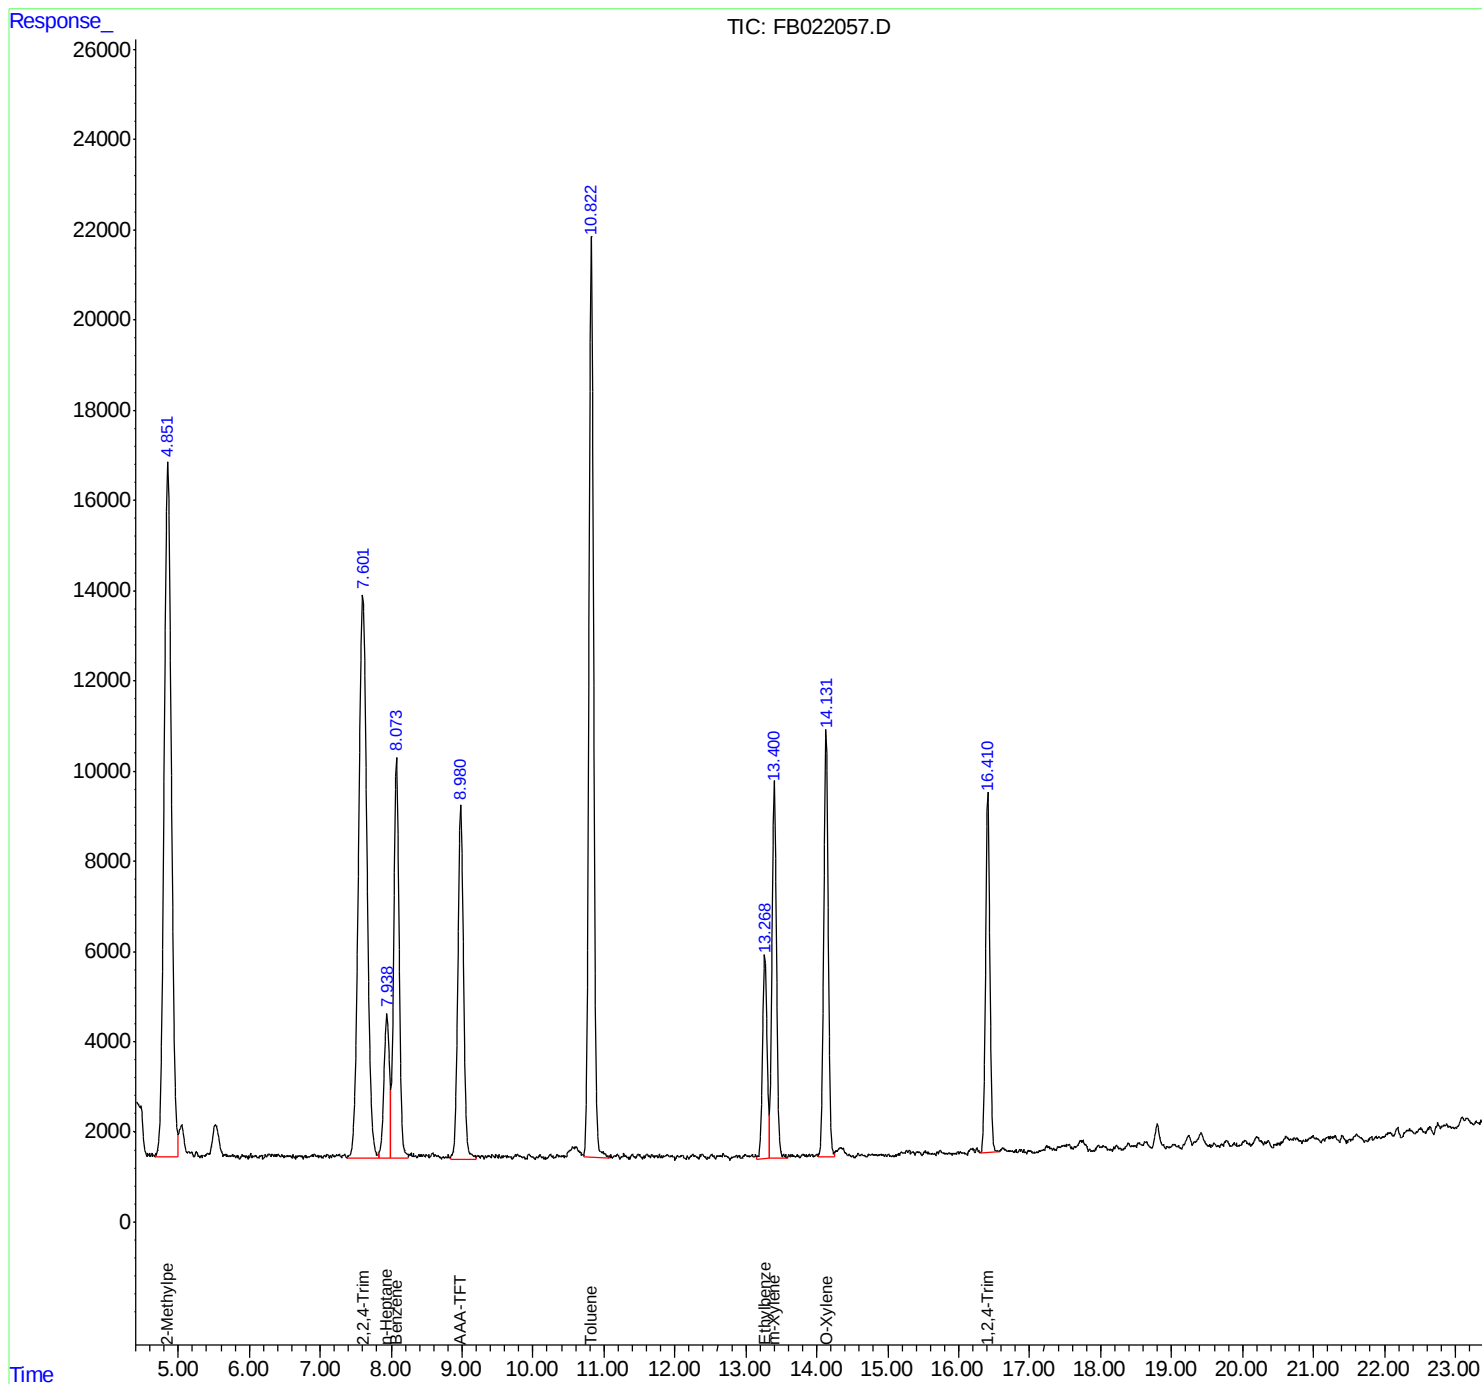

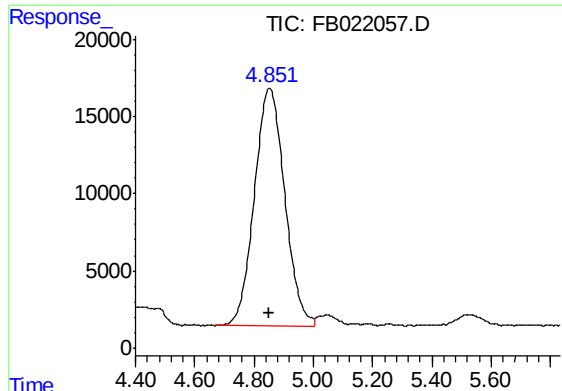


#1 2-Methylpentane

R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 1096042
Conc: 27.39 ng/ml

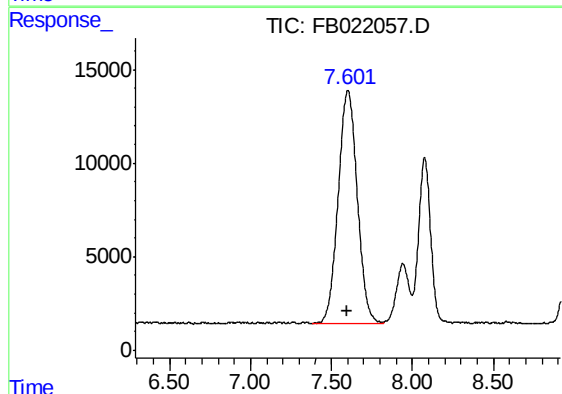


#2 2,2,4-Trimethylpentane

R.T.: 7.602 min
Delta R.T.: 0.002 min
Response: 1026115
Conc: 25.48 ng/ml

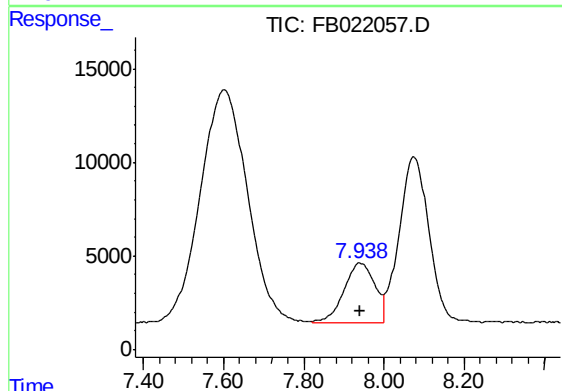


#3 n-Heptane

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 171992
Conc: 4.50 ng/ml

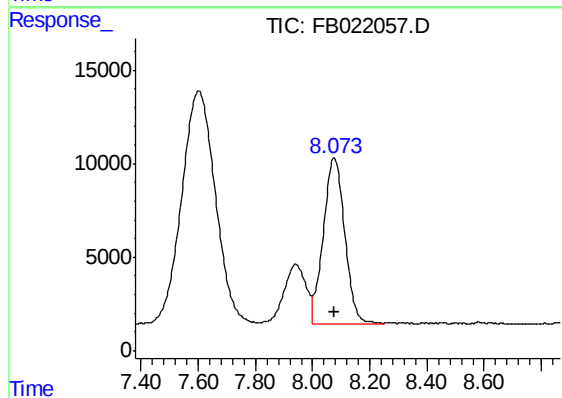


#4 Benzene

R.T.: 8.075 min
Delta R.T.: -0.001 min
Response: 465797
Conc: 10.38 ng/ml

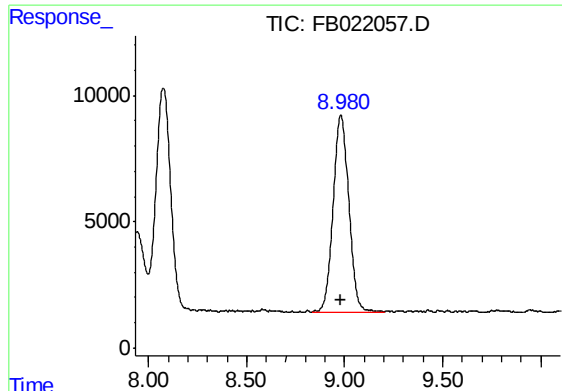


#5 AAA-TFT

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 436650
Conc: 20.56 ng/ml

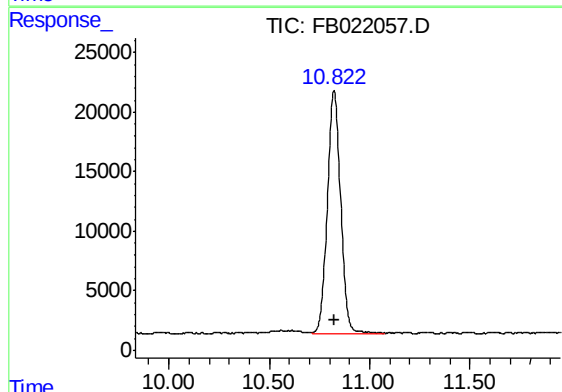


#6 Toluene

R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 942078
Conc: 30.64 ng/ml

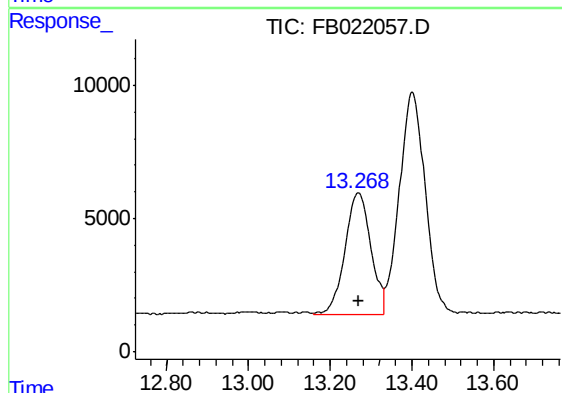


#7 Ethylbenzene

R.T.: 13.269 min
Delta R.T.: 0.000 min
Response: 200126
Conc: 9.81 ng/ml

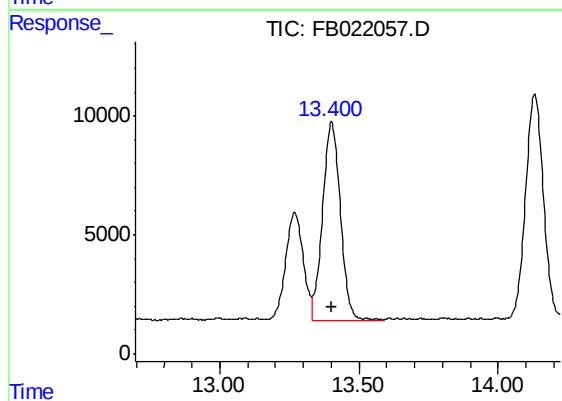


#8 m-Xylene

R.T.: 13.402 min
Delta R.T.: 0.000 min
Response: 369415
Conc: 17.54 ng/ml

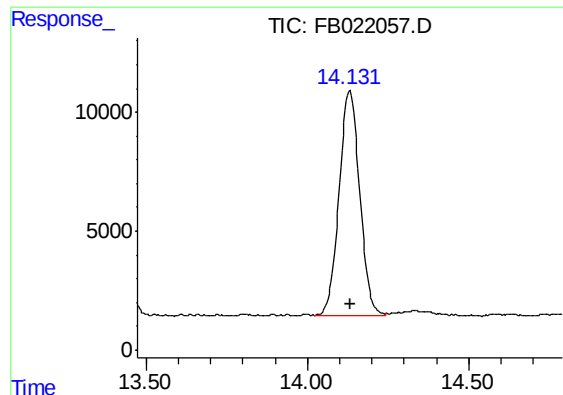

#9 O-Xylene

R.T.: 14.131 min
Delta R.T.: 0.000 min
Response: 421872
Conc: 18.86 ng/ml

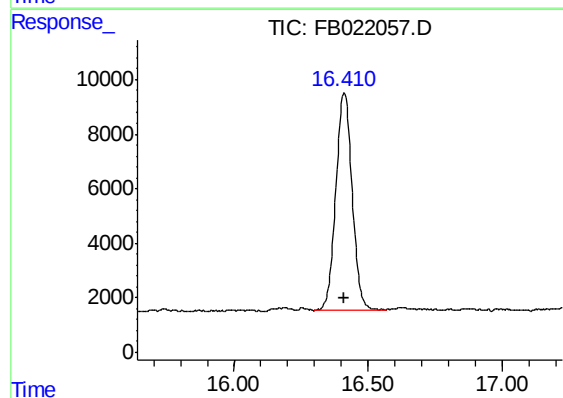

#10 1,2,4-Trimethylbenzene

R.T.: 16.411 min
Delta R.T.: 0.000 min
Response: 337266
Conc: 13.15 ng/ml