

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082120\
 Data File : FB024776.D
 Signal(s) : FID2B.CH
 Acq On : 21 Aug 2020 10:35
 Operator : DD/AJ
 Sample : BSF0821S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 21 23:48:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	418691	20.276 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	779457	32.390 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	926635	33.429 ng/ml
3) t n-Heptane	7.755	299650	11.020 ng/ml
4) t Benzene	7.889	363786	10.366 ng/ml
6) t Toluene	10.628	1068355	31.015 ng/ml
7) t Ethylbenzene	13.068	337795	10.552 ng/ml
8) t m-Xylene	13.201	660555	21.169 ng/ml
9) t O-Xylene	13.929	636727	21.054 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	527655	21.485 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082120\
Data File : FB024776.D
Signal(s) : FID2B.CH
Acq On : 21 Aug 2020 10:35
Operator : DD/AJ
Sample : BSF0821S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 21 23:48:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

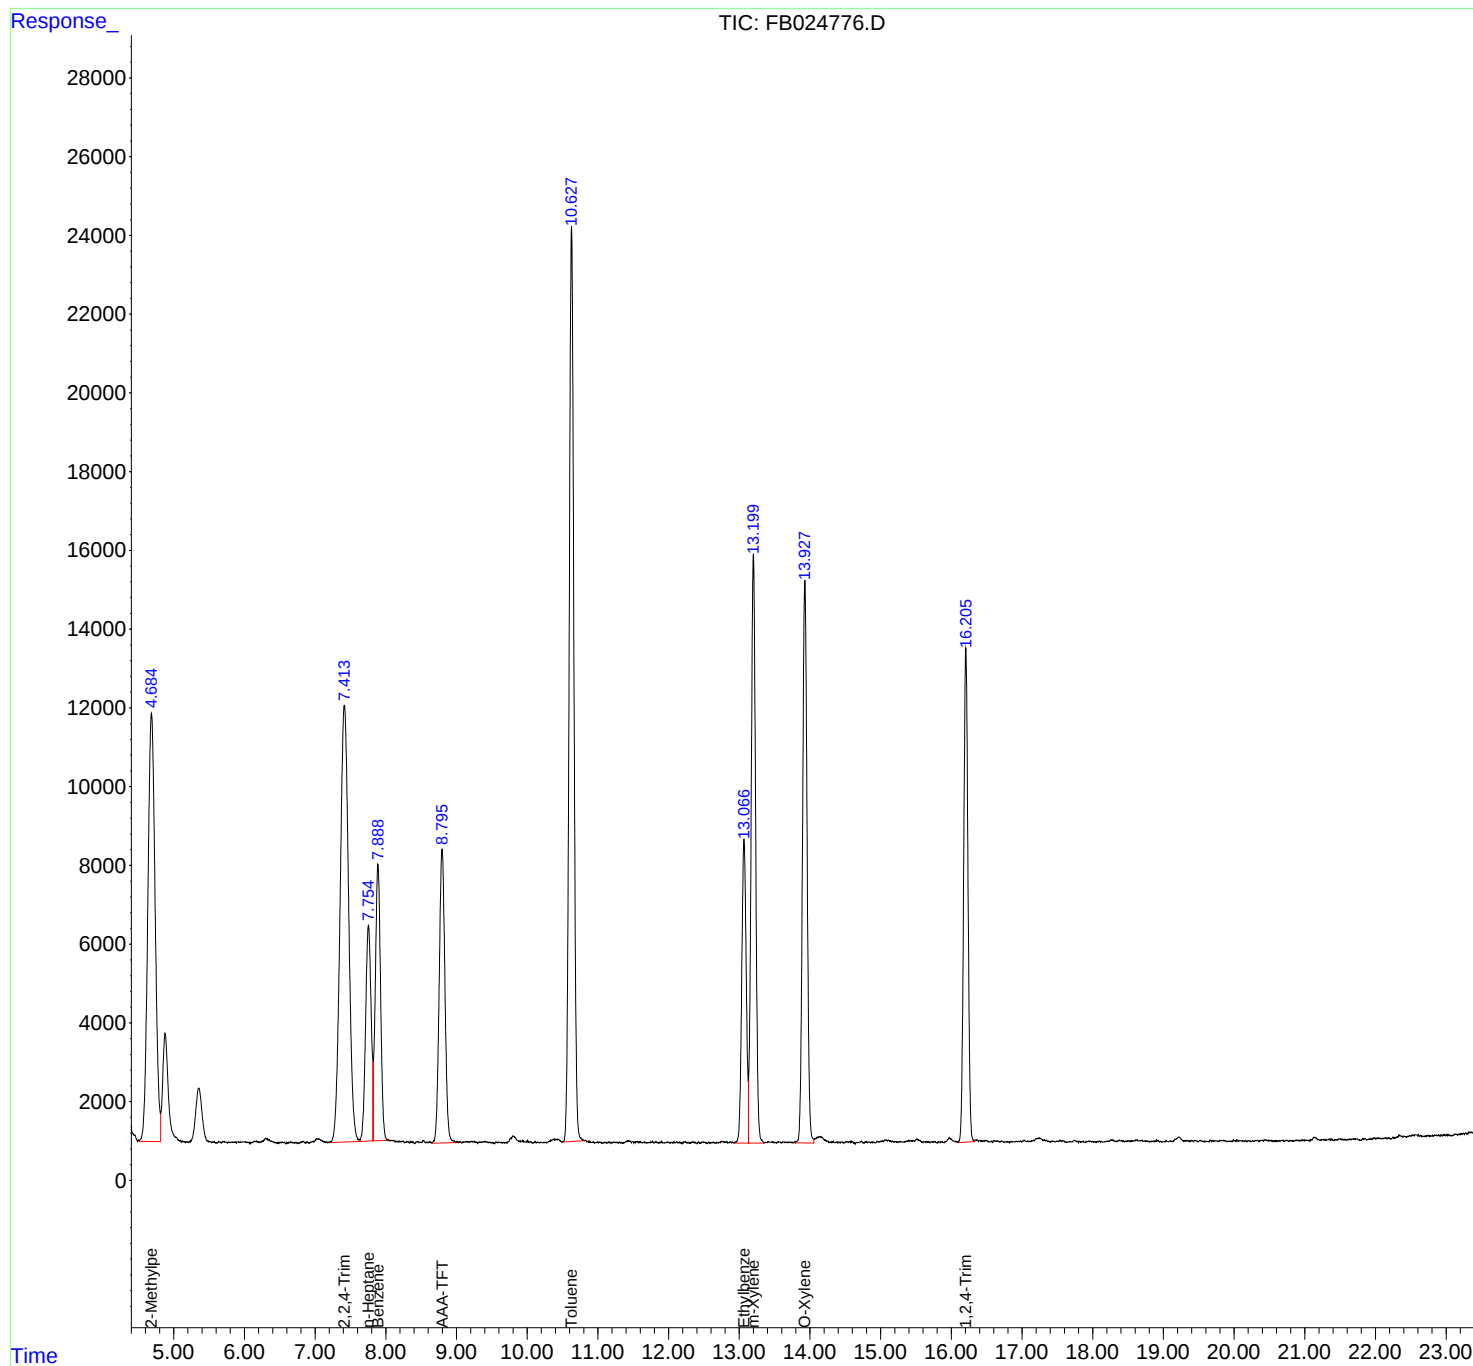

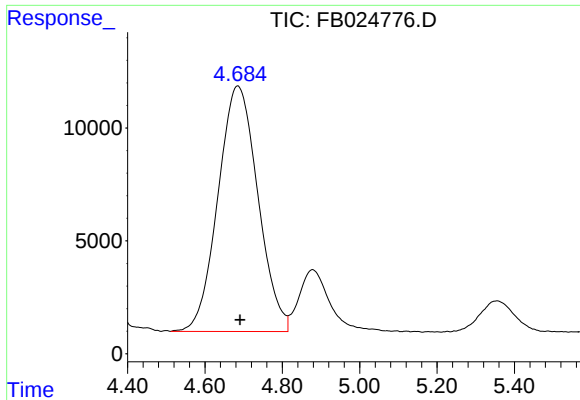


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.005 min
Response: 779457
Conc: 32.39 ng/ml

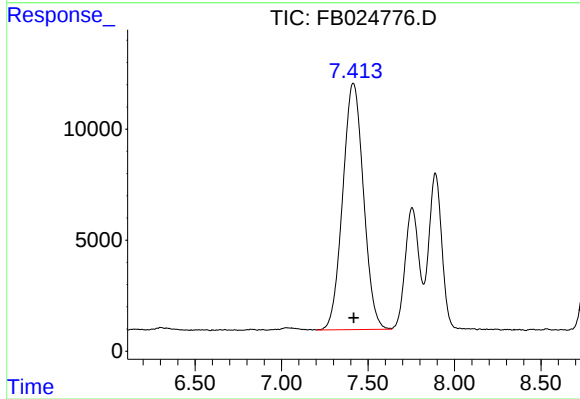


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.003 min
Response: 926635
Conc: 33.43 ng/ml

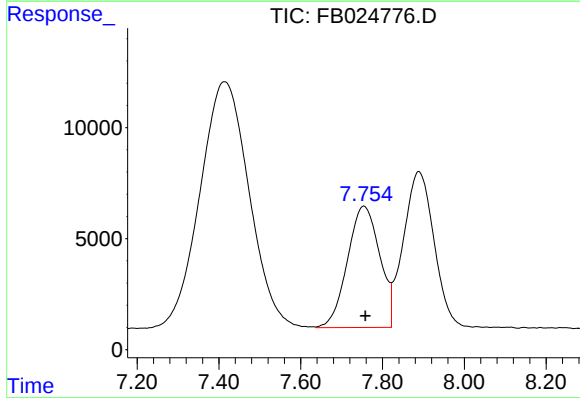


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 299650
Conc: 11.02 ng/ml

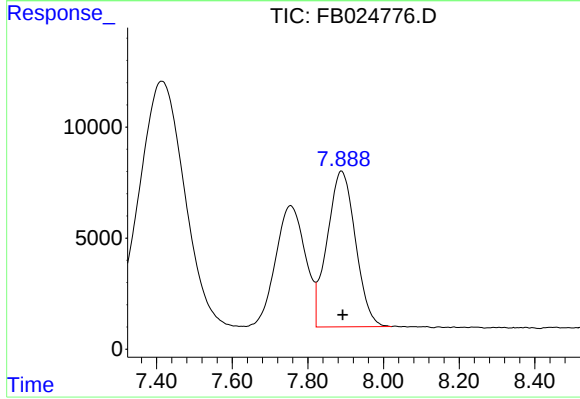


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 363786
Conc: 10.37 ng/ml

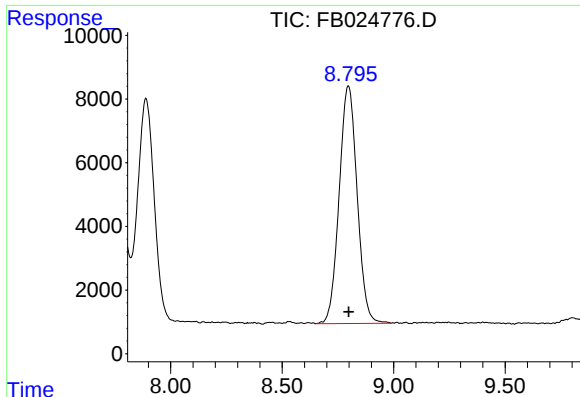


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 418691
Conc: 20.28 ng/ml

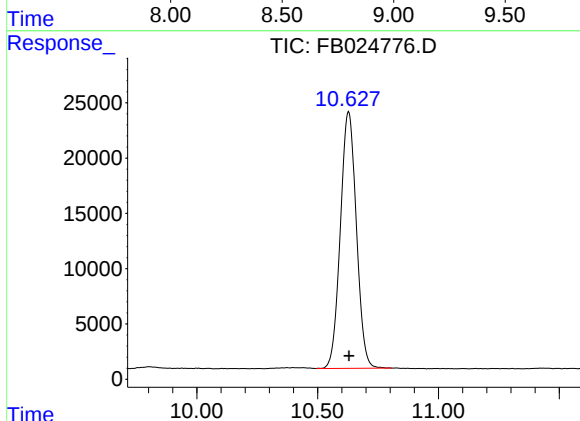


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.001 min
Response: 1068355
Conc: 31.01 ng/ml

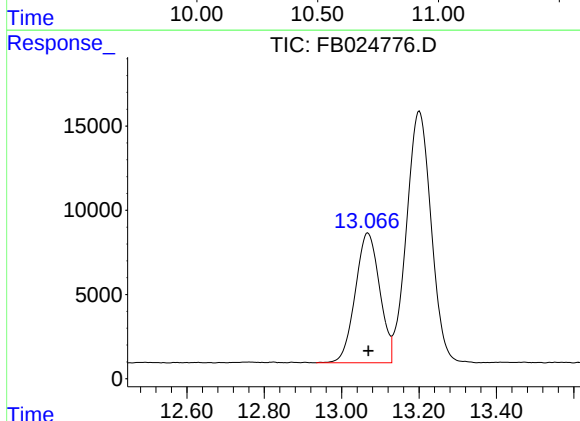


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.001 min
Response: 337795
Conc: 10.55 ng/ml

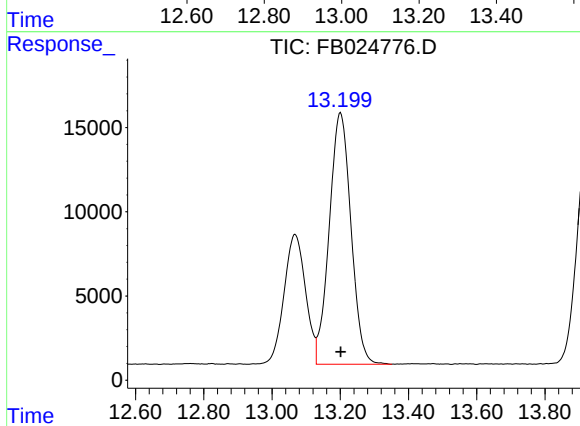


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 660555
Conc: 21.17 ng/ml

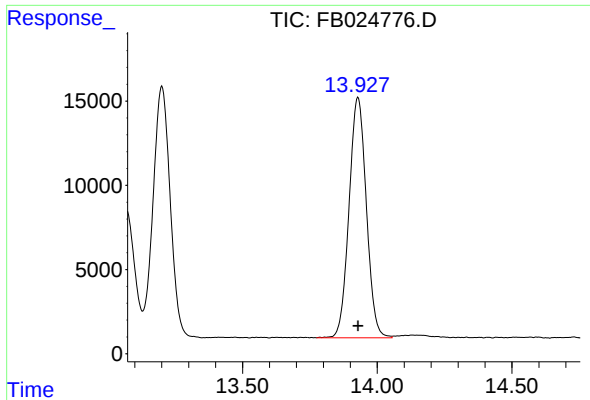

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 636727
Conc: 21.05 ng/ml

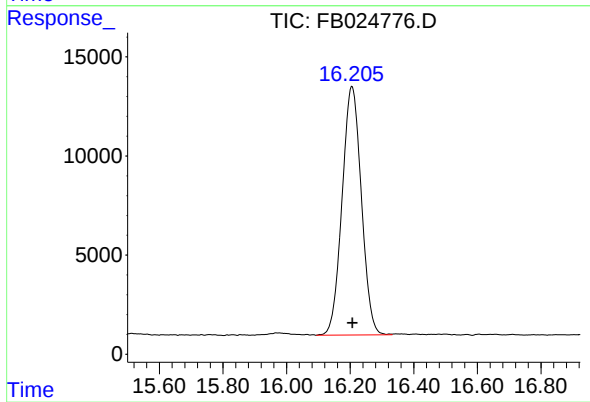

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 527655
Conc: 21.48 ng/ml