

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082123\
 Data File : FB030271.D
 Signal(s) : FID2B.CH
 Acq On : 21 Aug 2023 11:33
 Operator : YP/AJ
 Sample : 04089-01
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 22 01:08:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	146310	11.904 ng/ml
Target Compounds			
7) t Ethylbenzene	13.039	15061	0.702 ng/ml
9) t O-Xylene	13.914	15507	0.756 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	13539	0.692 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082123\
Data File : FB030271.D
Signal(s) : FID2B.CH
Acq On : 21 Aug 2023 11:33
Operator : YP/AJ
Sample : 04089-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 22 01:08:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

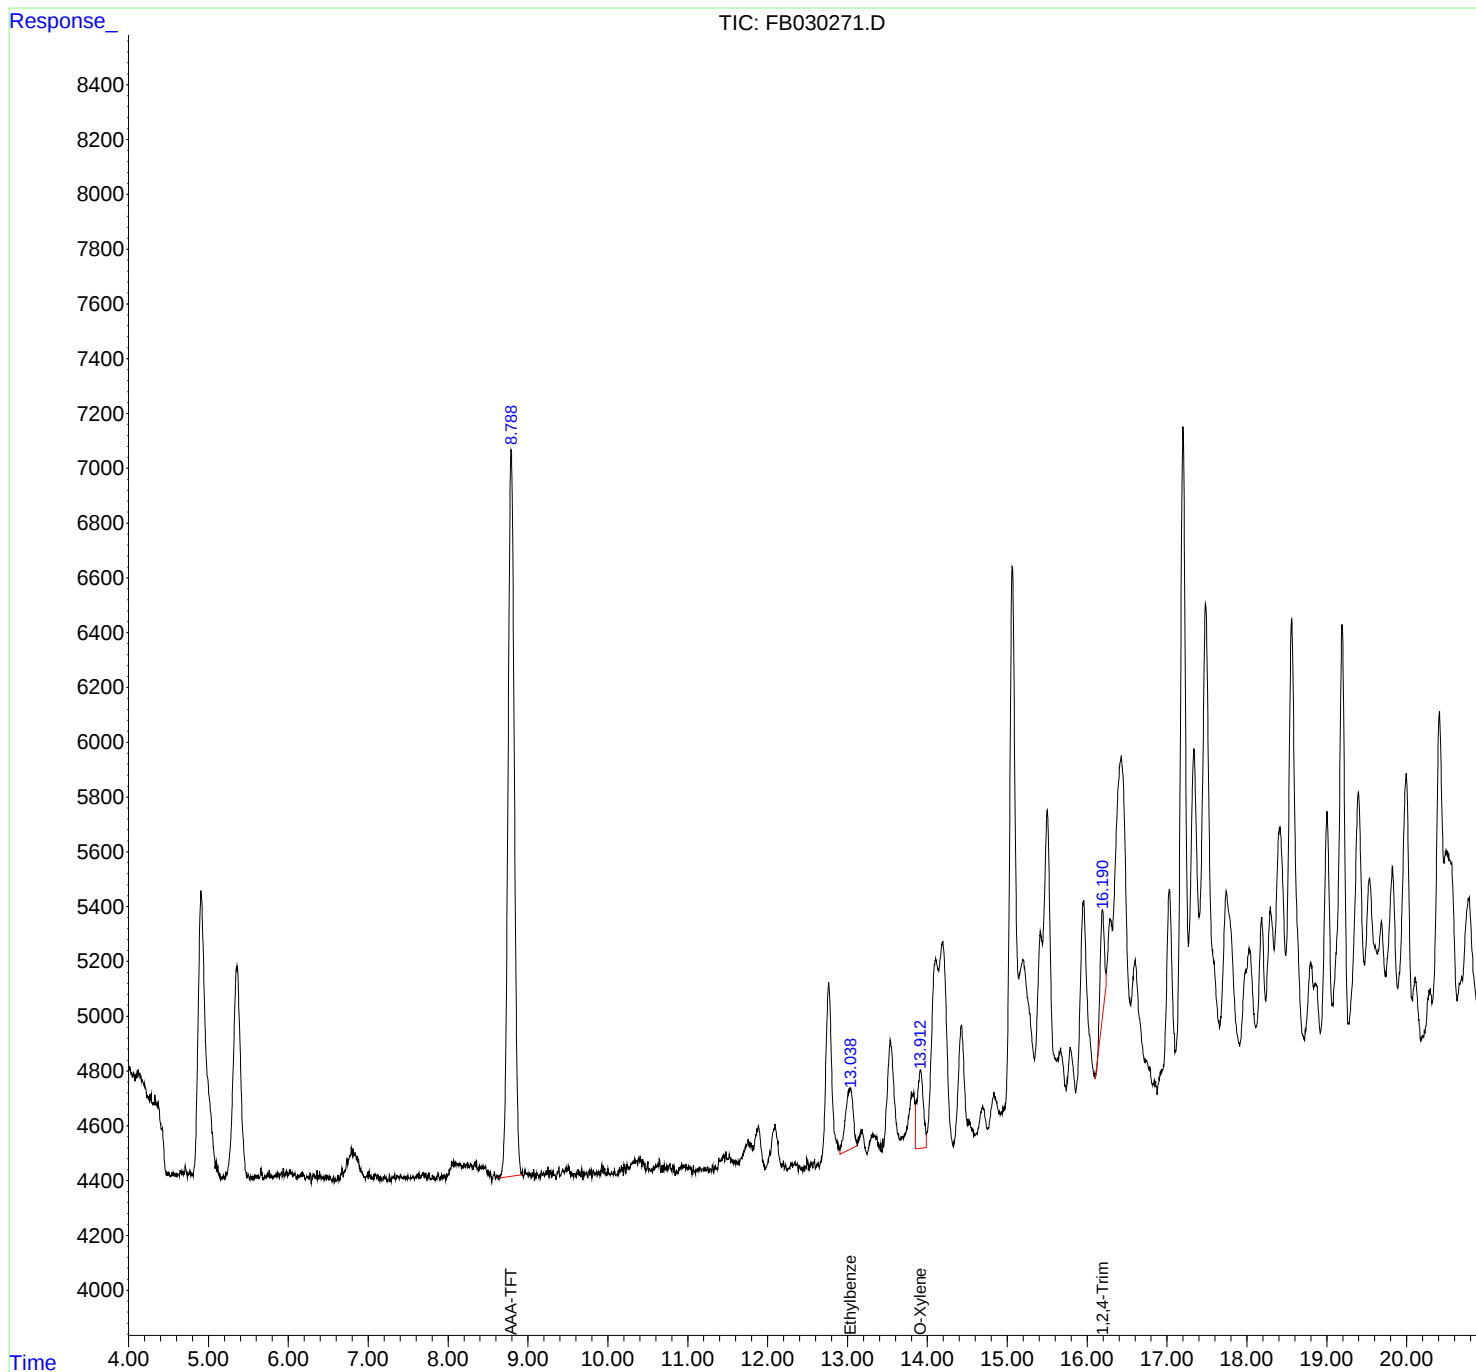


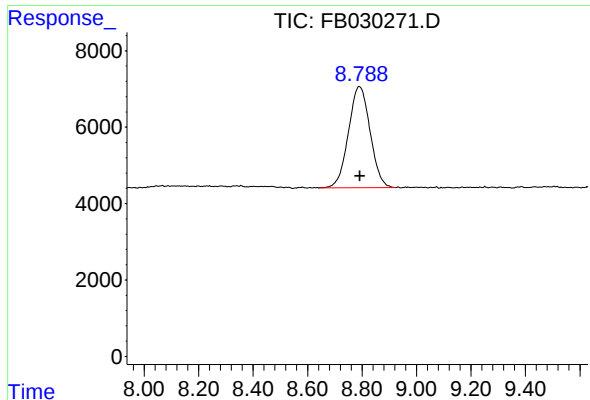

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 146310
Conc: 11.90 ng/ml

Instrument :
FID_B
ClientSampleId :

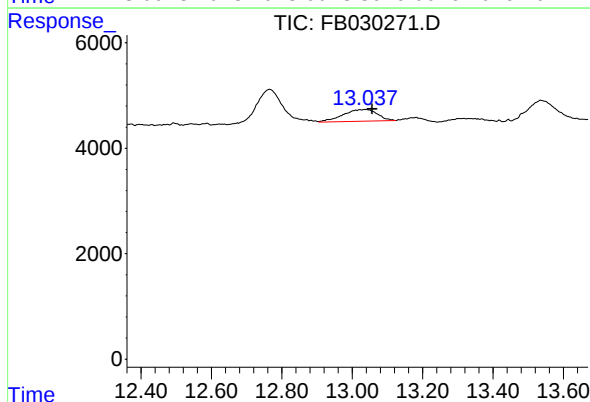


#7 Ethylbenzene

R.T.: 13.039 min
Delta R.T.: -0.018 min
Response: 15061
Conc: 0.70 ng/ml

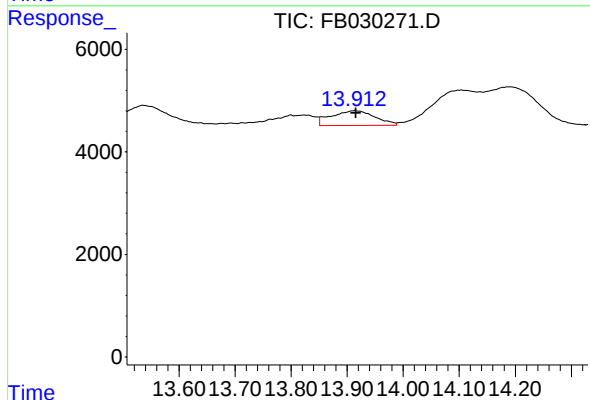

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.002 min
Response: 15507
Conc: 0.76 ng/ml

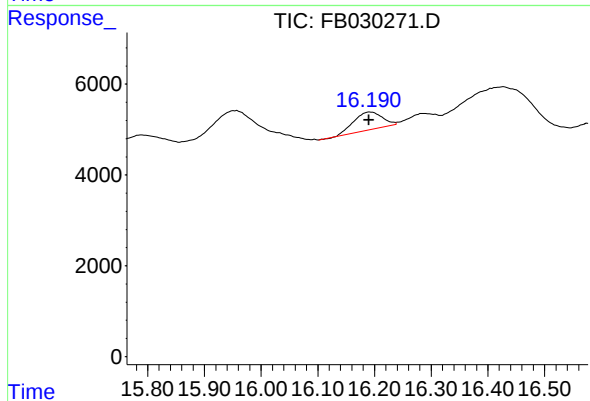

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 13539
Conc: 0.69 ng/ml