

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082123\  
Data File : FB030270.D  
Signal(s) : FID2B.CH  
Acq On : 21 Aug 2023 10:54  
Operator : YP/AJ  
Sample : 04089-01  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BU-3-081823

Integration File: Calibration.e  
Quant Time: Aug 22 01:08:24 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072423.M  
Quant Title :  
QLast Update : Tue Jul 25 06:41:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082123\  
Data File : FB030270.D  
Signal(s) : FID2B.CH  
Acq On : 21 Aug 2023 10:54  
Operator : YP/AJ  
Sample : 04089-01  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BU-3-081823

Integration File: Calibration.e  
Quant Time: Aug 22 01:08:24 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB072423.M  
Quant Title :  
QLast Update : Tue Jul 25 06:41:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

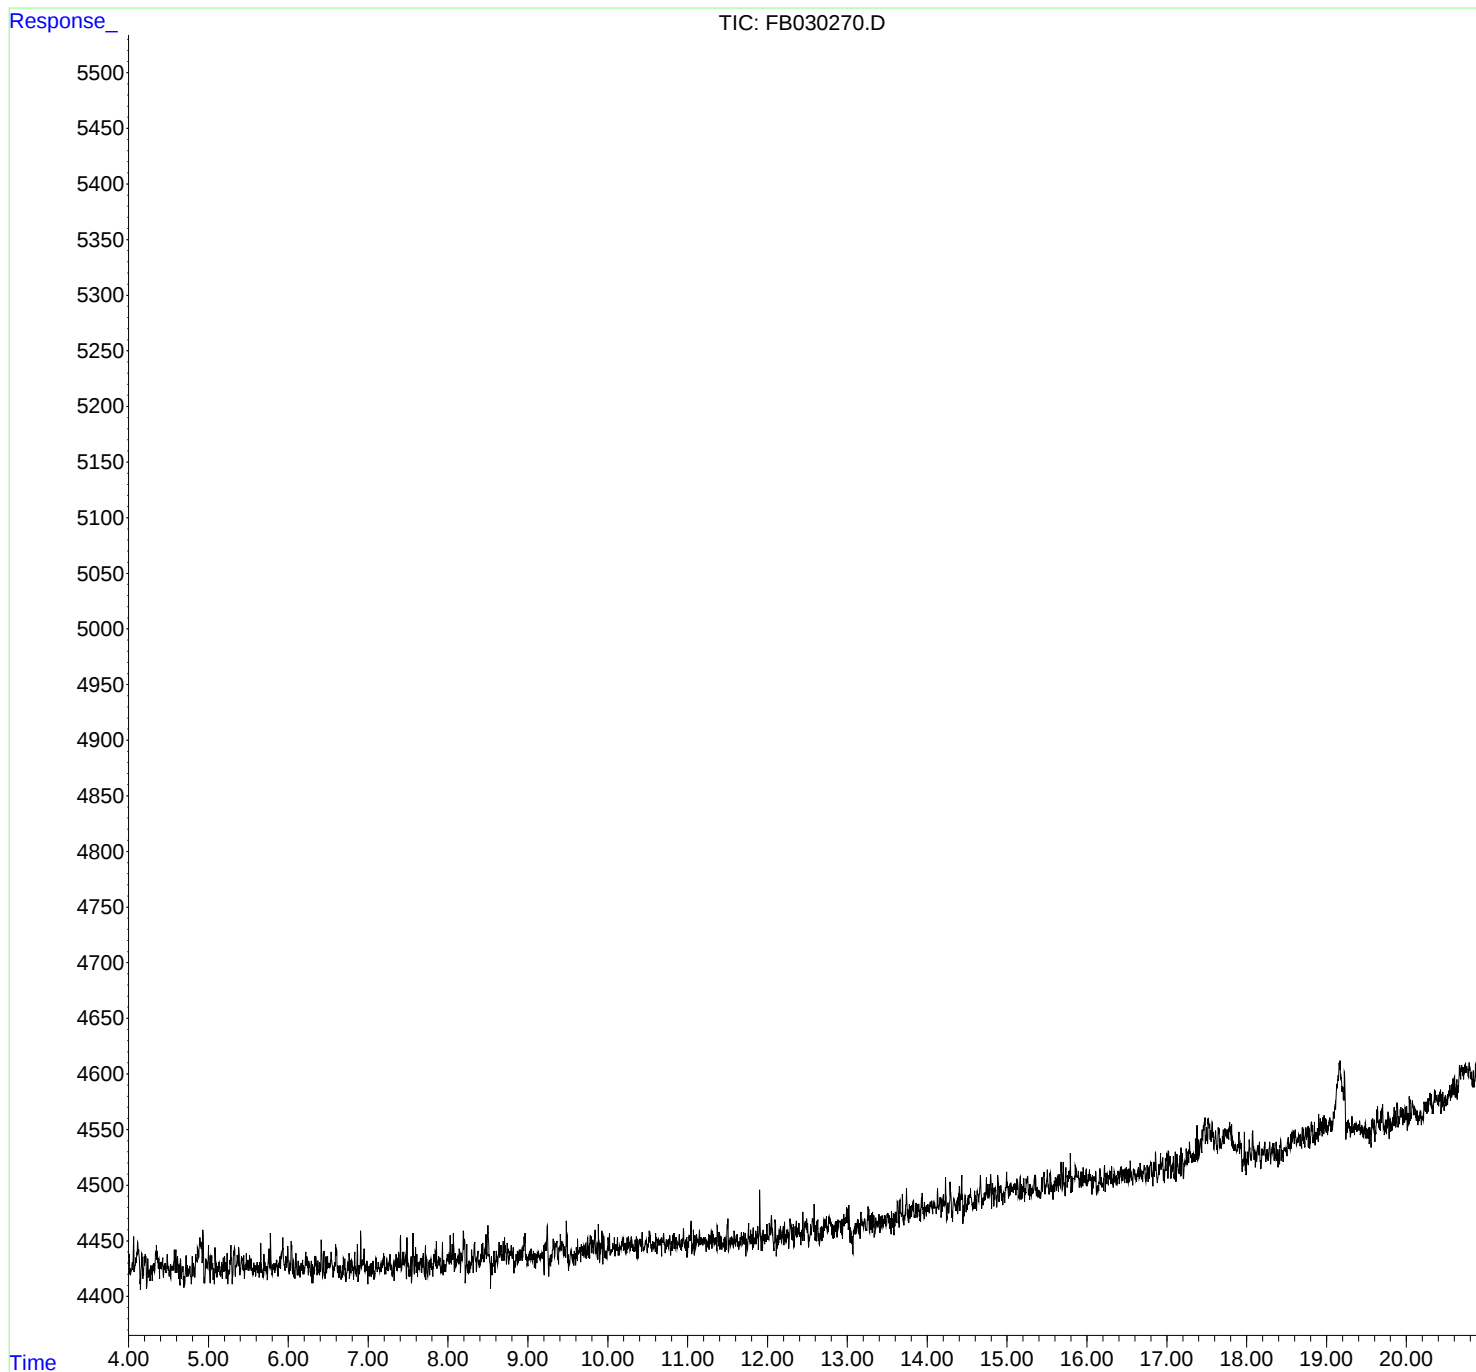

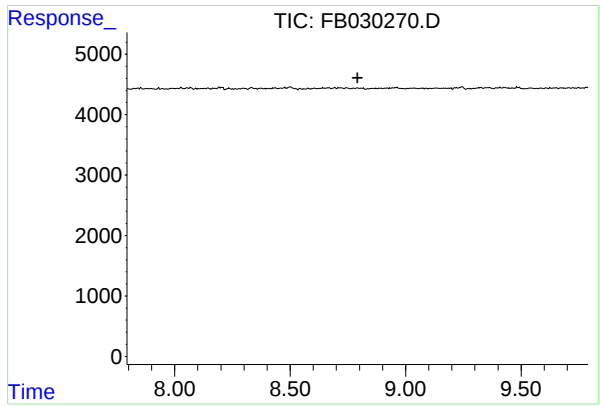

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
BU-3-081823