

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082223\
 Data File : FB030290.D
 Signal(s) : FID2B.CH
 Acq On : 22 Aug 2023 12:52
 Operator : YP/AJ
 Sample : FB082223GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB082223GROICV

Integration File: Calibration.e
 Quant Time: Aug 22 12:57:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
 Quant Title :
 QLast Update : Tue Aug 22 12:20:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	205841	17.295 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	528304	28.936 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	644749	32.677 ng/ml
3) t n-Heptane	7.748	202404	9.494 ng/ml
4) t Benzene	7.885	237795	9.573 ng/ml
6) t Toluene	10.617	681391	28.415 ng/ml
7) t Ethylbenzene	13.053	220544	9.838 ng/ml
8) t m-Xylene	13.186	444622	19.942 ng/ml
9) t O-Xylene	13.912	441137	20.683 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	456122	21.525 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082223\
Data File : FB030290.D
Signal(s) : FID2B.CH
Acq On : 22 Aug 2023 12:52
Operator : YP/AJ
Sample : FB082223GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB082223GROICV

Integration File: Calibration.e
Quant Time: Aug 22 12:57:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 12:20:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

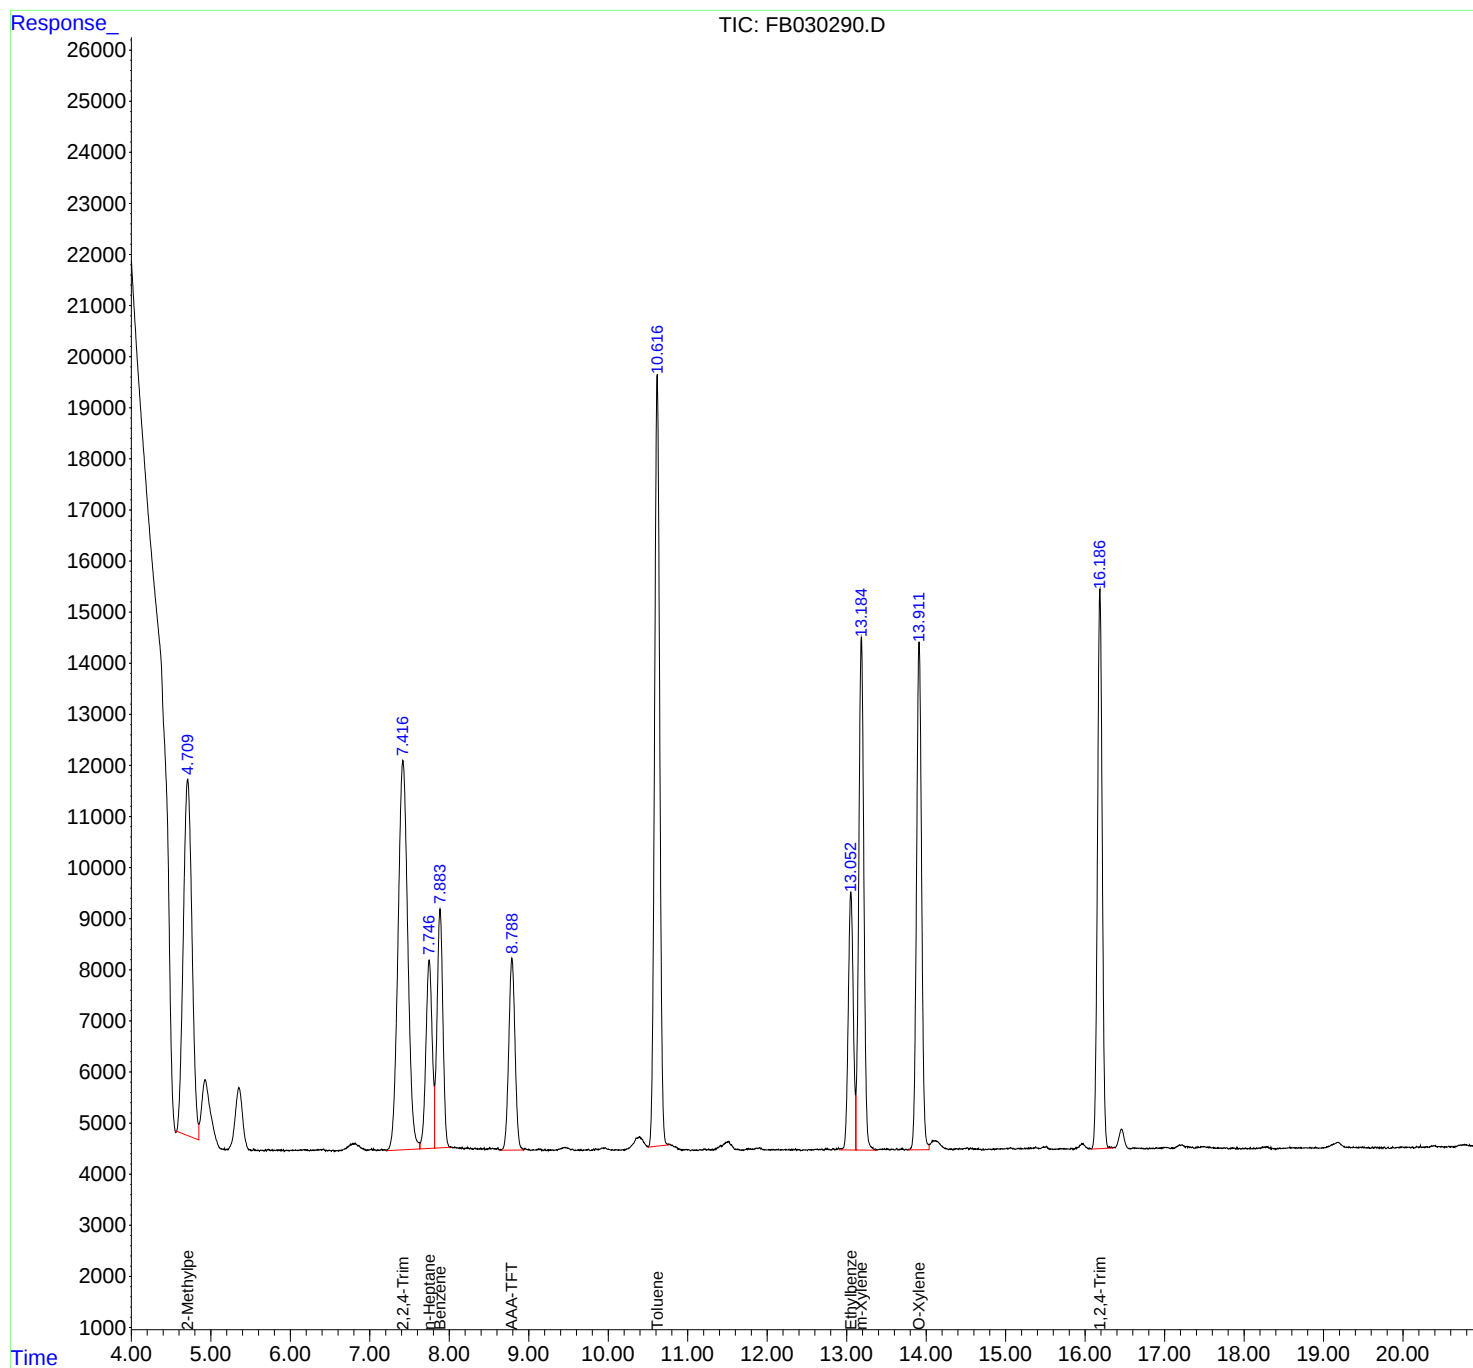


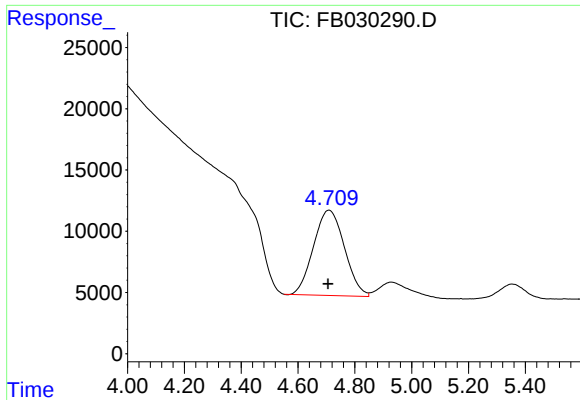

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.004 min
Response: 528304
Conc: 28.94 ng/ml

Instrument :
FID_B
ClientSampleId :
FB082223GROICV

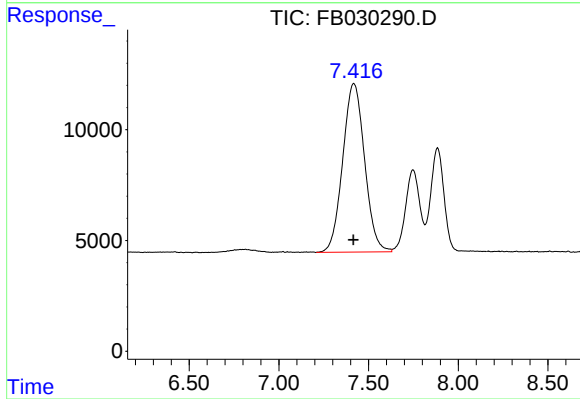


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 644749
Conc: 32.68 ng/ml

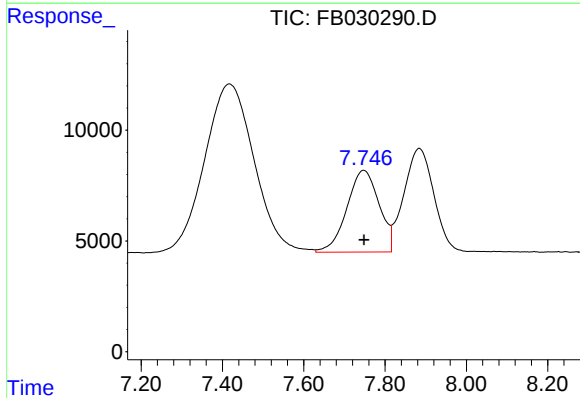


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 202404
Conc: 9.49 ng/ml

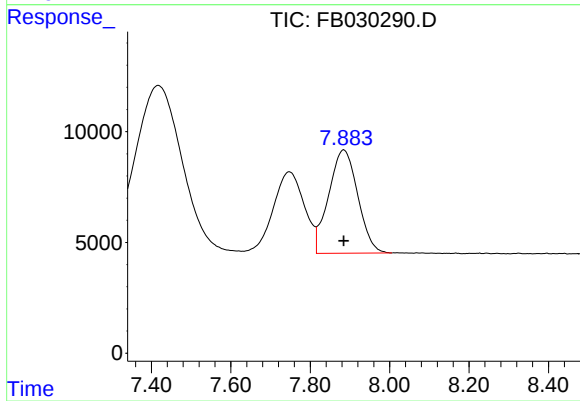

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 237795
Conc: 9.57 ng/ml

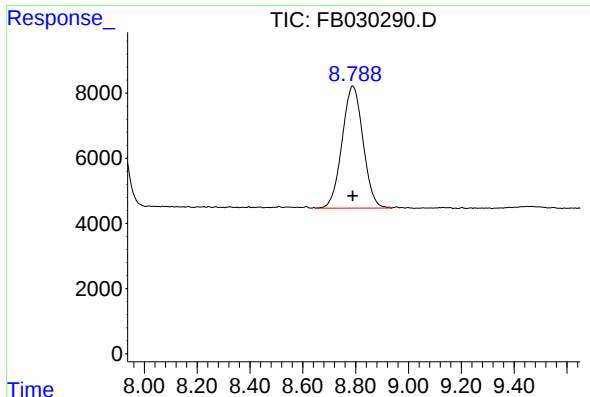

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 205841
Conc: 17.30 ng/ml

Instrument :
FID_B
ClientSampleId :
FB082223GROICV

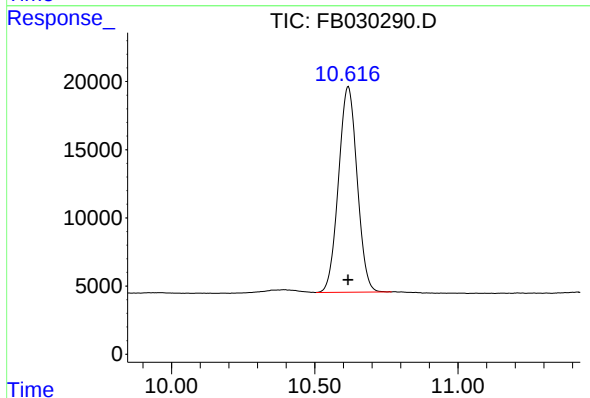


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 681391
Conc: 28.41 ng/ml

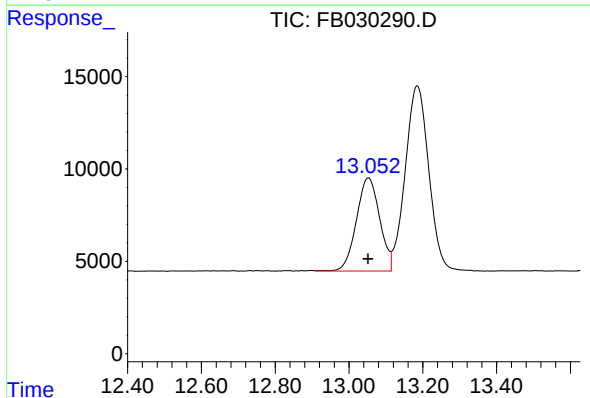


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.002 min
Response: 220544
Conc: 9.84 ng/ml

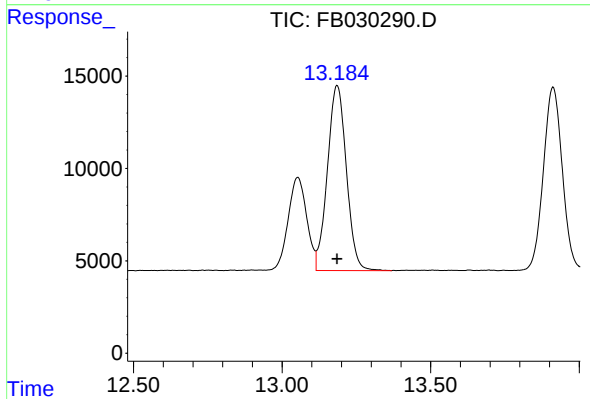

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.001 min
Response: 444622
Conc: 19.94 ng/ml

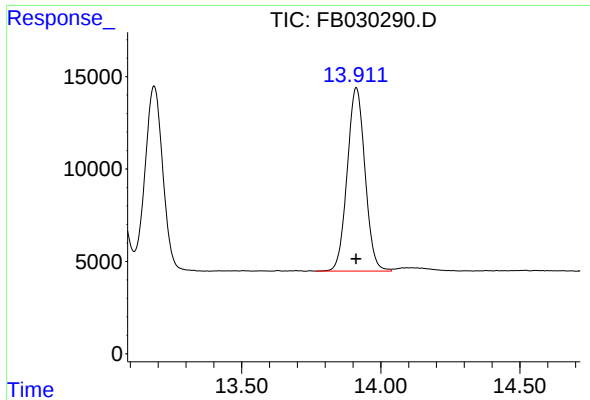

#9 O-Xylene


R.T.: 13.912 min
Delta R.T.: 0.001 min
Response: 441137
Conc: 20.68 ng/ml

Instrument :

FID_B

ClientSampleId :

FB082223GROICV

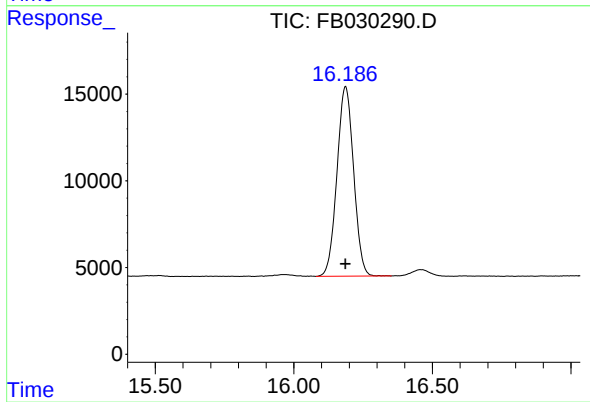

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 456122
Conc: 21.53 ng/ml