

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082318\
Data File : FB017519.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2018 12:45
Operator : MJ/SJ
Sample : J4612-05MSD
Misc : 5.03g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 23 13:44:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.112	166855	20.238 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.964	387674	27.667 ng/ml
2) t	2,2,4-Trimethylpentane	7.728	333219	23.646 ng/ml
3) t	n-Heptane	8.069	97532	7.077 ng/ml
4) t	Benzene	8.207	177059	10.043 ng/ml
6) t	Toluene	10.961	414968	28.846 ng/ml
7) t	Ethylbenzene	13.411	135392	9.181 ng/ml
8) t	m-Xylene	13.543	287709	18.508 ng/ml
9) t	O-Xylene	14.275	306111	18.648 ng/ml
10) t	1,2,4-Trimethylbenzene	16.558	338658	17.388 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082318\
Data File : FB017519.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2018 12:45
Operator : MJ/SJ
Sample : J4612-05MSD
Misc : 5.03g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 23 13:44:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

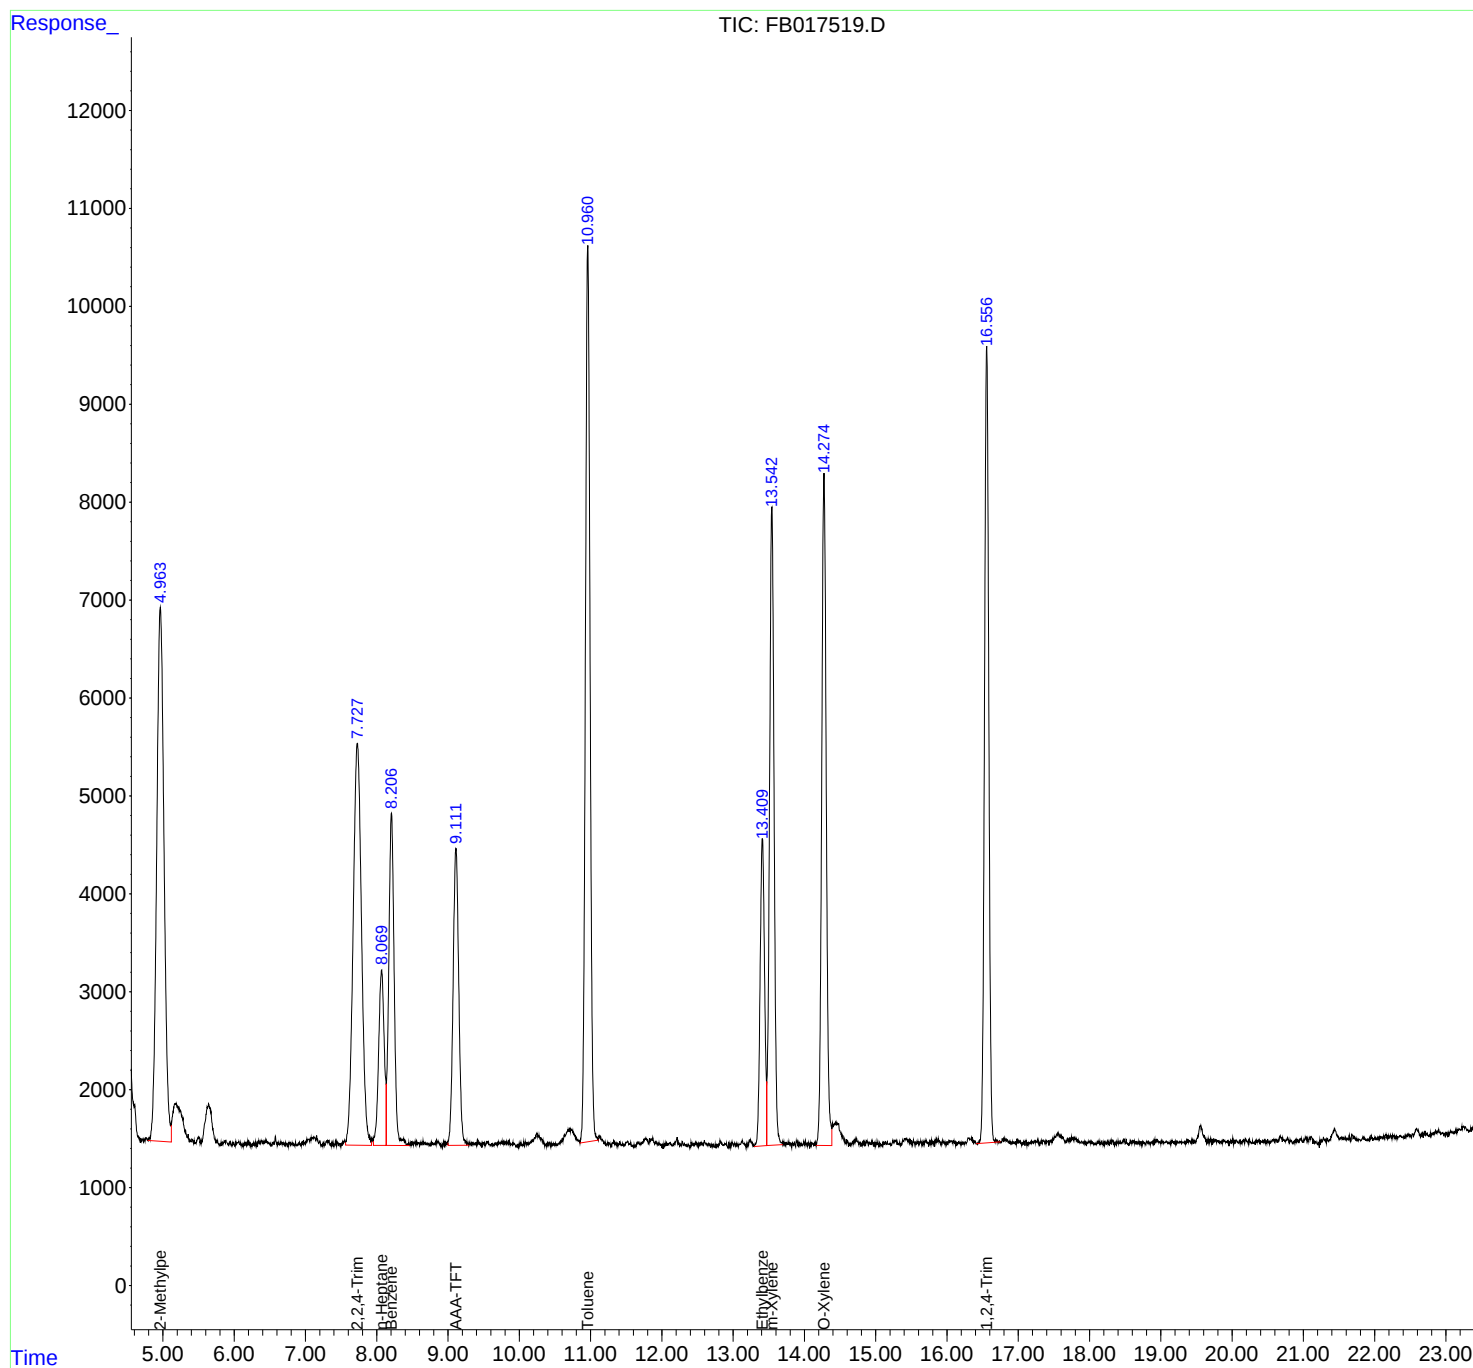

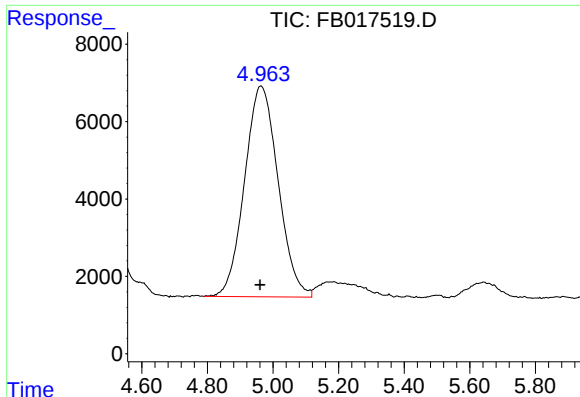


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: 0.003 min
Response: 387674
Conc: 27.67 ng/ml

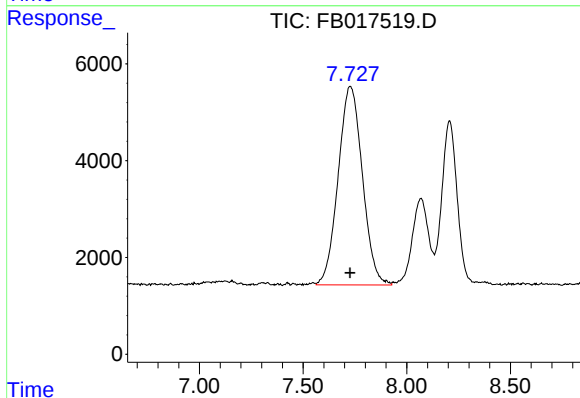


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 333219
Conc: 23.65 ng/ml

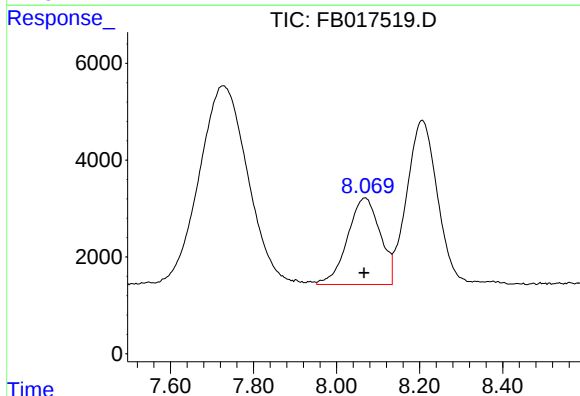


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.003 min
Response: 97532
Conc: 7.08 ng/ml

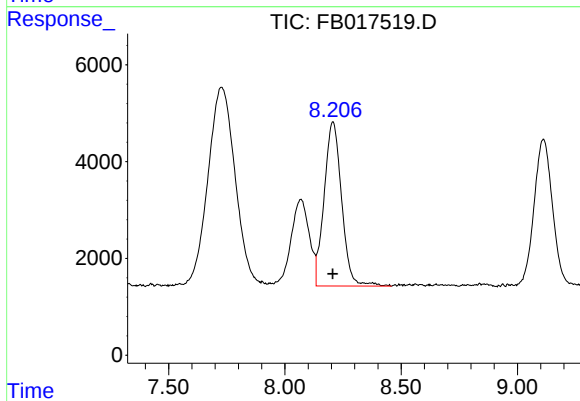


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.001 min
Response: 177059
Conc: 10.04 ng/ml

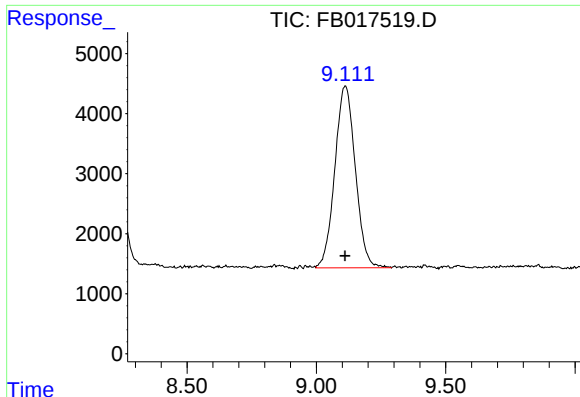


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.001 min
Response: 166855
Conc: 20.24 ng/ml

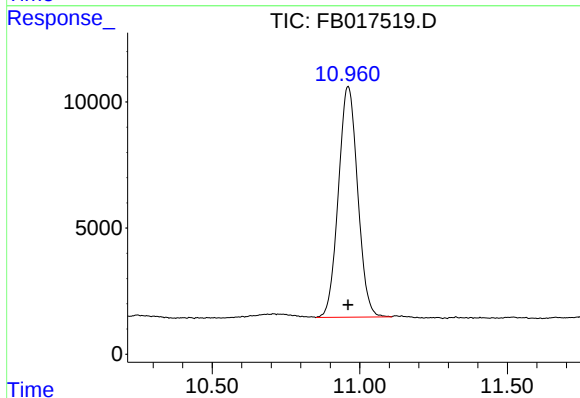


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 414968
Conc: 28.85 ng/ml

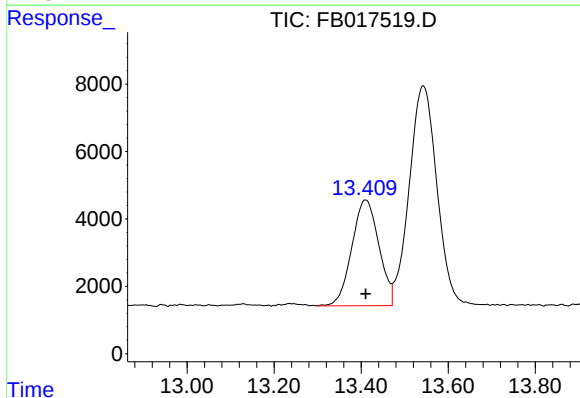


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 135392
Conc: 9.18 ng/ml

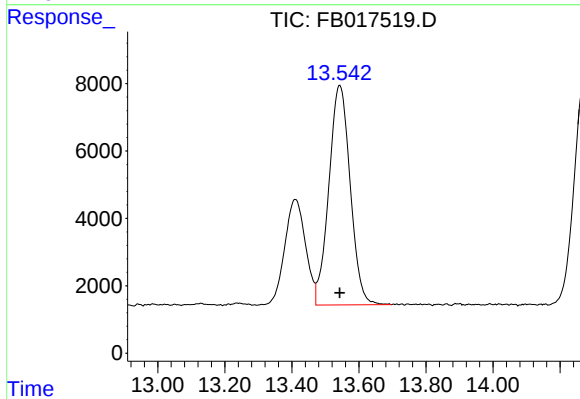


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: 0.000 min
Response: 287709
Conc: 18.51 ng/ml

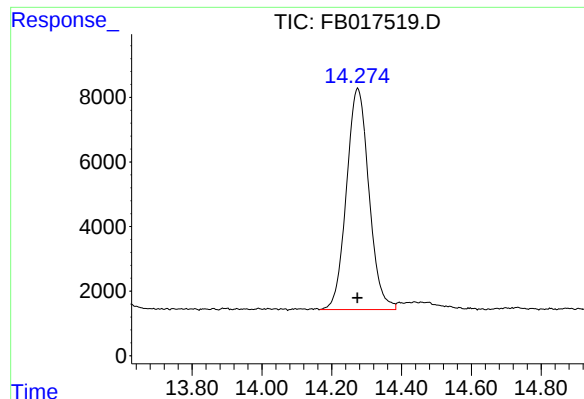

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.001 min
Response: 306111
Conc: 18.65 ng/ml

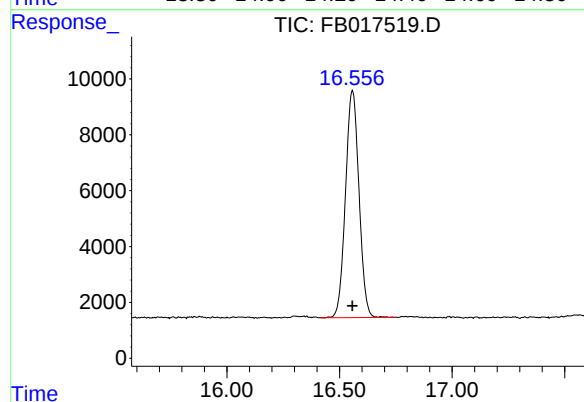

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 338658
Conc: 17.39 ng/ml