

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082318\
 Data File : FB017516.D
 Signal(s) : FID2B.CH
 Acq On : 23 Aug 2018 9:26
 Operator : MJ/SJ
 Sample : BSF0823S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 23 13:44:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	171845	20.843 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.966	458375	32.712 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	458472	32.534 ng/ml
3) t n-Heptane	8.068	141563	10.272 ng/ml
4) t Benzene	8.206	187225	10.619 ng/ml
6) t Toluene	10.961	464037	32.256 ng/ml
7) t Ethylbenzene	13.411	152195	10.320 ng/ml
8) t m-Xylene	13.544	322702	20.759 ng/ml
9) t O-Xylene	14.276	347460	21.167 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	407962	20.946 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082318\
Data File : FB017516.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2018 9:26
Operator : MJ/SJ
Sample : BSF0823S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 23 13:44:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

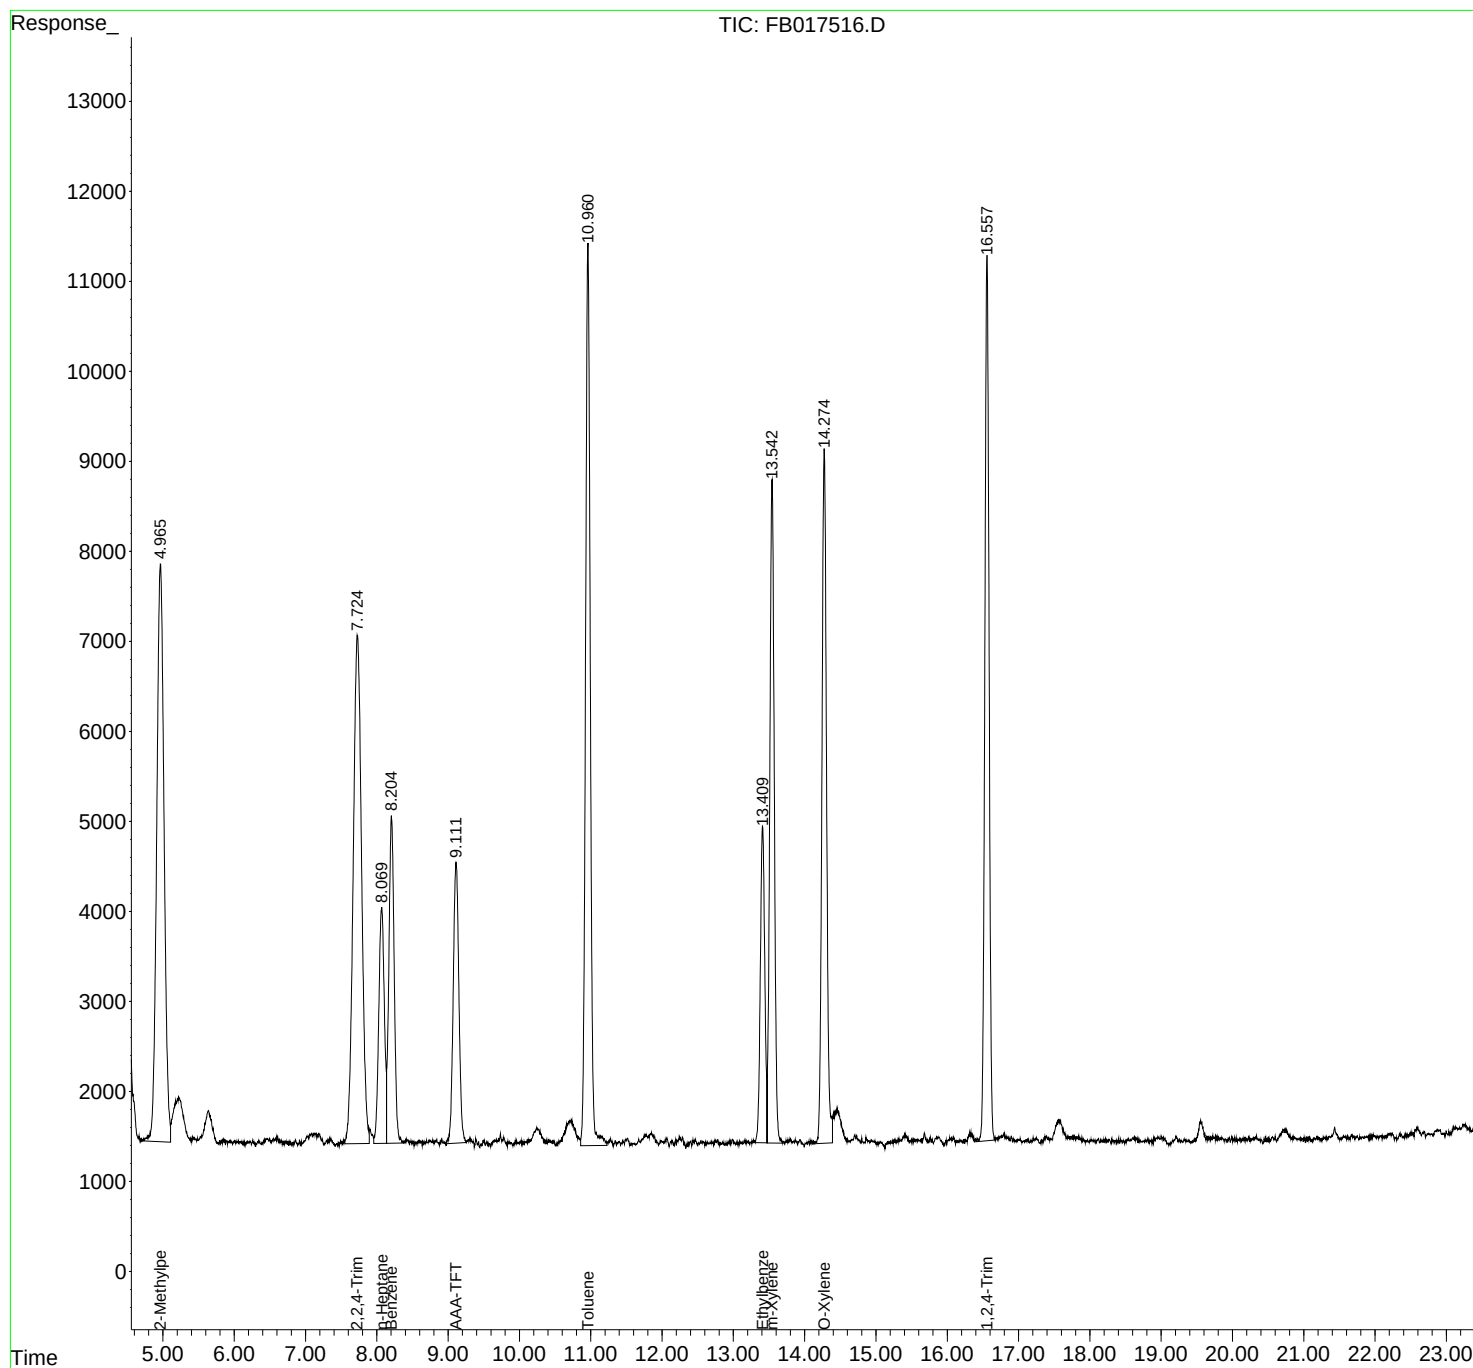

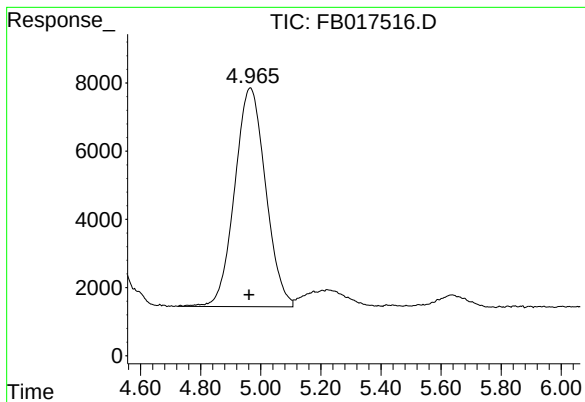


#1 2-Methylpentane

R.T.: 4.966 min
Delta R.T.: 0.005 min
Response: 458375
Conc: 32.71 ng/ml

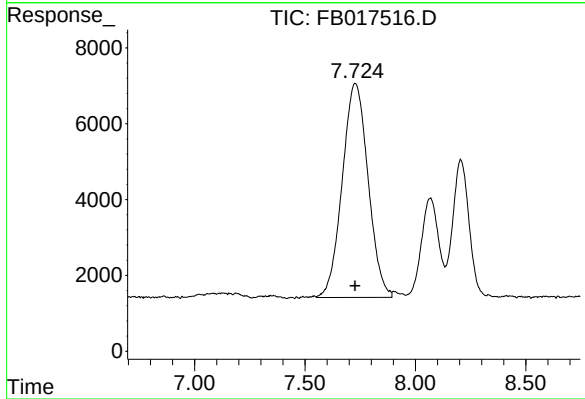


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 458472
Conc: 32.53 ng/ml

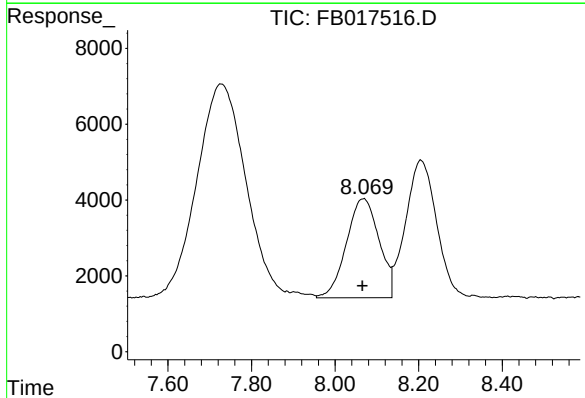


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.002 min
Response: 141563
Conc: 10.27 ng/ml

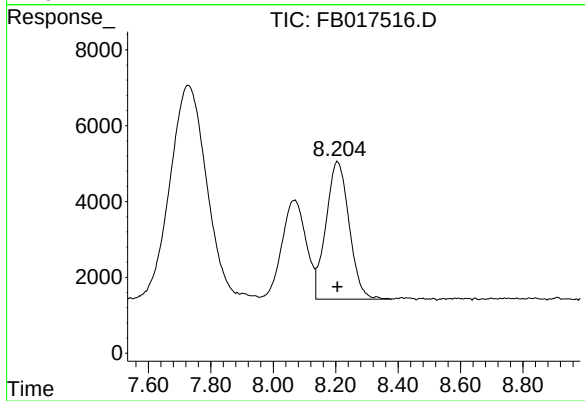


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 187225
Conc: 10.62 ng/ml

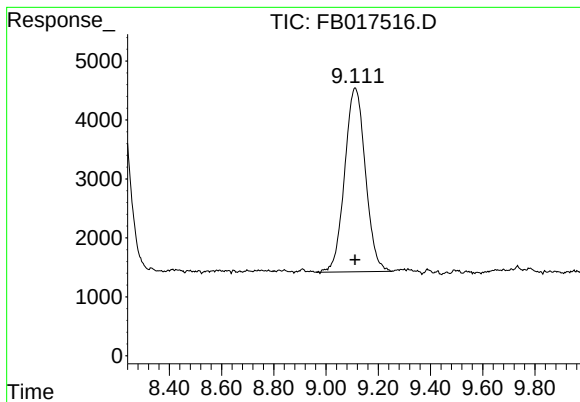


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.001 min
Response: 171845
Conc: 20.84 ng/ml

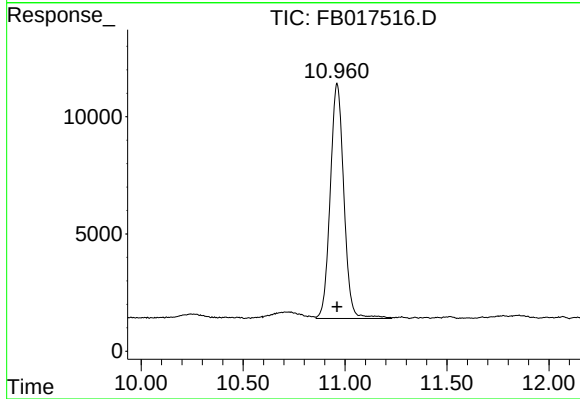


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 464037
Conc: 32.26 ng/ml

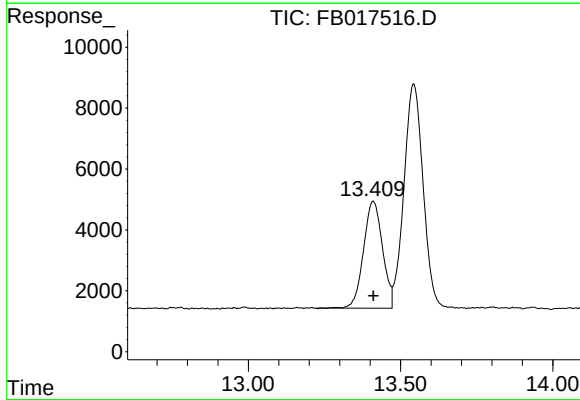


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 152195
Conc: 10.32 ng/ml

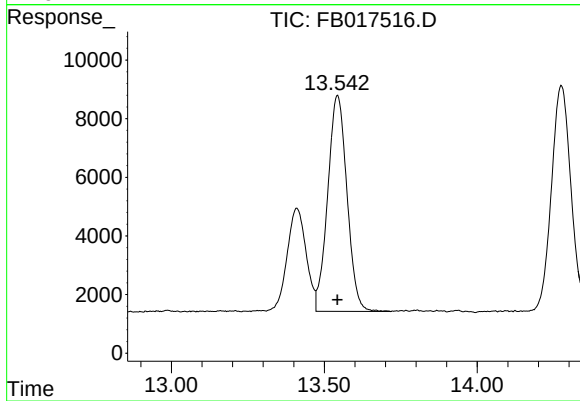


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 322702
Conc: 20.76 ng/ml

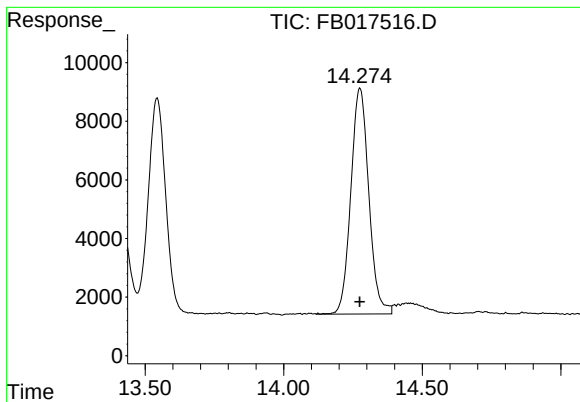

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.001 min
Response: 347460
Conc: 21.17 ng/ml

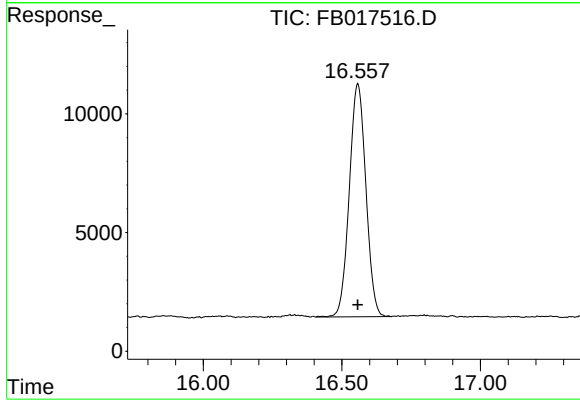

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.000 min
Response: 407962
Conc: 20.95 ng/ml