

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082319\
 Data File : FB022113.D
 Signal(s) : FID2B.CH
 Acq On : 23 Aug 2019 10:04
 Operator : DD/AJ
 Sample : BSF0823S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 24 09:41:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.981	393922	18.546 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.853	1197022	29.909 ng/ml
2) t	2,2,4-Trimethylpentane	7.601	1148072	28.504 ng/ml
3) t	n-Heptane	7.940	364462	9.541 ng/ml
4) t	Benzene	8.076	439469	9.789 ng/ml
6) t	Toluene	10.822	881225	28.665 ng/ml
7) t	Ethylbenzene	13.268	217235	10.645 ng/ml
8) t	m-Xylene	13.401	458090	21.751 ng/ml
9) t	O-Xylene	14.130	486459	21.751 ng/ml
10) t	1,2,4-Trimethylbenzene	16.410	521428	20.332 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082319\
Data File : FB022113.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2019 10:04
Operator : DD/AJ
Sample : BSF0823S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 24 09:41:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

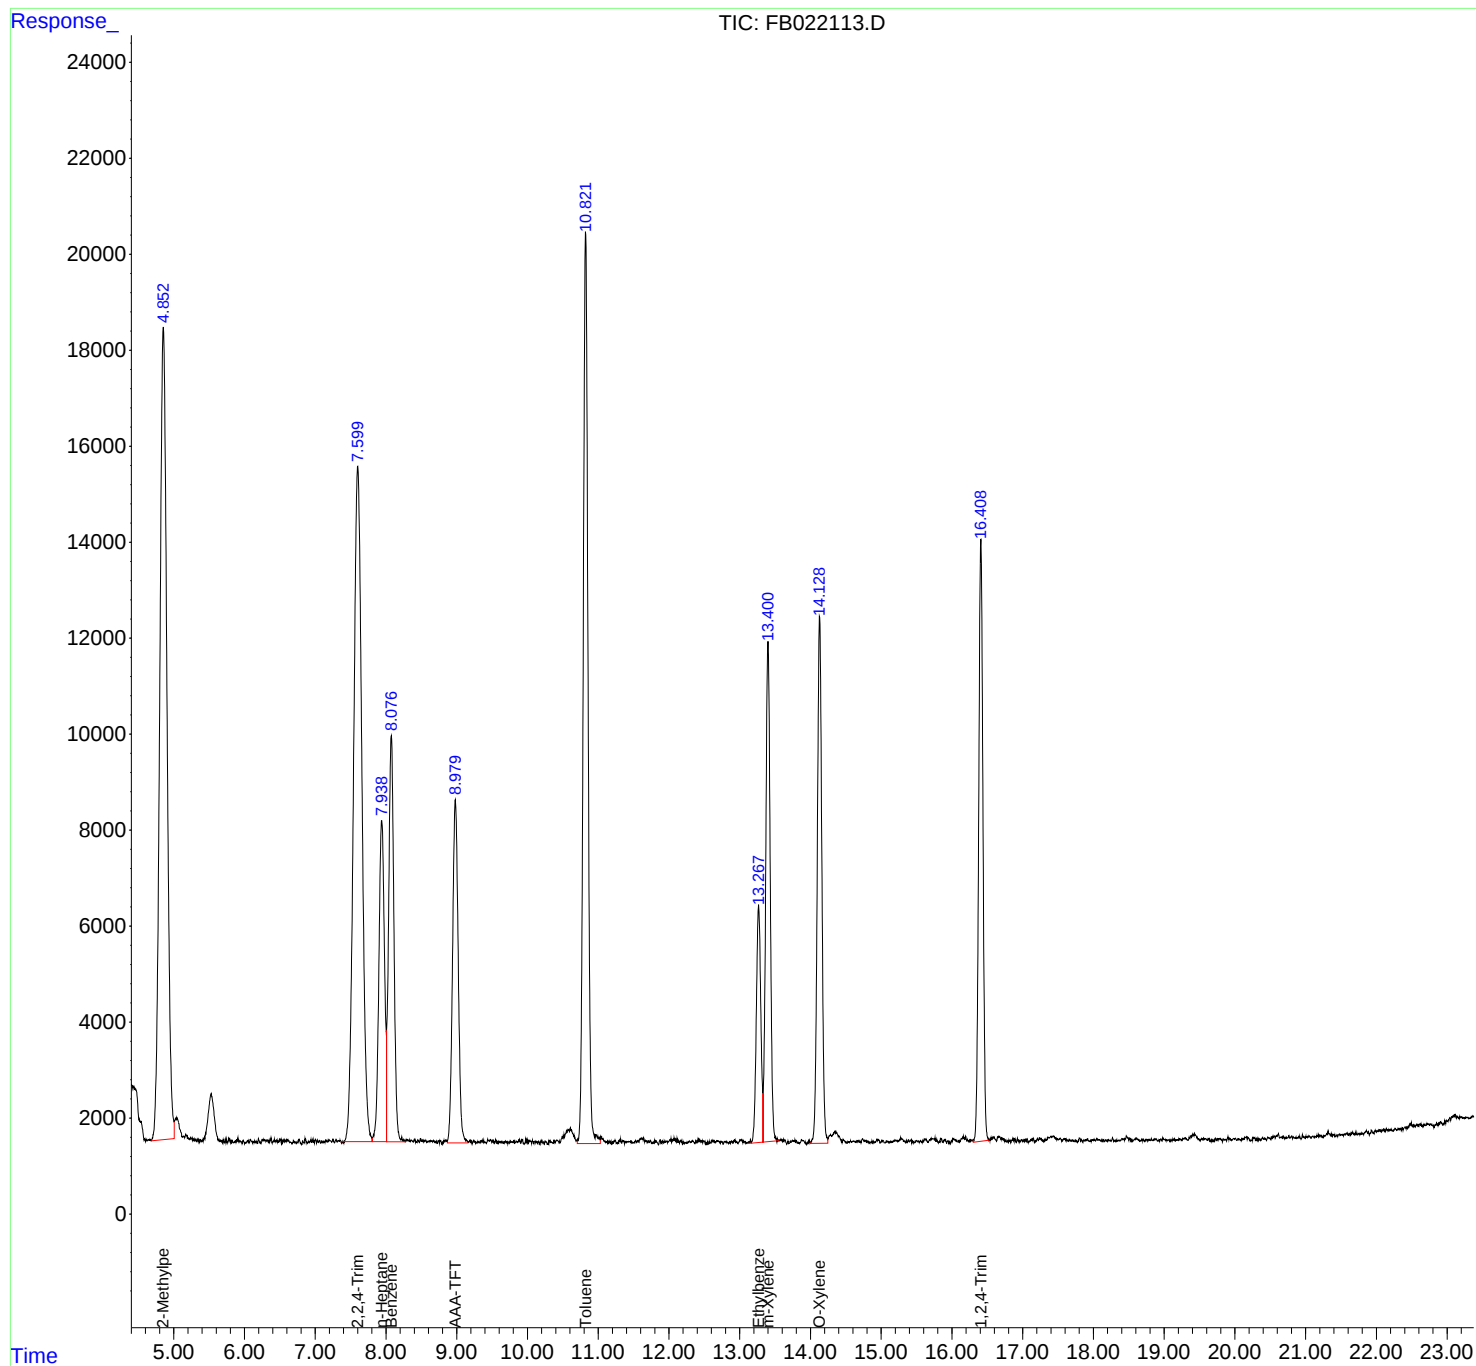

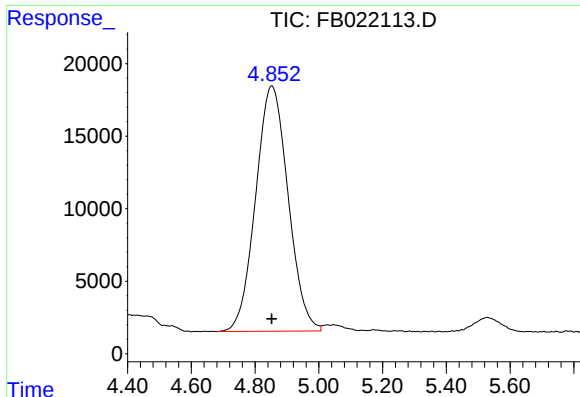


#1 2-Methylpentane

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 1197022
Conc: 29.91 ng/ml

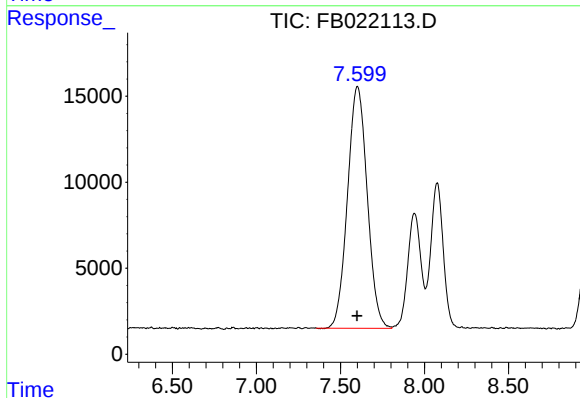


#2 2,2,4-Trimethylpentane

R.T.: 7.601 min
Delta R.T.: 0.001 min
Response: 1148072
Conc: 28.50 ng/ml

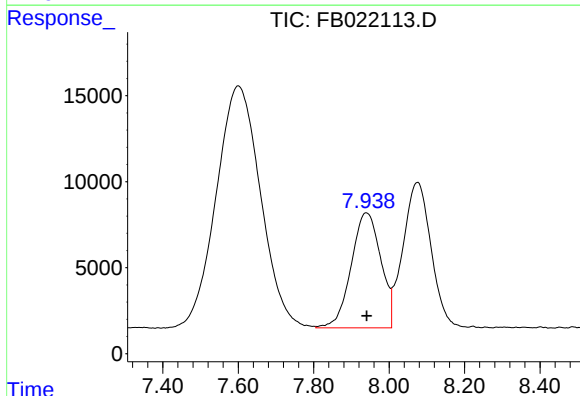


#3 n-Heptane

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 364462
Conc: 9.54 ng/ml

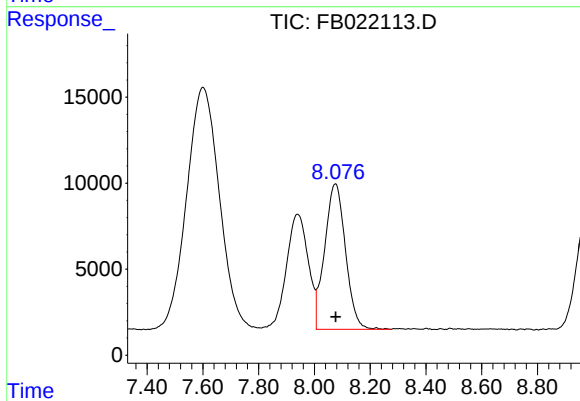


#4 Benzene

R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 439469
Conc: 9.79 ng/ml

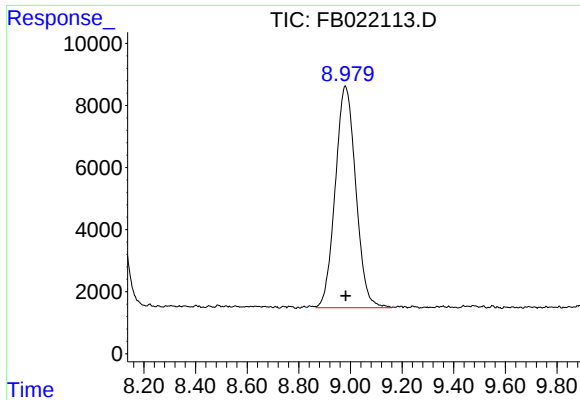


#5 AAA-TFT

R.T.: 8.981 min
Delta R.T.: -0.001 min
Response: 393922
Conc: 18.55 ng/ml

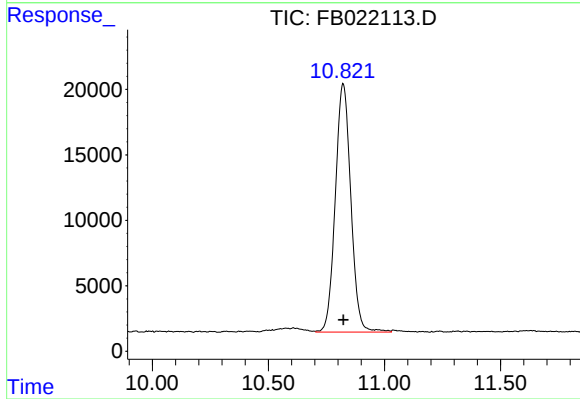


#6 Toluene

R.T.: 10.822 min
Delta R.T.: 0.000 min
Response: 881225
Conc: 28.67 ng/ml

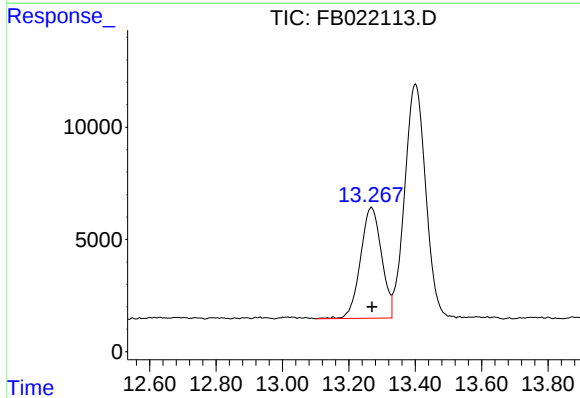


#7 Ethylbenzene

R.T.: 13.268 min
Delta R.T.: -0.002 min
Response: 217235
Conc: 10.65 ng/ml

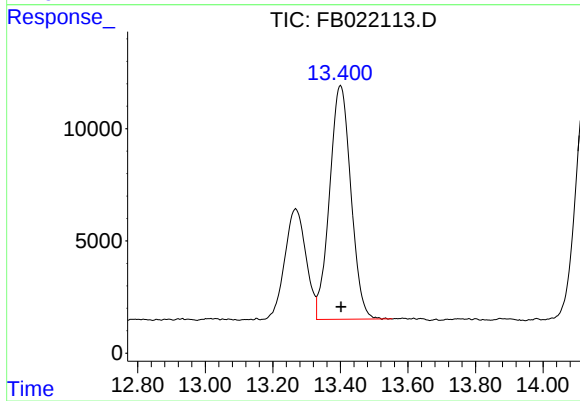


#8 m-Xylene

R.T.: 13.401 min
Delta R.T.: 0.000 min
Response: 458090
Conc: 21.75 ng/ml

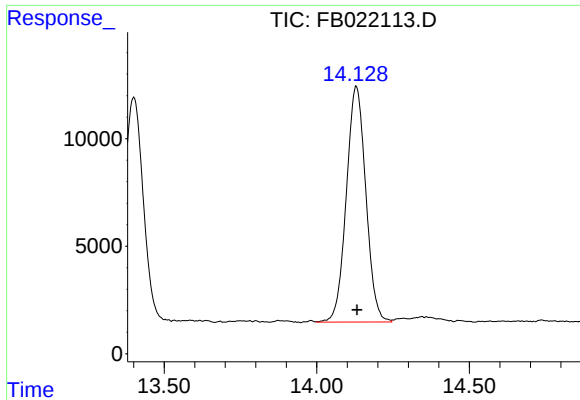

#9 O-Xylene

R.T.: 14.130 min
Delta R.T.: -0.002 min
Response: 486459
Conc: 21.75 ng/ml

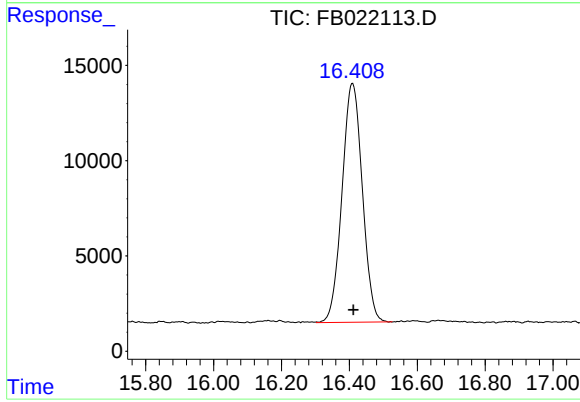

#10 1,2,4-Trimethylbenzene

R.T.: 16.410 min
Delta R.T.: -0.002 min
Response: 521428
Conc: 20.33 ng/ml