

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082322\
Data File : FB028028.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2022 16:04
Operator : AJ/MA
Sample : N4277-01 50X
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 23 18:49:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	206269	17.798 ng/ml
Target Compounds			
4) t Benzene	7.946	9371	0.403 ng/ml
8) t m-Xylene	13.194	6130	0.300 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	6665	0.342 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082322\
Data File : FB028028.D
Signal(s) : FID2B.CH
Acq On : 23 Aug 2022 16:04
Operator : AJ/MA
Sample : N4277-01 50X
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 23 18:49:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

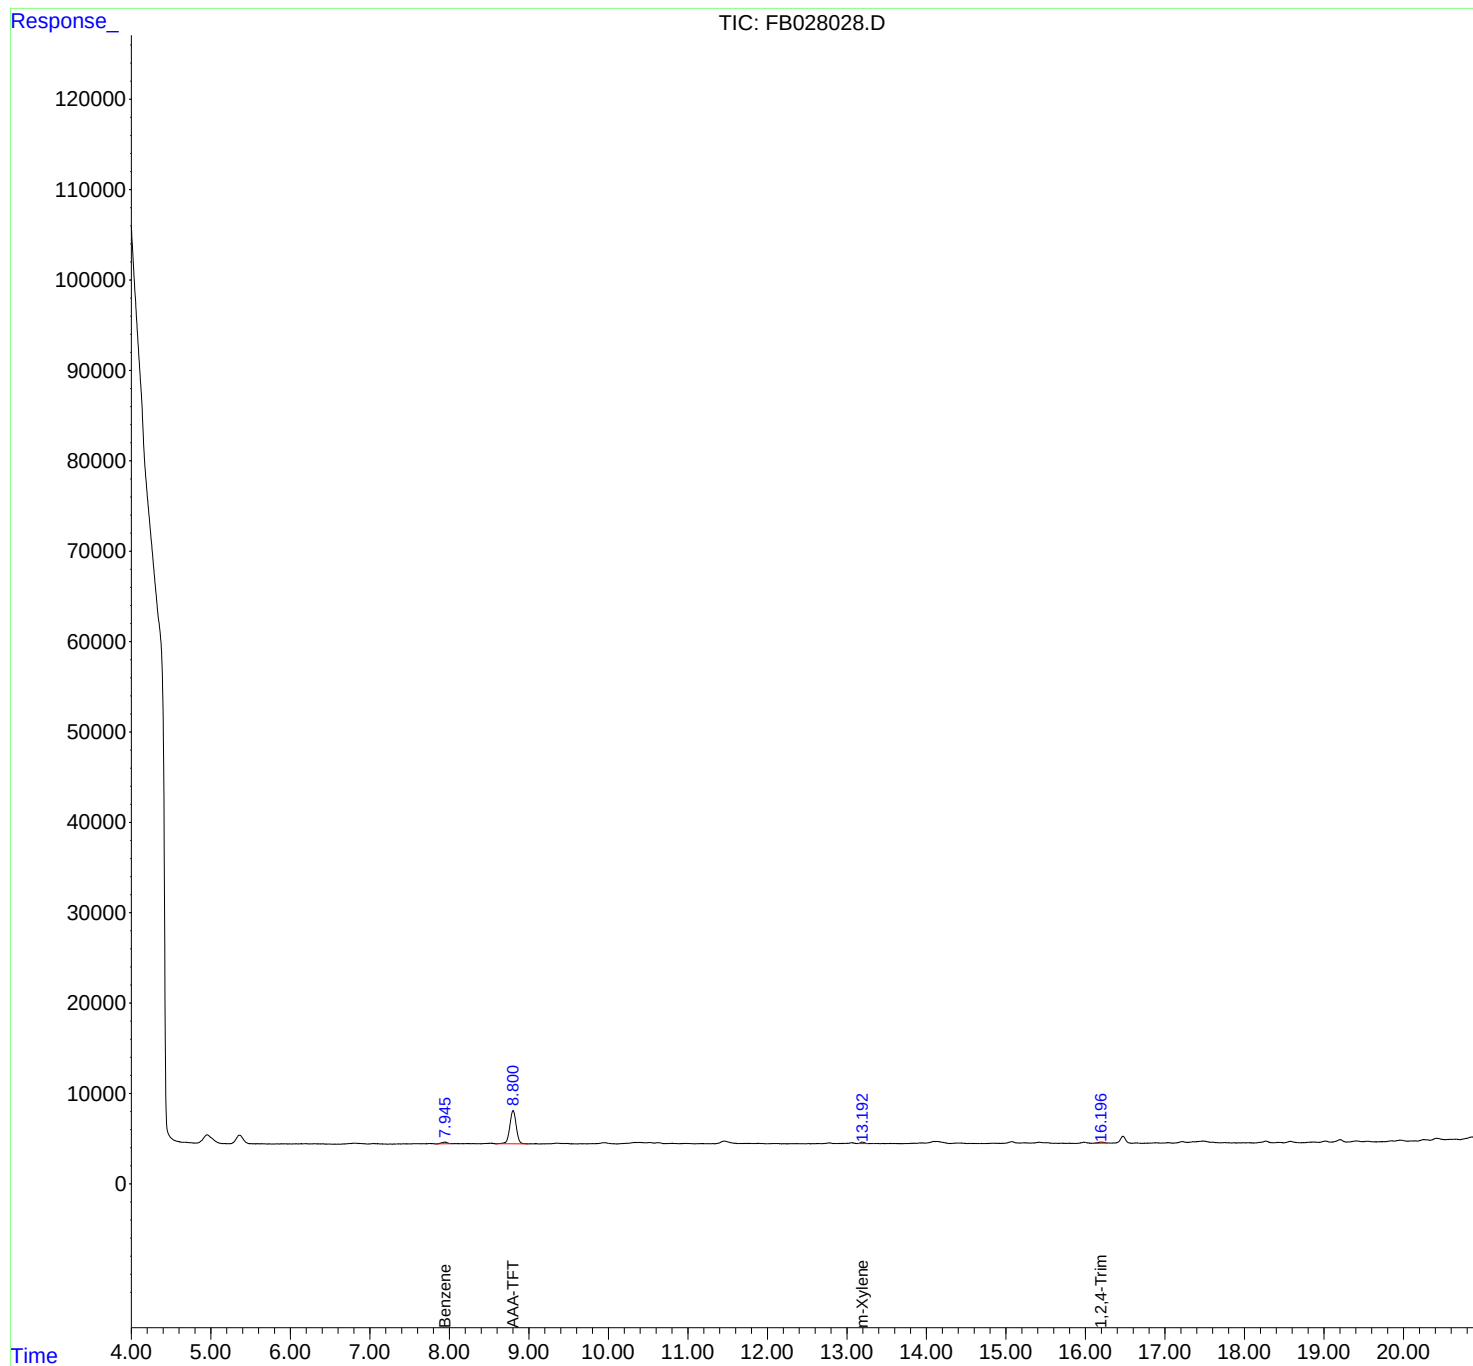


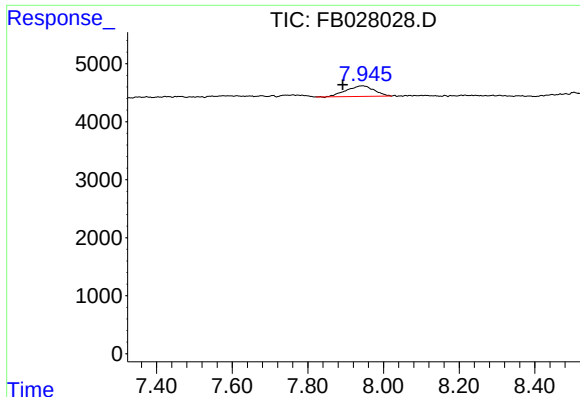

#4 Benzene


R.T.: 7.946 min
Delta R.T.: 0.054 min
Response: 9371
Conc: 0.40 ng/ml

Instrument :
FID_B
ClientSampleId :

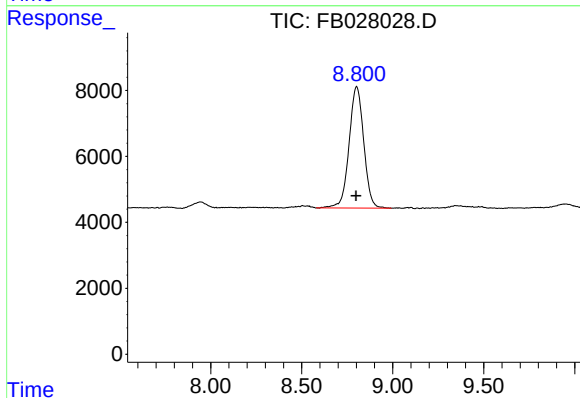


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.004 min
Response: 206269
Conc: 17.80 ng/ml

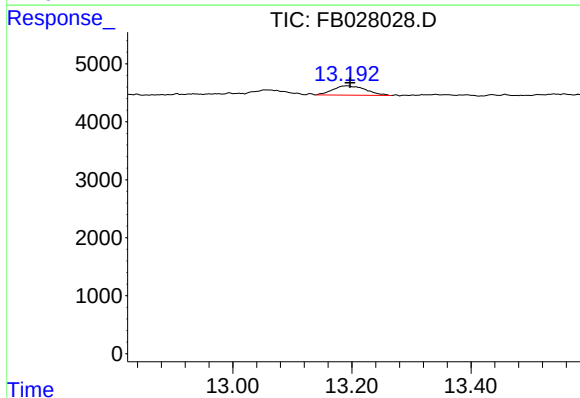

#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: -0.004 min
Response: 6130
Conc: 0.30 ng/ml

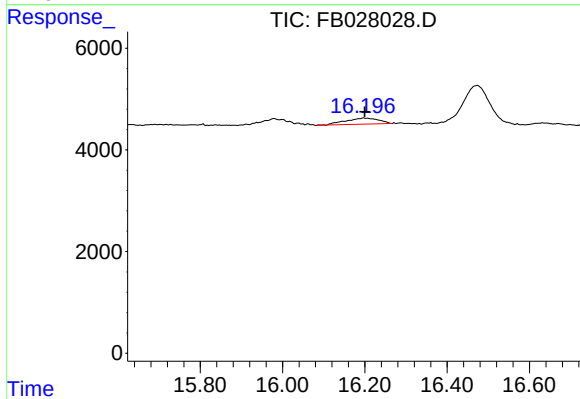

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.002 min
Response: 6665
Conc: 0.34 ng/ml