

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
 Data File : FB017534.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2018 10:45
 Operator : MJ/SJ
 Sample : J4282-11MS
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 24 11:07:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	166783	20.229 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	341879	24.399 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	327302	23.226 ng/ml
3) t n-Heptane	8.064	99113	7.192 ng/ml
4) t Benzene	8.202	165002	9.359 ng/ml
6) t Toluene	10.958	404418	28.112 ng/ml
7) t Ethylbenzene	13.408	133960	9.084 ng/ml
8) t m-Xylene	13.540	278627	17.924 ng/ml
9) t O-Xylene	14.272	302194	18.409 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	329978	16.942 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
Data File : FB017534.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2018 10:45
Operator : MJ/SJ
Sample : J4282-11MS
Misc : 5.01g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 24 11:07:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

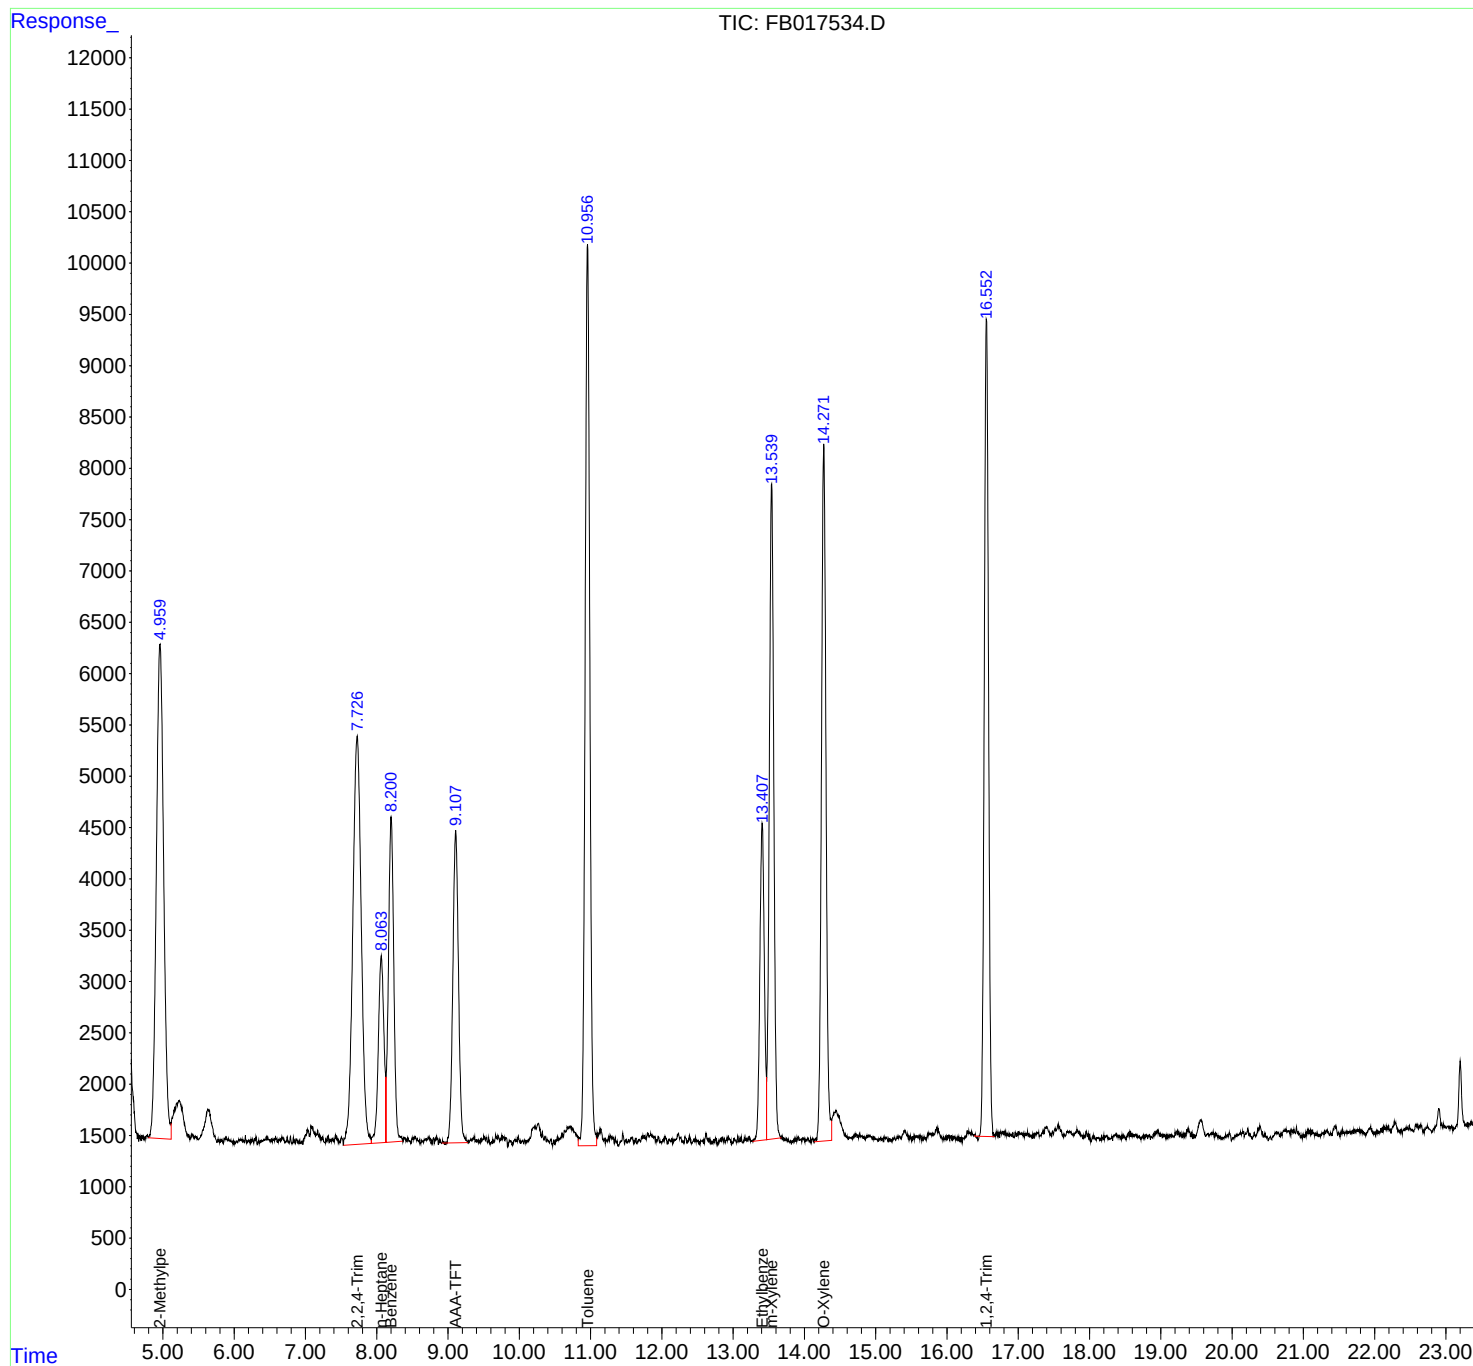

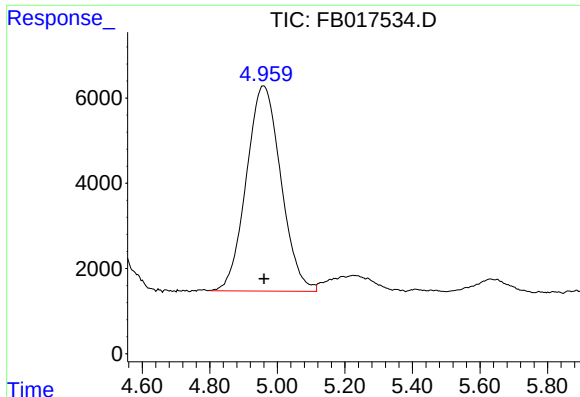


#1 2-Methylpentane

R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 341879
Conc: 24.40 ng/ml

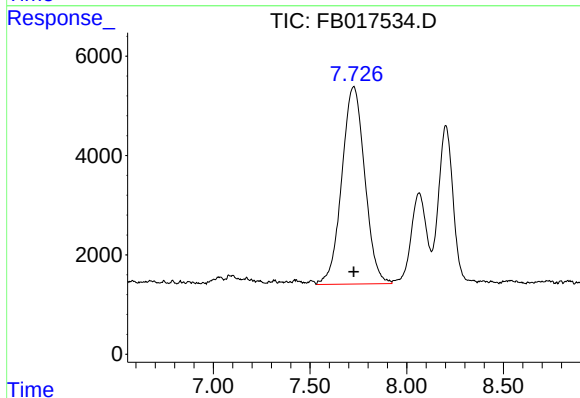


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 327302
Conc: 23.23 ng/ml

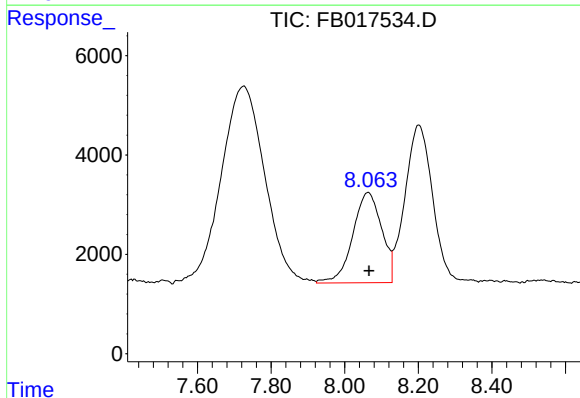


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.002 min
Response: 99113
Conc: 7.19 ng/ml

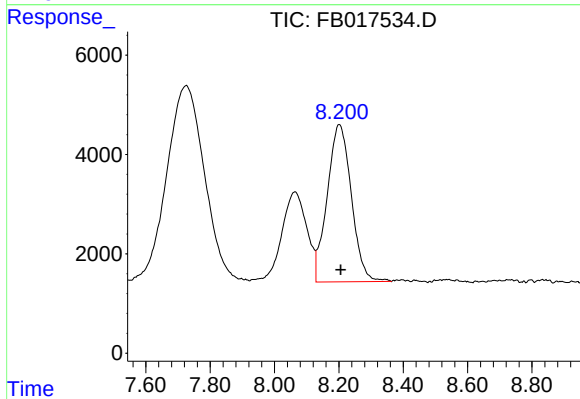


#4 Benzene

R.T.: 8.202 min
Delta R.T.: -0.003 min
Response: 165002
Conc: 9.36 ng/ml

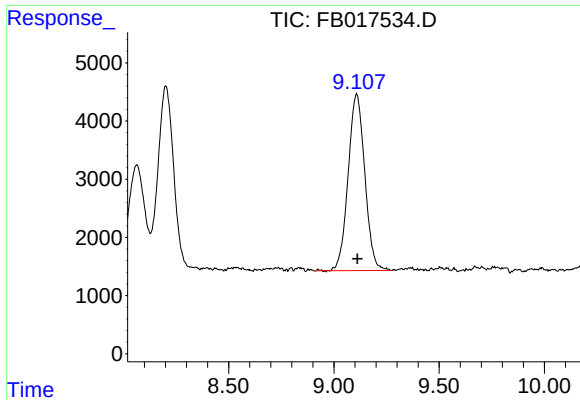


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.003 min
Response: 166783
Conc: 20.23 ng/ml

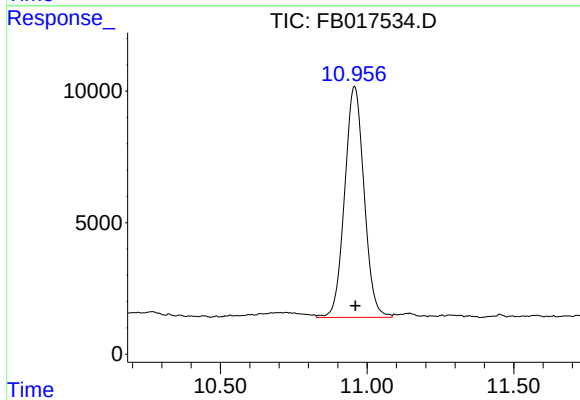


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.003 min
Response: 404418
Conc: 28.11 ng/ml

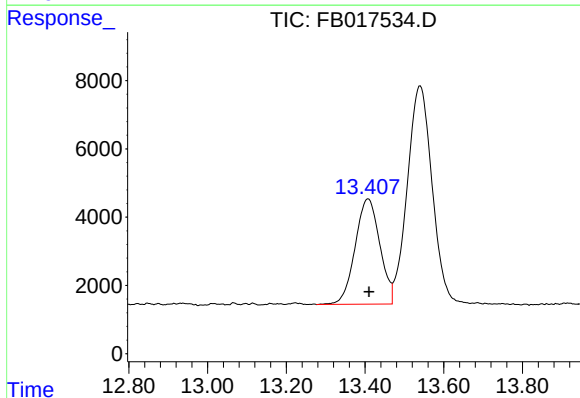


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.002 min
Response: 133960
Conc: 9.08 ng/ml

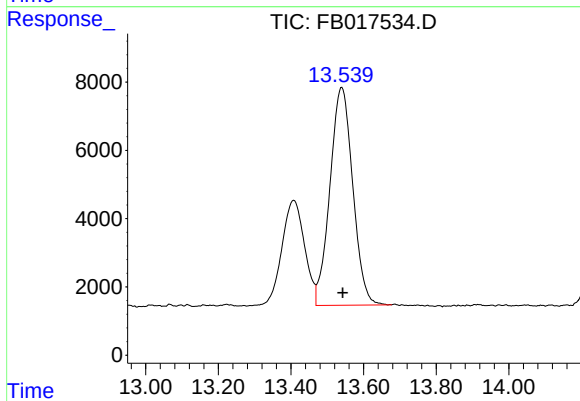


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.003 min
Response: 278627
Conc: 17.92 ng/ml

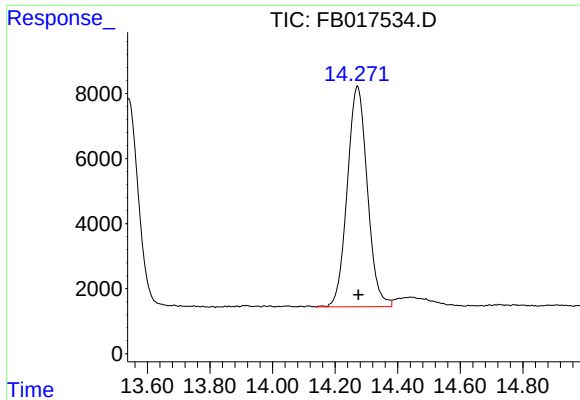

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 302194
Conc: 18.41 ng/ml

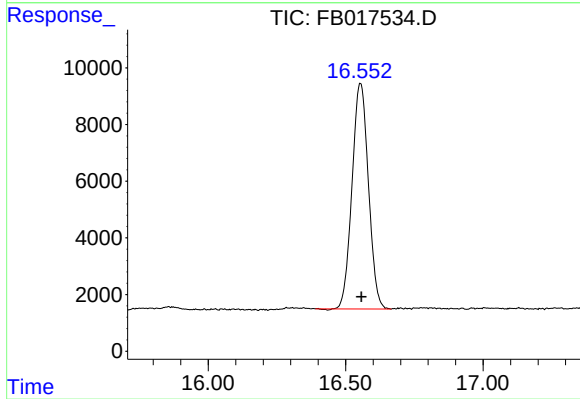

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.003 min
Response: 329978
Conc: 16.94 ng/ml