

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
 Data File : FB017535.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2018 11:15
 Operator : MJ/SJ
 Sample : J4282-11MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 24 11:38:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.108	168793	20.473 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.962	368809	26.320 ng/ml
2) t	2,2,4-Trimethylpentane	7.726	344386	24.438 ng/ml
3) t	n-Heptane	8.065	99654	7.231 ng/ml
4) t	Benzene	8.205	166343	9.435 ng/ml
6) t	Toluene	10.959	406359	28.247 ng/ml
7) t	Ethylbenzene	13.408	143246	9.713 ng/ml
8) t	m-Xylene	13.541	292450	18.813 ng/ml
9) t	O-Xylene	14.272	313809	19.117 ng/ml
10) t	1,2,4-Trimethylbenzene	16.555	346027	17.766 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
Data File : FB017535.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2018 11:15
Operator : MJ/SJ
Sample : J4282-11MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 24 11:38:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

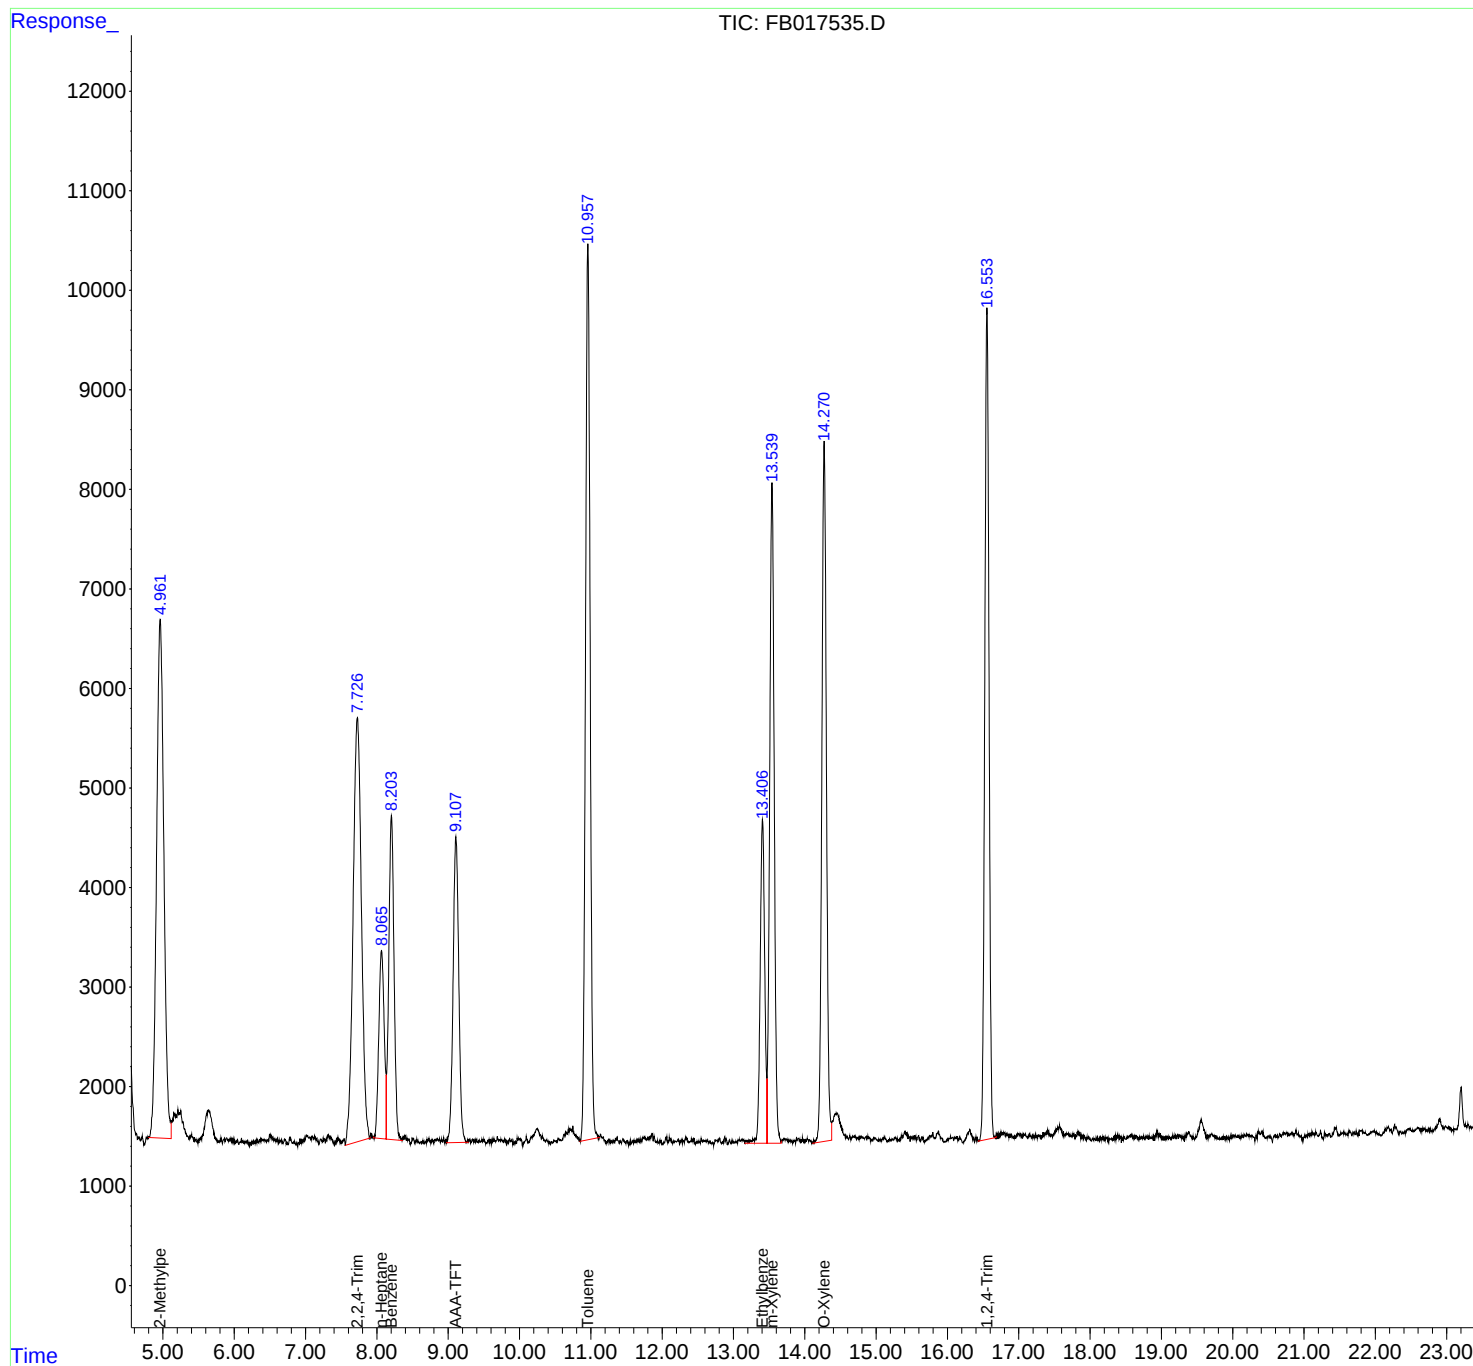

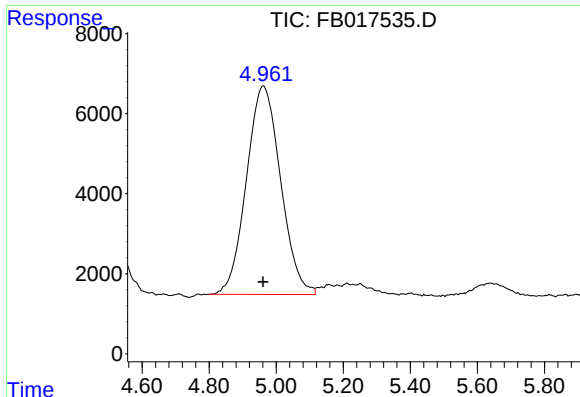


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.001 min
Response: 368809
Conc: 26.32 ng/ml

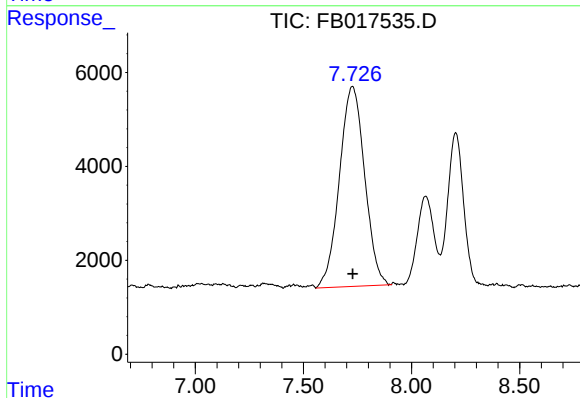


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: 0.000 min
Response: 344386
Conc: 24.44 ng/ml

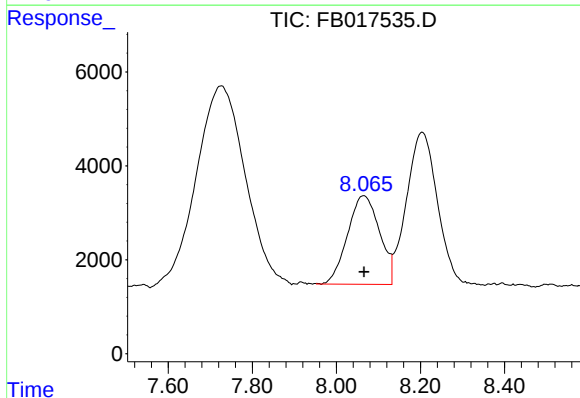


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 99654
Conc: 7.23 ng/ml

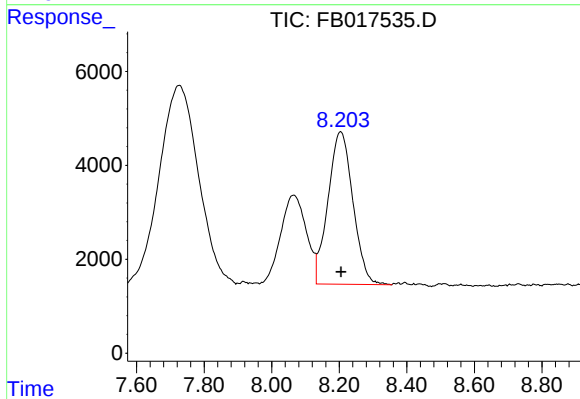


#4 Benzene

R.T.: 8.205 min
Delta R.T.: 0.000 min
Response: 166343
Conc: 9.43 ng/ml

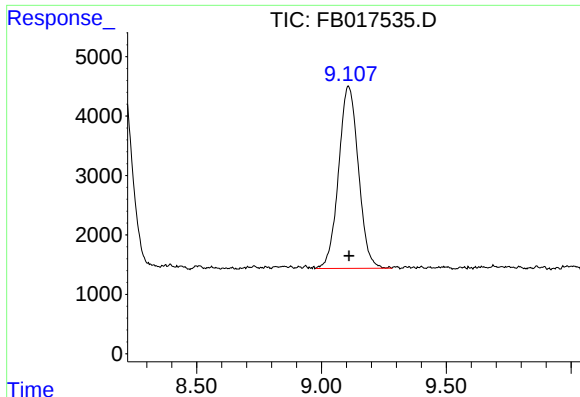


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.003 min
Response: 168793
Conc: 20.47 ng/ml

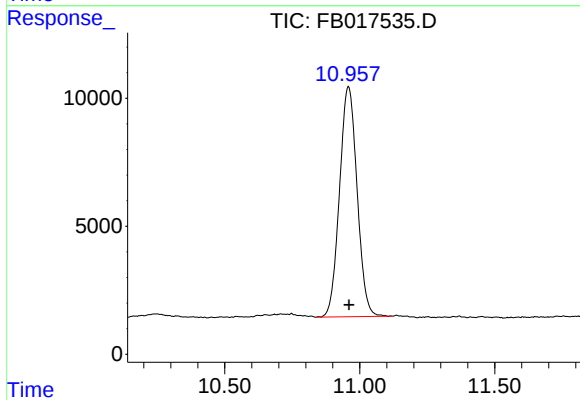


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.002 min
Response: 406359
Conc: 28.25 ng/ml

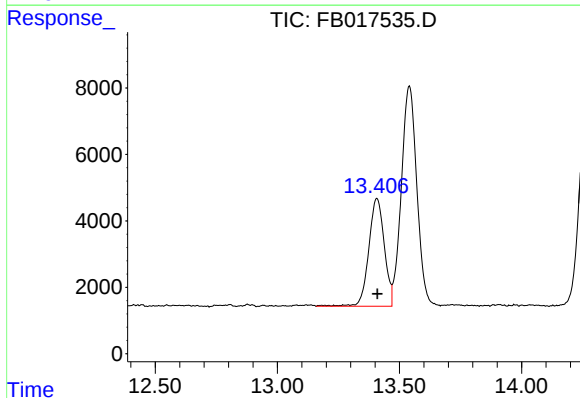


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 143246
Conc: 9.71 ng/ml

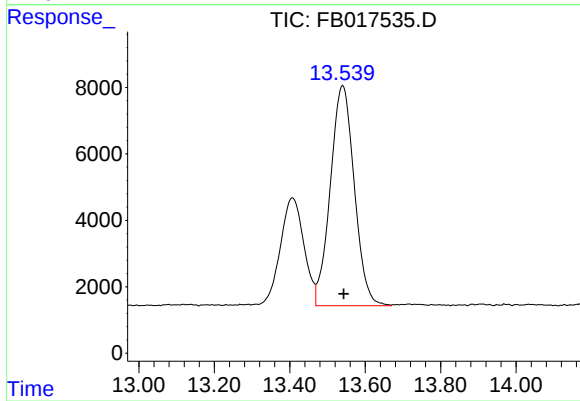


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.002 min
Response: 292450
Conc: 18.81 ng/ml

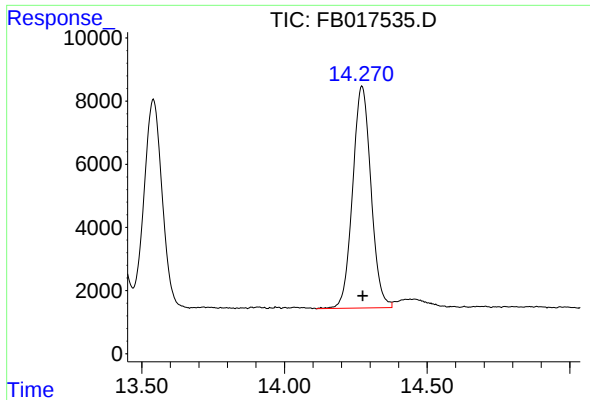

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 313809
Conc: 19.12 ng/ml

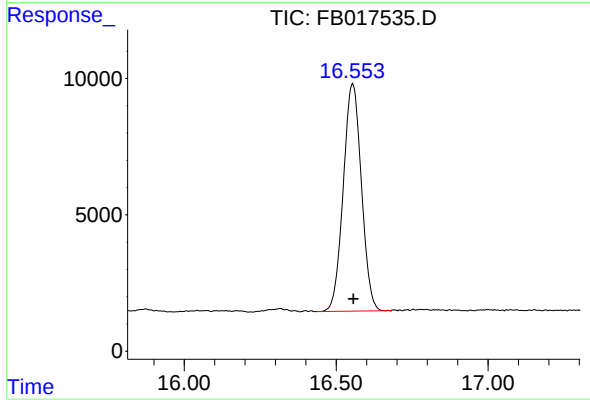

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.003 min
Response: 346027
Conc: 17.77 ng/ml