

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
 Data File : FB017531.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2018 9:11
 Operator : MJ/SJ
 Sample : BSF0824S1
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 24 09:51:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.110	182397	22.123 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.962	409585	29.230 ng/ml
2) t	2,2,4-Trimethylpentane	7.726	421197	29.889 ng/ml
3) t	n-Heptane	8.065	123404	8.954 ng/ml
4) t	Benzene	8.204	170220	9.655 ng/ml
6) t	Toluene	10.959	442929	30.789 ng/ml
7) t	Ethylbenzene	13.409	150711	10.220 ng/ml
8) t	m-Xylene	13.541	322758	20.762 ng/ml
9) t	O-Xylene	14.273	344978	21.015 ng/ml
10) t	1,2,4-Trimethylbenzene	16.556	404698	20.779 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082418\
Data File : FB017531.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2018 9:11
Operator : MJ/SJ
Sample : BSF0824S1
Misc : 5.03g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 24 09:51:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

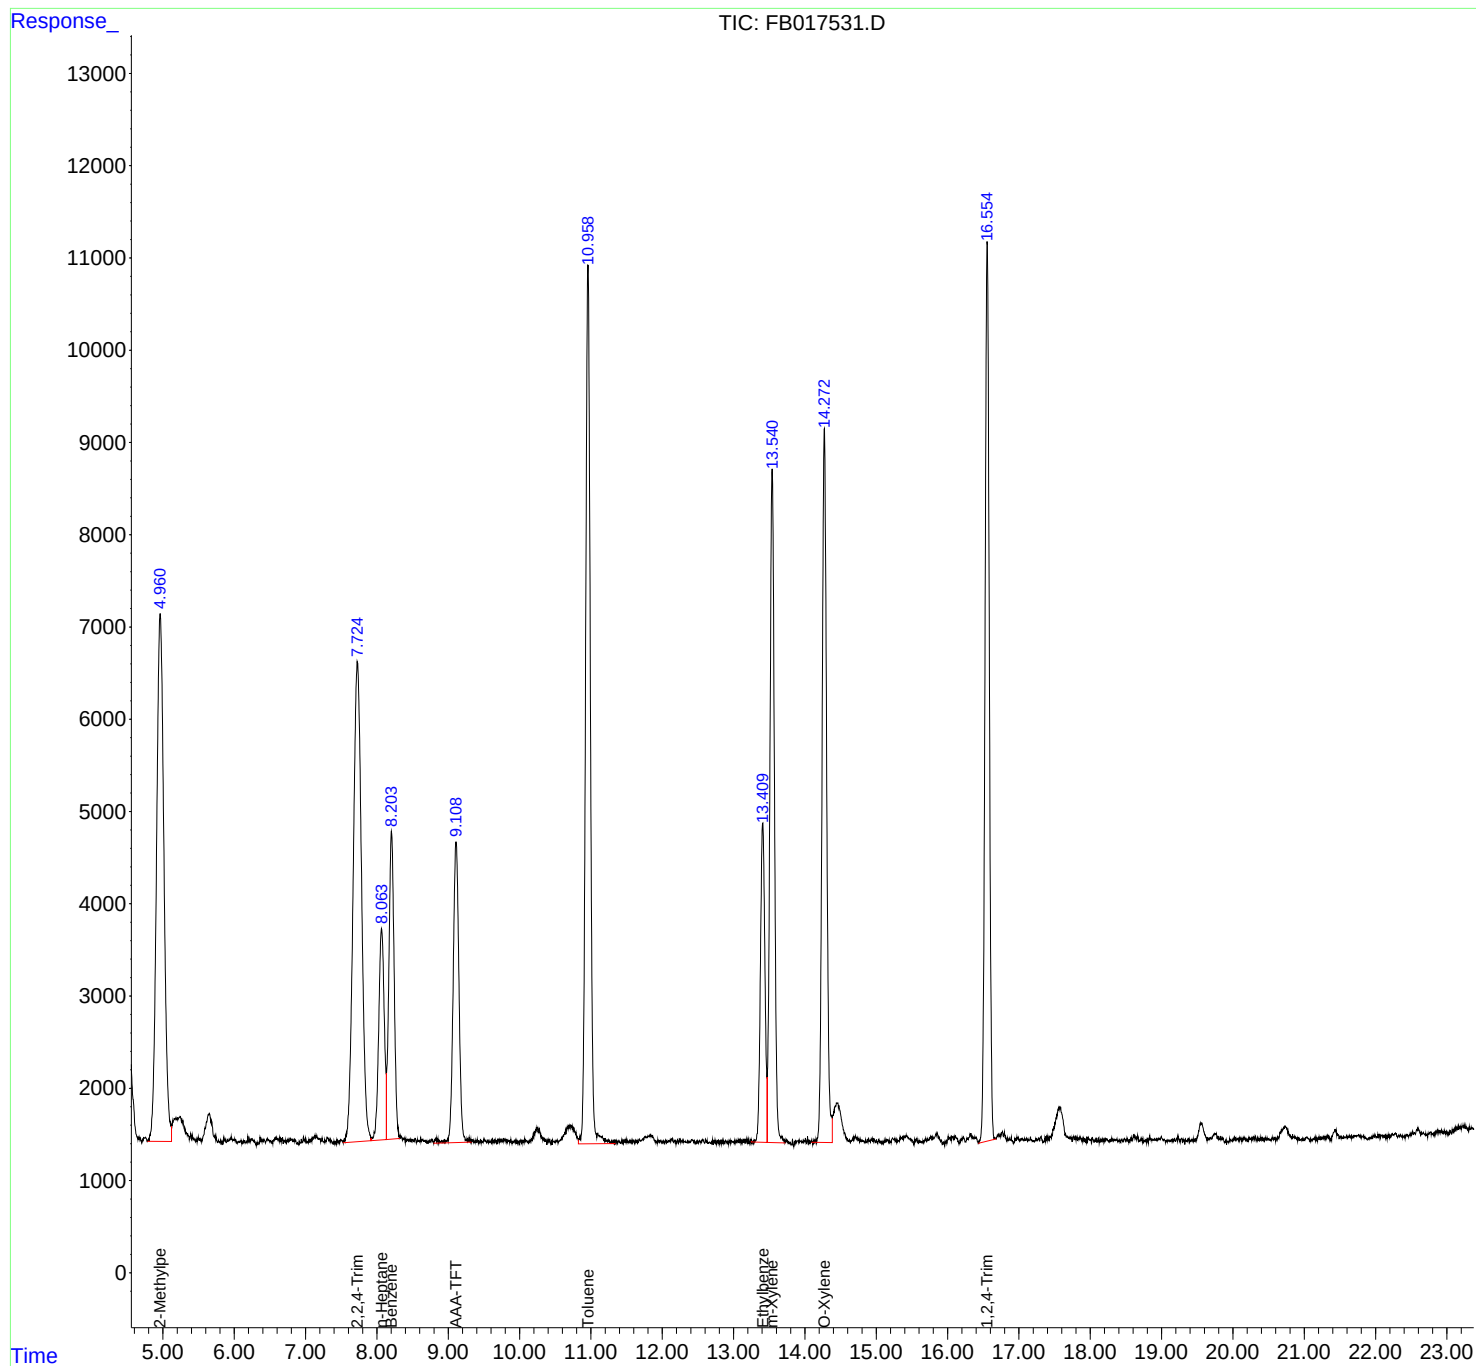

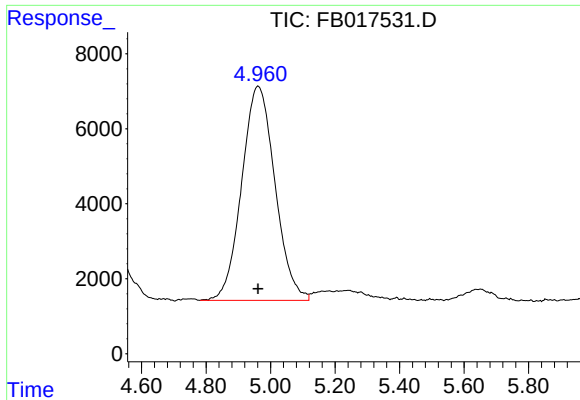


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 409585
Conc: 29.23 ng/ml

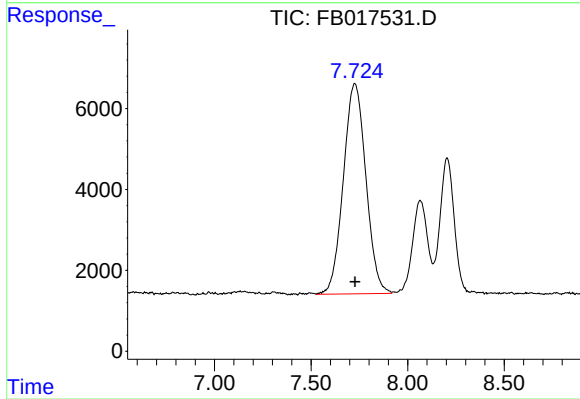


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 421197
Conc: 29.89 ng/ml

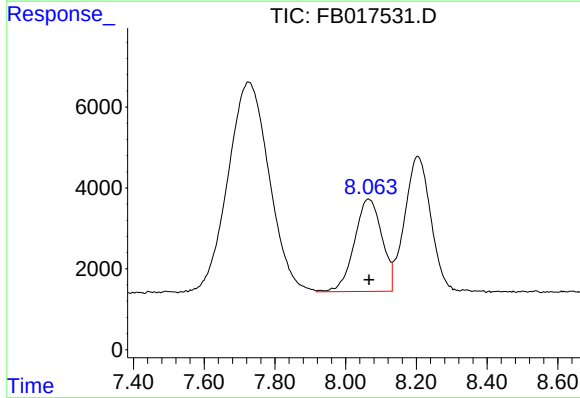


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 123404
Conc: 8.95 ng/ml

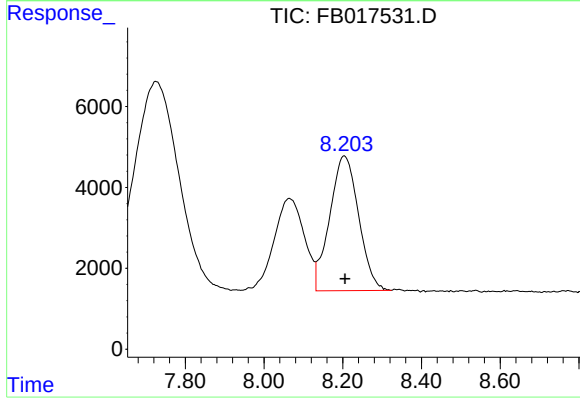


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.001 min
Response: 170220
Conc: 9.65 ng/ml

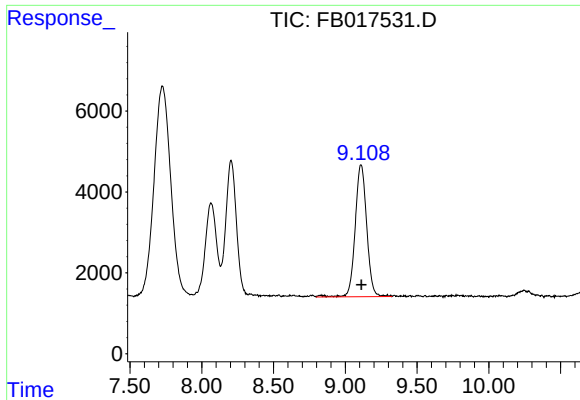


#5 AAA-TFT

R.T.: 9.110 min
 Delta R.T.: -0.001 min
 Response: 182397
 Conc: 22.12 ng/ml

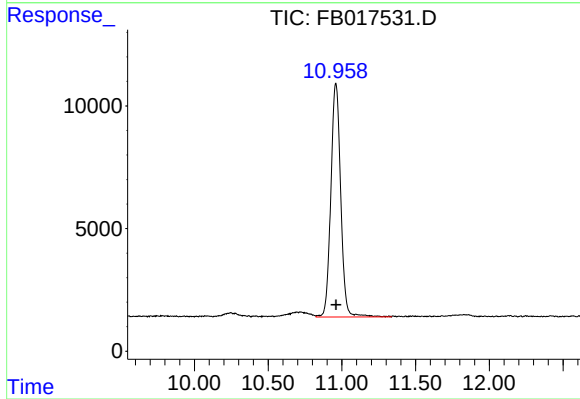


#6 Toluene

R.T.: 10.959 min
 Delta R.T.: 0.000 min
 Response: 442929
 Conc: 30.79 ng/ml

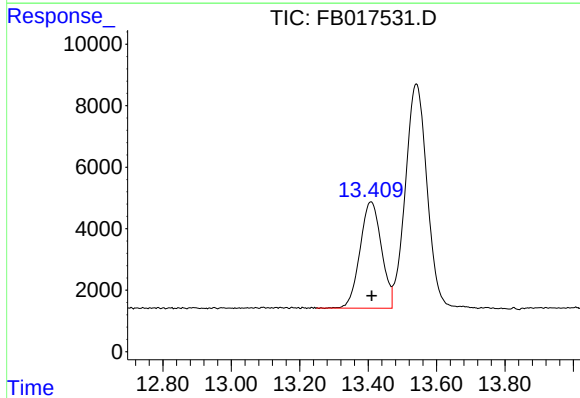


#7 Ethylbenzene

R.T.: 13.409 min
 Delta R.T.: -0.002 min
 Response: 150711
 Conc: 10.22 ng/ml

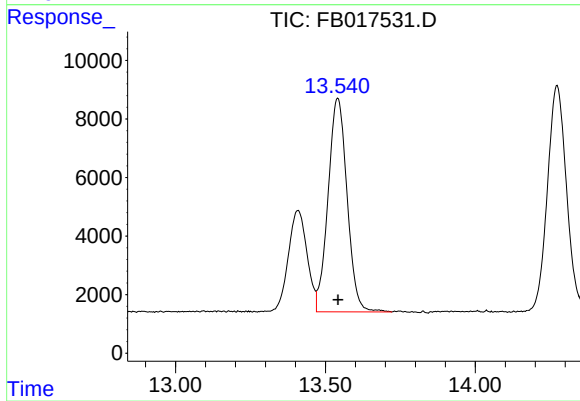


#8 m-Xylene

R.T.: 13.541 min
 Delta R.T.: -0.001 min
 Response: 322758
 Conc: 20.76 ng/ml

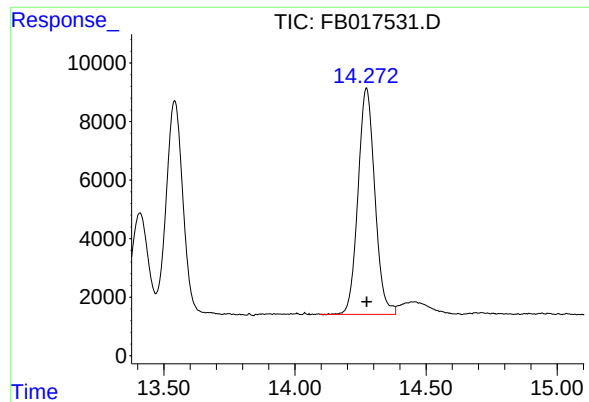

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.001 min
Response: 344978
Conc: 21.02 ng/ml

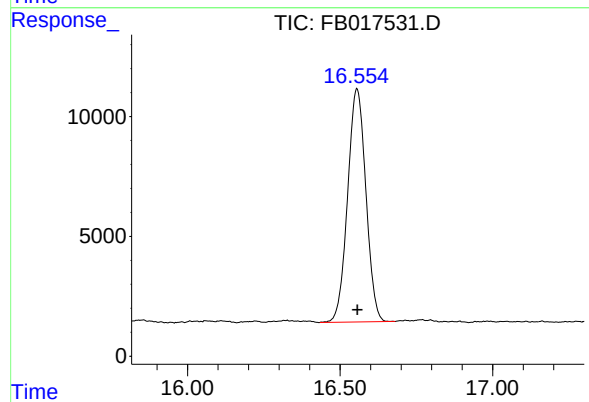

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.002 min
Response: 404698
Conc: 20.78 ng/ml