

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
 Data File : FB022172.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2019 19:01
 Operator : DD/AJ
 Sample : K4496-01MSD
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S600-M-1.0-1.5-082219MSD

Integration File: Calibration.e
 Quant Time: Aug 26 00:51:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.984	442969	20.855 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1141561	28.523 ng/ml
2) t 2,2,4-Trimethylpentane	7.604	1146224	28.458 ng/ml
3) t n-Heptane	7.943	358145	9.376 ng/ml
4) t Benzene	8.078	448008	9.979 ng/ml
6) t Toluene	10.825	892125	29.020 ng/ml
7) t Ethylbenzene	13.271	215289	10.550 ng/ml
8) t m-Xylene	13.403	451506	21.439 ng/ml
9) t O-Xylene	14.132	481152	21.514 ng/ml
10) t 1,2,4-Trimethylbenzene	16.412	517319	20.172 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
Data File : FB022172.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2019 19:01
Operator : DD/AJ
Sample : K4496-01MSD
Misc : 5.02/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MSD

Integration File: Calibration.e
Quant Time: Aug 26 00:51:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

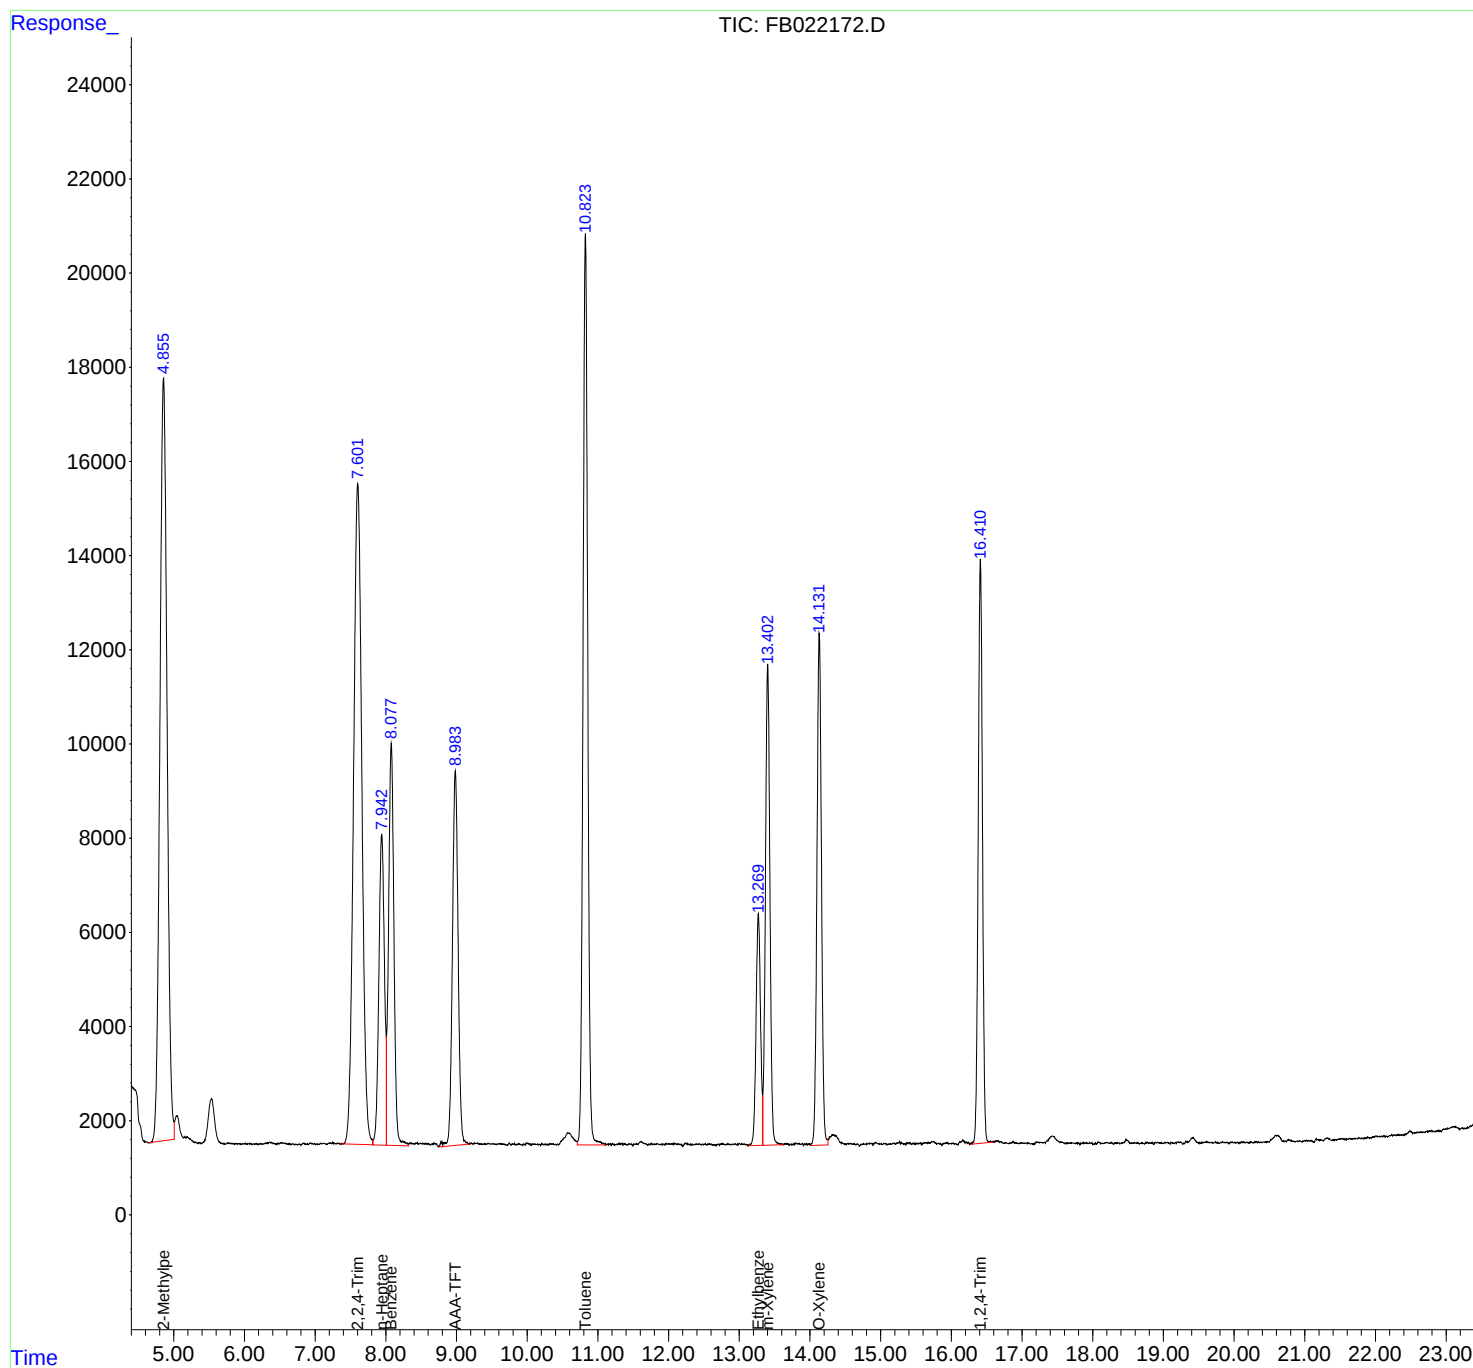


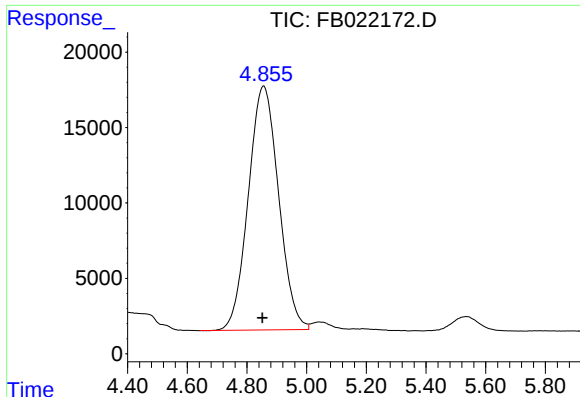

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 1141561
Conc: 28.52 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MSD

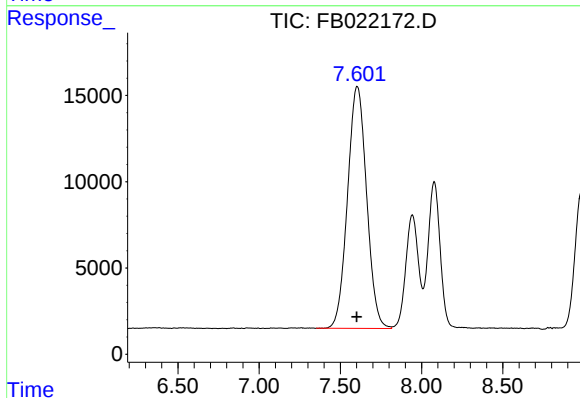


#2 2,2,4-Trimethylpentane

R.T.: 7.604 min
Delta R.T.: 0.004 min
Response: 1146224
Conc: 28.46 ng/ml

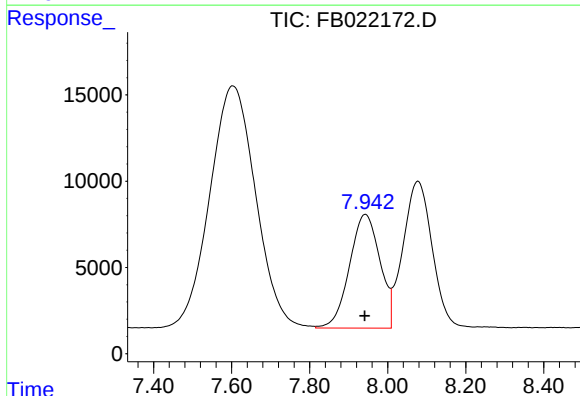


#3 n-Heptane

R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 358145
Conc: 9.38 ng/ml

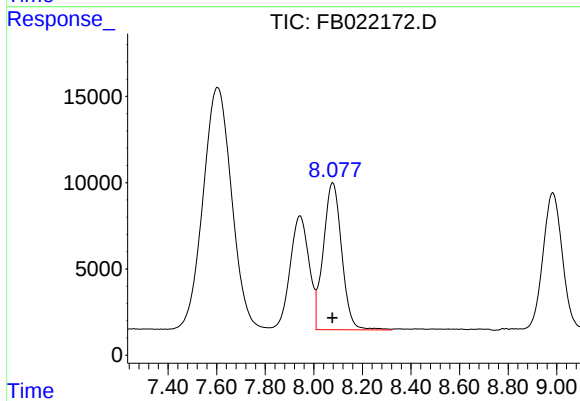

#4 Benzene


R.T.: 8.078 min
Delta R.T.: 0.002 min
Response: 448008
Conc: 9.98 ng/ml

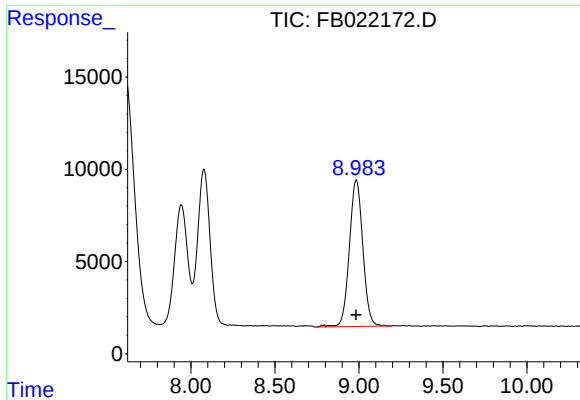

#5 AAA-TFT


R.T.: 8.984 min
Delta R.T.: 0.002 min
Response: 442969
Conc: 20.86 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MSD

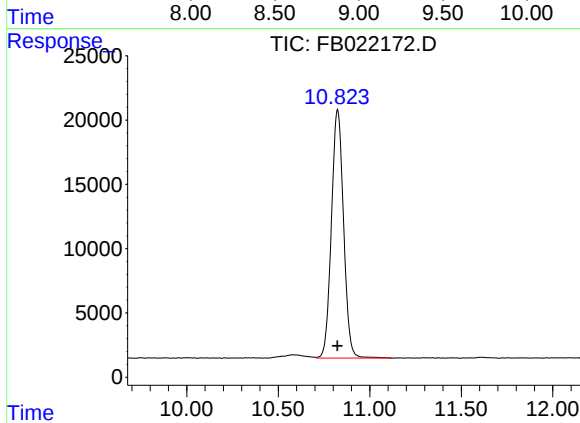


#6 Toluene

R.T.: 10.825 min
Delta R.T.: 0.002 min
Response: 892125
Conc: 29.02 ng/ml

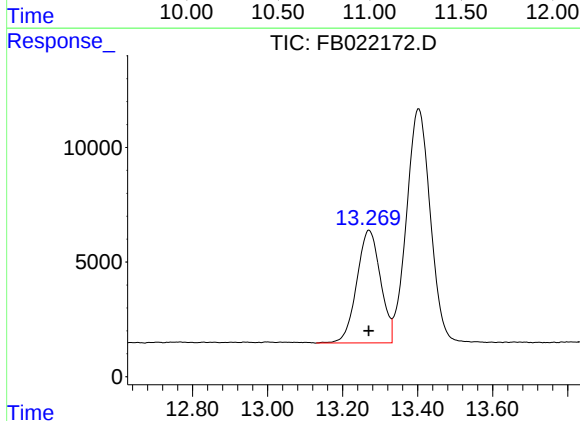


#7 Ethylbenzene

R.T.: 13.271 min
Delta R.T.: 0.001 min
Response: 215289
Conc: 10.55 ng/ml

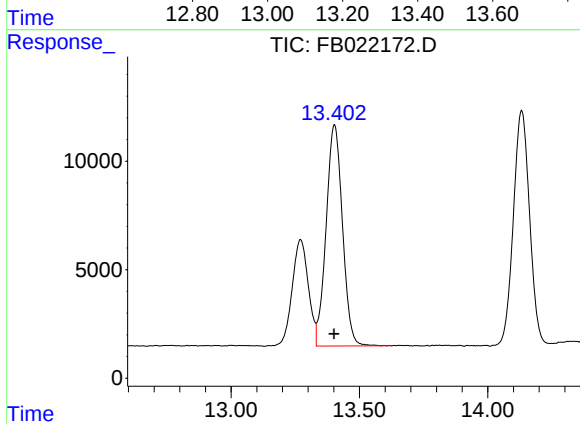

#8 m-Xylene


R.T.: 13.403 min
Delta R.T.: 0.001 min
Response: 451506
Conc: 21.44 ng/ml

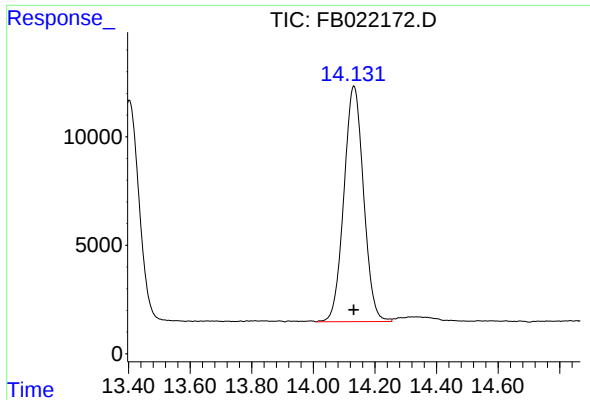

#9 O-Xylene

R.T.: 14.132 min
Delta R.T.: 0.000 min
Response: 481152
Conc: 21.51 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MSD

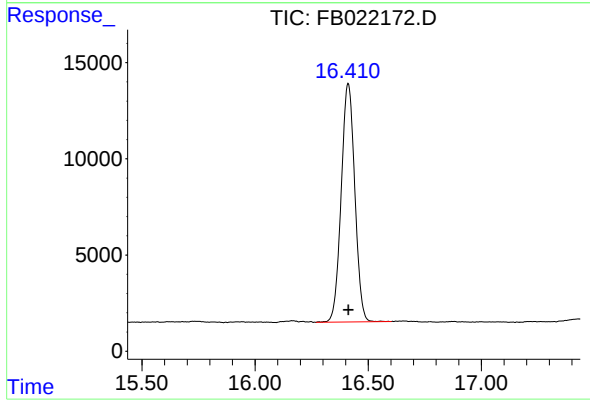

#10 1,2,4-Trimethylbenzene

R.T.: 16.412 min
Delta R.T.: 0.000 min
Response: 517319
Conc: 20.17 ng/ml