

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
 Data File : FB022155.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2019 9:55
 Operator : DD/AJ
 Sample : BSF0824S1
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0824S1

Integration File: Calibration.e
 Quant Time: Aug 26 00:48:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	416018	19.586 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	1179502	29.471 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	1178388	29.257 ng/ml
3) t n-Heptane	7.945	372244	9.745 ng/ml
4) t Benzene	8.080	413852	9.219 ng/ml
6) t Toluene	10.827	847632	27.572 ng/ml
7) t Ethylbenzene	13.273	211234	10.351 ng/ml
8) t m-Xylene	13.406	446941	21.222 ng/ml
9) t O-Xylene	14.135	470473	21.036 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	515502	20.101 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
Data File : FB022155.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2019 9:55
Operator : DD/AJ
Sample : BSF0824S1
Misc : 5.00/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0824S1

Integration File: Calibration.e
Quant Time: Aug 26 00:48:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

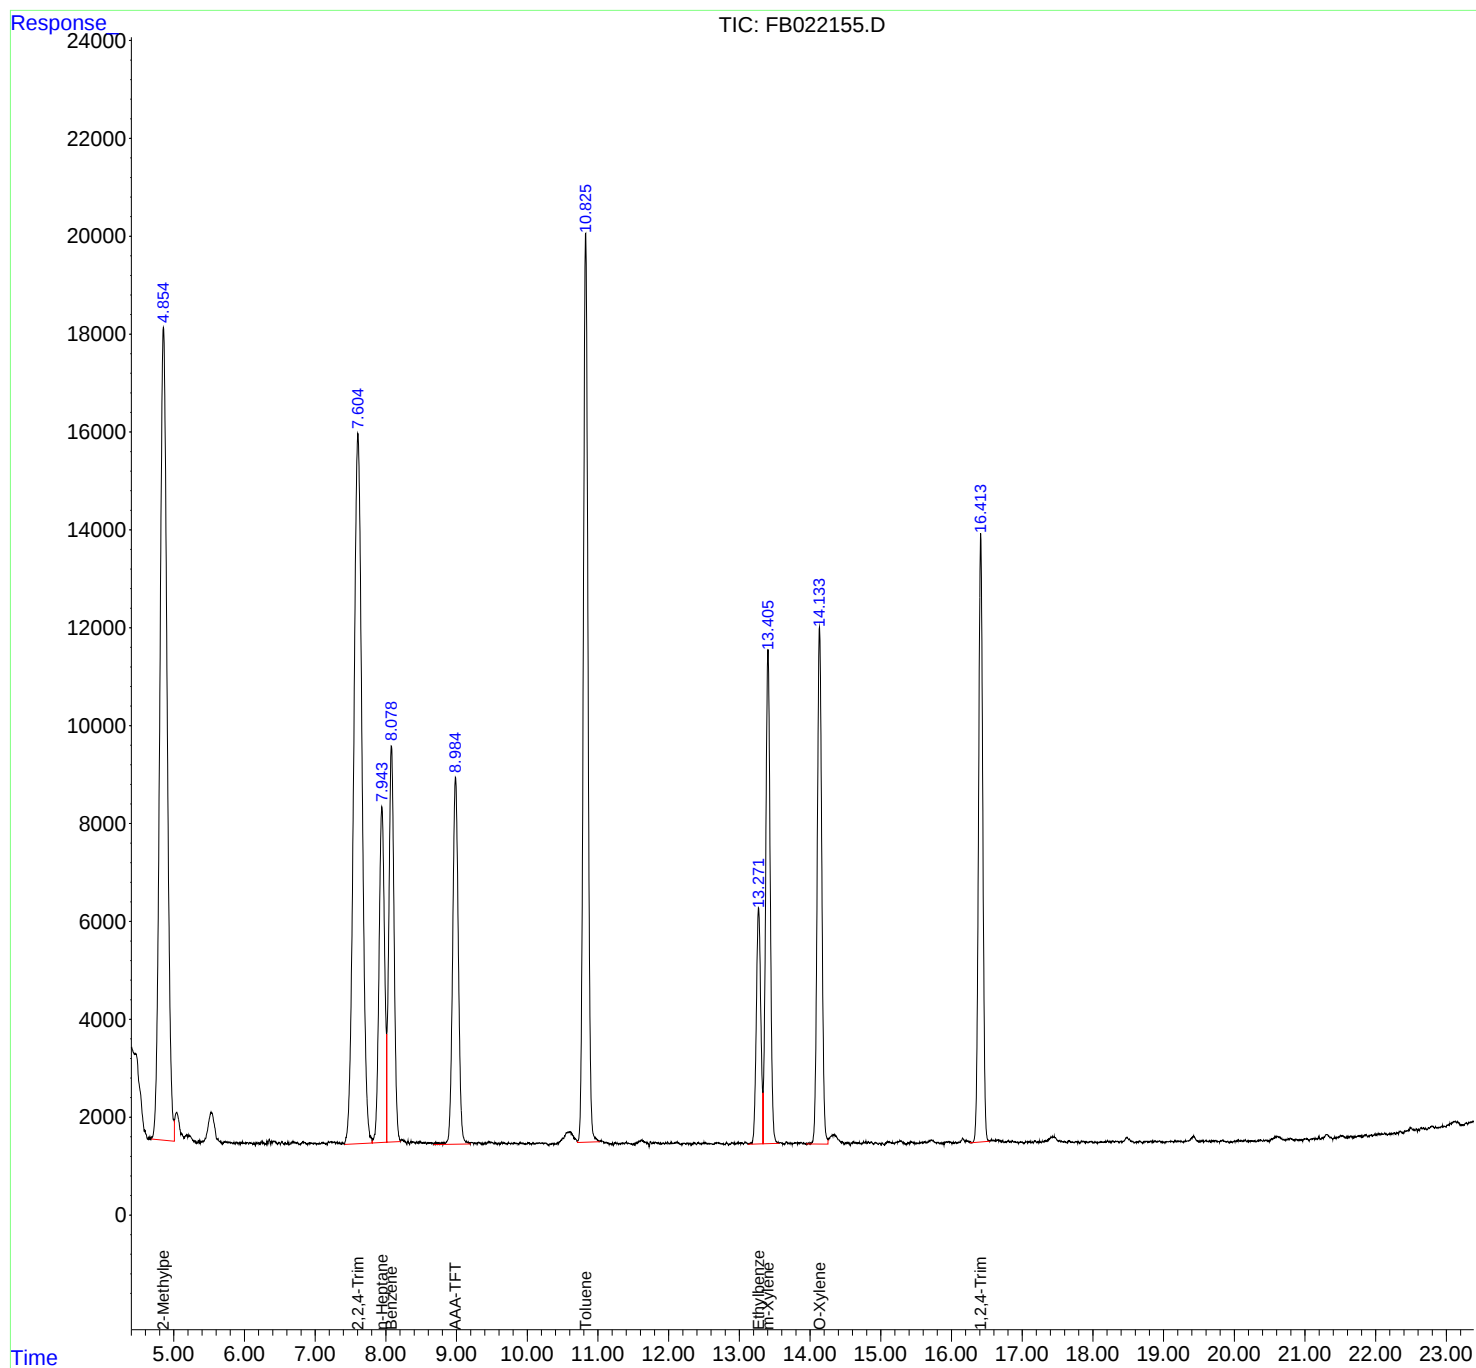


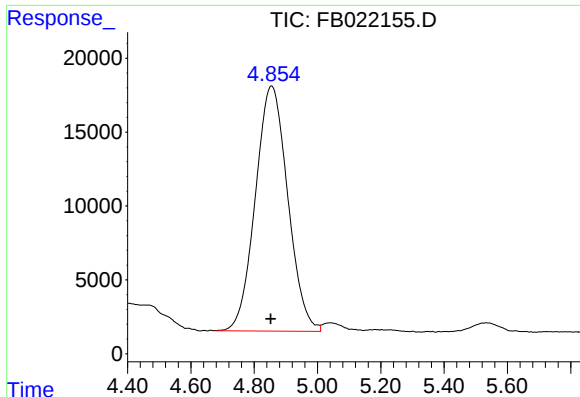

#1 2-Methylpentane


R.T.: 4.855 min
Delta R.T.: 0.003 min
Response: 1179502
Conc: 29.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0824S1

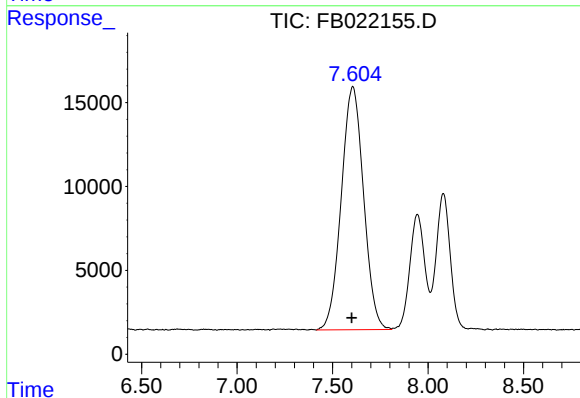


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: 0.006 min
Response: 1178388
Conc: 29.26 ng/ml

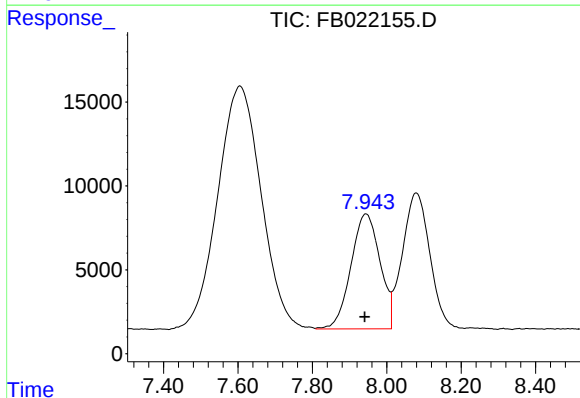


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: 0.003 min
Response: 372244
Conc: 9.74 ng/ml

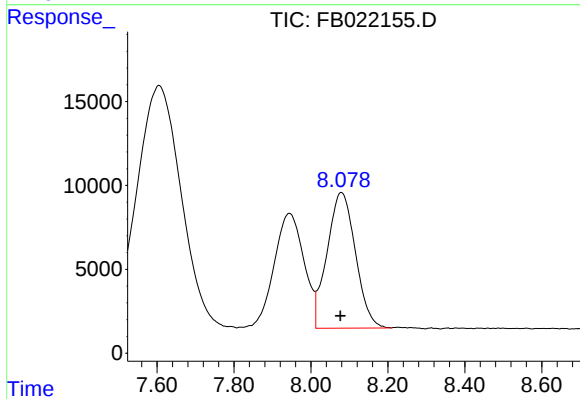

#4 Benzene


R.T.: 8.080 min
Delta R.T.: 0.004 min
Response: 413852
Conc: 9.22 ng/ml

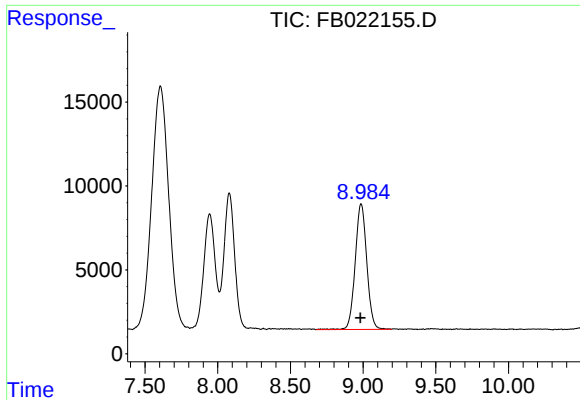

#5 AAA-TFT


R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 416018
Conc: 19.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0824S1

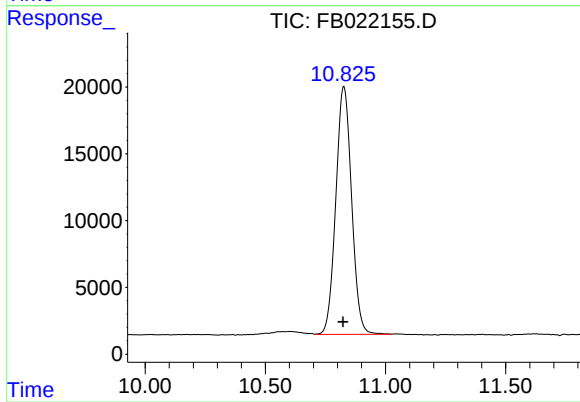


#6 Toluene

R.T.: 10.827 min
Delta R.T.: 0.004 min
Response: 847632
Conc: 27.57 ng/ml

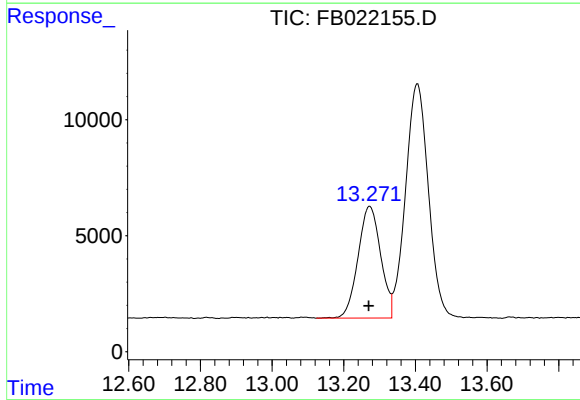


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.003 min
Response: 211234
Conc: 10.35 ng/ml

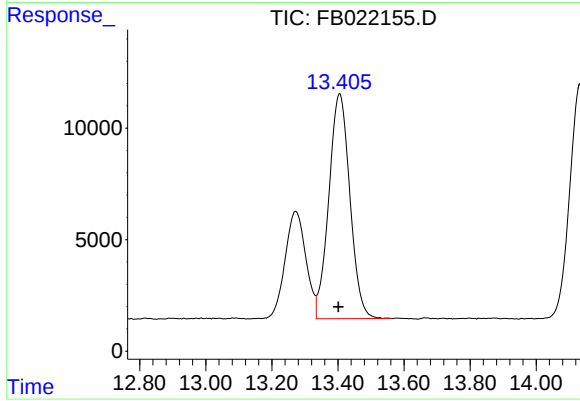

#8 m-Xylene


R.T.: 13.406 min
Delta R.T.: 0.004 min
Response: 446941
Conc: 21.22 ng/ml

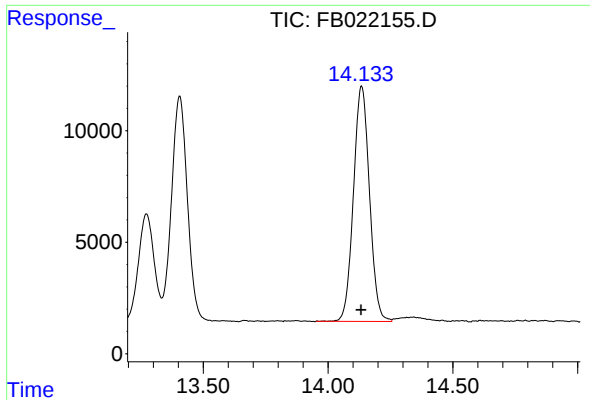

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.003 min
Response: 470473
Conc: 21.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0824S1

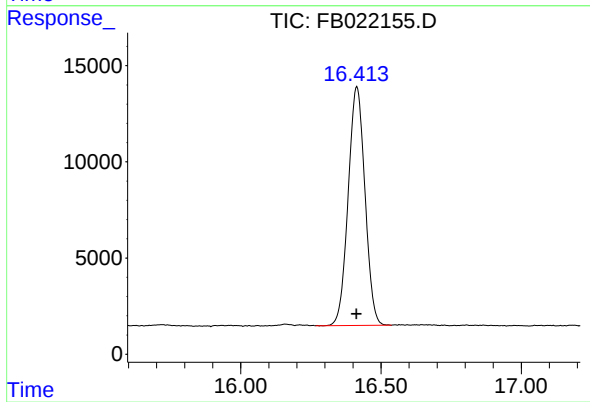

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.002 min
Response: 515502
Conc: 20.10 ng/ml