

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
 Data File : FB022171.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2019 18:31
 Operator : DD/AJ
 Sample : K4496-01MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S600-M-1.0-1.5-082219MS

Integration File: Calibration.e
 Quant Time: Aug 26 00:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.983	454351	21.391 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	1168391	29.193 ng/ml
2) t 2,2,4-Trimethylpentane	7.602	1198952	29.767 ng/ml
3) t n-Heptane	7.941	372096	9.741 ng/ml
4) t Benzene	8.076	447038	9.958 ng/ml
6) t Toluene	10.824	917754	29.853 ng/ml
7) t Ethylbenzene	13.270	213785	10.476 ng/ml
8) t m-Xylene	13.403	446454	21.199 ng/ml
9) t O-Xylene	14.132	473577	21.175 ng/ml
10) t 1,2,4-Trimethylbenzene	16.412	514636	20.067 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082419\
Data File : FB022171.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2019 18:31
Operator : DD/AJ
Sample : K4496-01MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MS

Integration File: Calibration.e
Quant Time: Aug 26 00:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

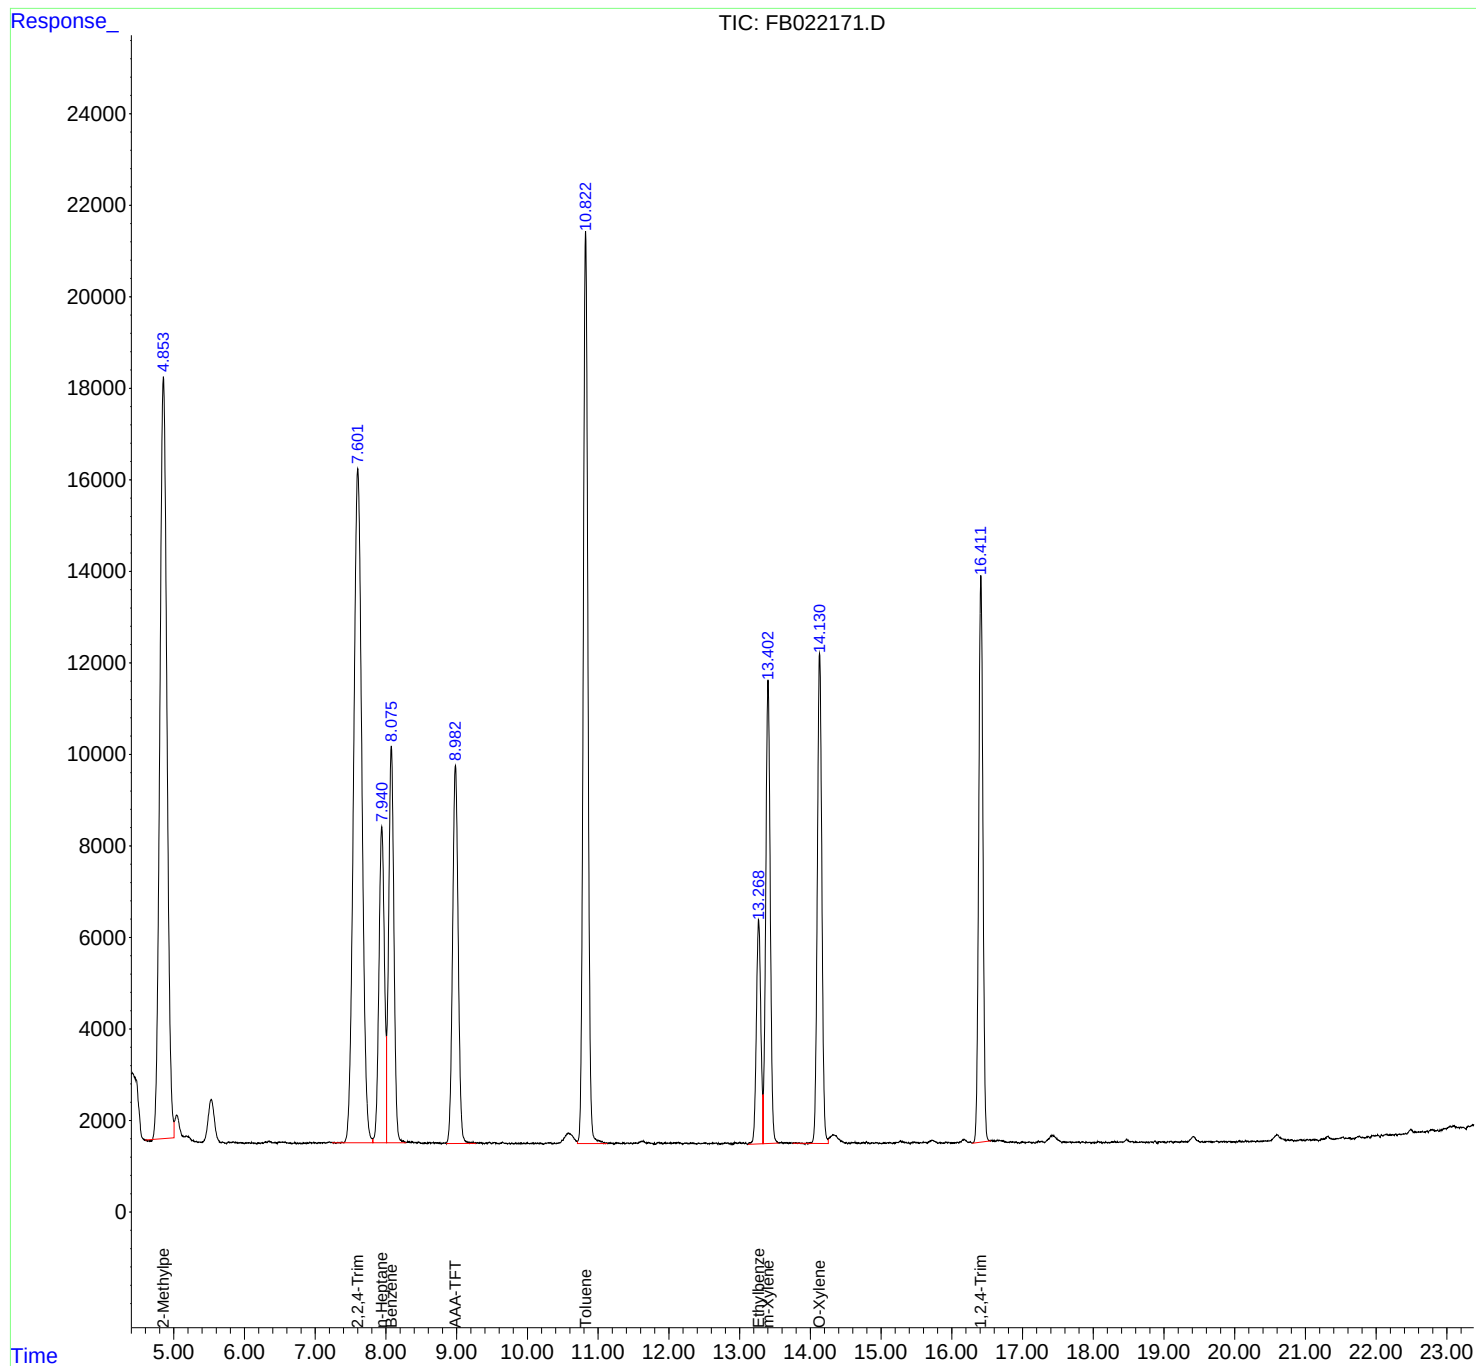


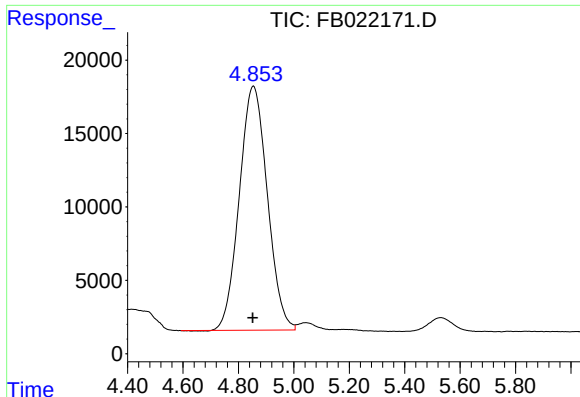

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: 0.002 min
Response: 1168391
Conc: 29.19 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MS

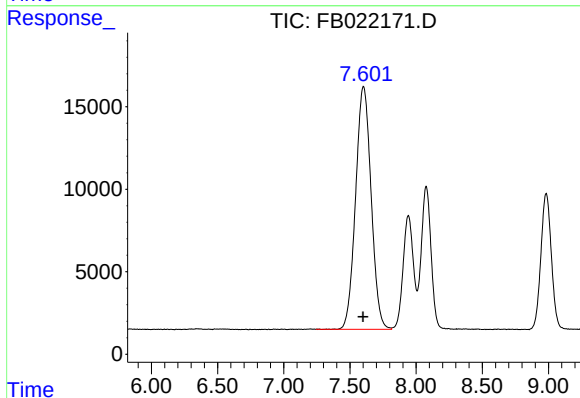


#2 2,2,4-Trimethylpentane

R.T.: 7.602 min
Delta R.T.: 0.003 min
Response: 1198952
Conc: 29.77 ng/ml

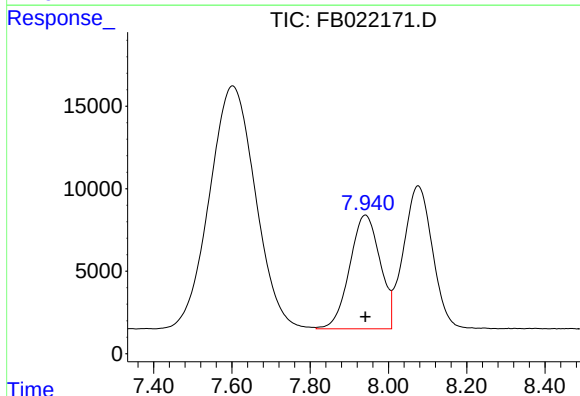


#3 n-Heptane

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 372096
Conc: 9.74 ng/ml

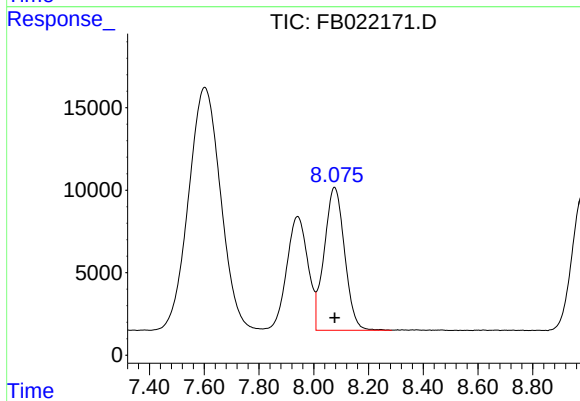

#4 Benzene


R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 447038
Conc: 9.96 ng/ml

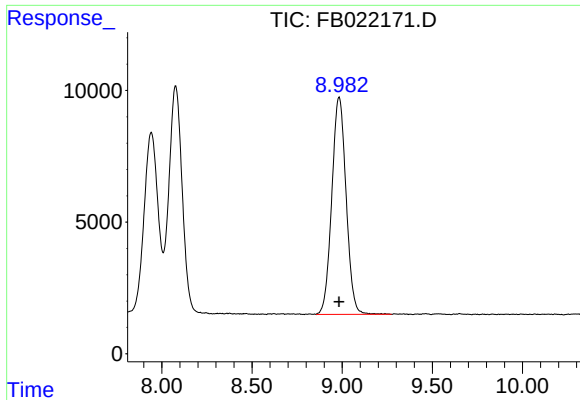

#5 AAA-TFT


R.T.: 8.983 min
Delta R.T.: 0.000 min
Response: 454351
Conc: 21.39 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MS

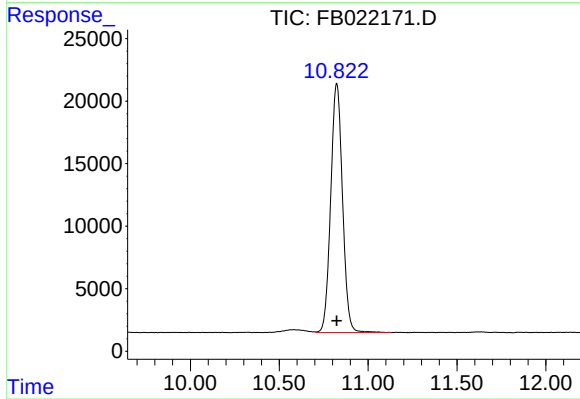


#6 Toluene

R.T.: 10.824 min
Delta R.T.: 0.000 min
Response: 917754
Conc: 29.85 ng/ml

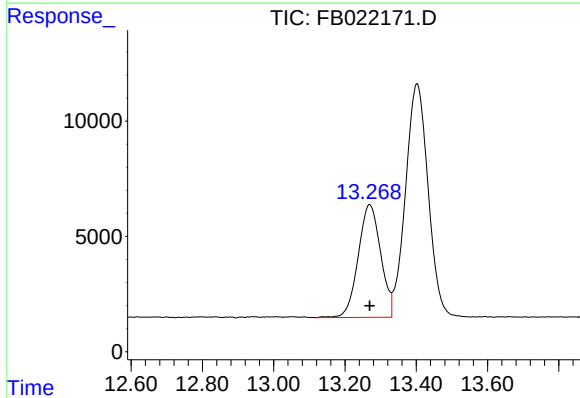


#7 Ethylbenzene

R.T.: 13.270 min
Delta R.T.: 0.000 min
Response: 213785
Conc: 10.48 ng/ml

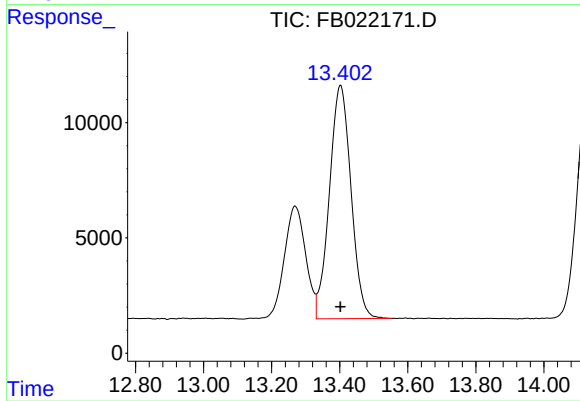

#8 m-Xylene


R.T.: 13.403 min
Delta R.T.: 0.001 min
Response: 446454
Conc: 21.20 ng/ml

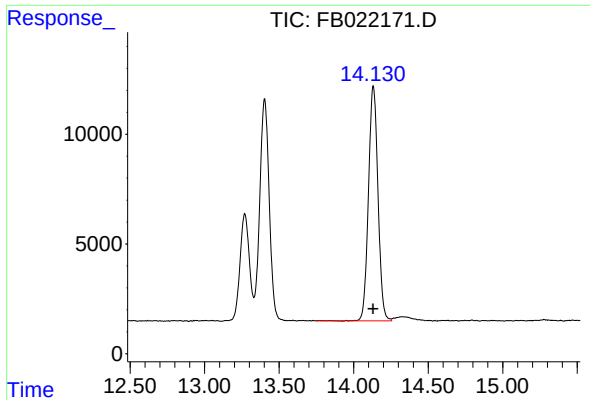

#9 O-Xylene

R.T.: 14.132 min
Delta R.T.: 0.000 min
Response: 473577
Conc: 21.17 ng/ml

Instrument :
FID_B
ClientSampleId :
S600-M-1.0-1.5-082219MS

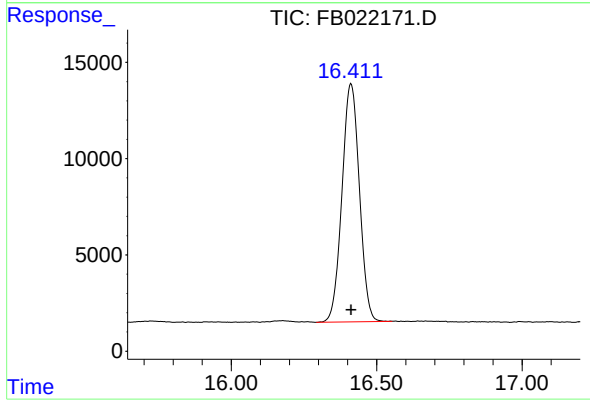

#10 1,2,4-Trimethylbenzene

R.T.: 16.412 min
Delta R.T.: 0.000 min
Response: 514636
Conc: 20.07 ng/ml