

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082420\
 Data File : FB024788.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2020 15:11
 Operator : DD/AJ
 Sample : L3773-01MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 25 00:54:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	472089	22.862 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	712593	29.612 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	702853	25.356 ng/ml
3) t n-Heptane	7.761	236909	8.713 ng/ml
4) t Benzene	7.894	368526	10.501 ng/ml
6) t Toluene	10.632	1053332	30.579 ng/ml
7) t Ethylbenzene	13.072	306190	9.564 ng/ml
8) t m-Xylene	13.205	606971	19.451 ng/ml
9) t O-Xylene	13.933	589461	19.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	479526	19.525 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082420\
Data File : FB024788.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2020 15:11
Operator : DD/AJ
Sample : L3773-01MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 25 00:54:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

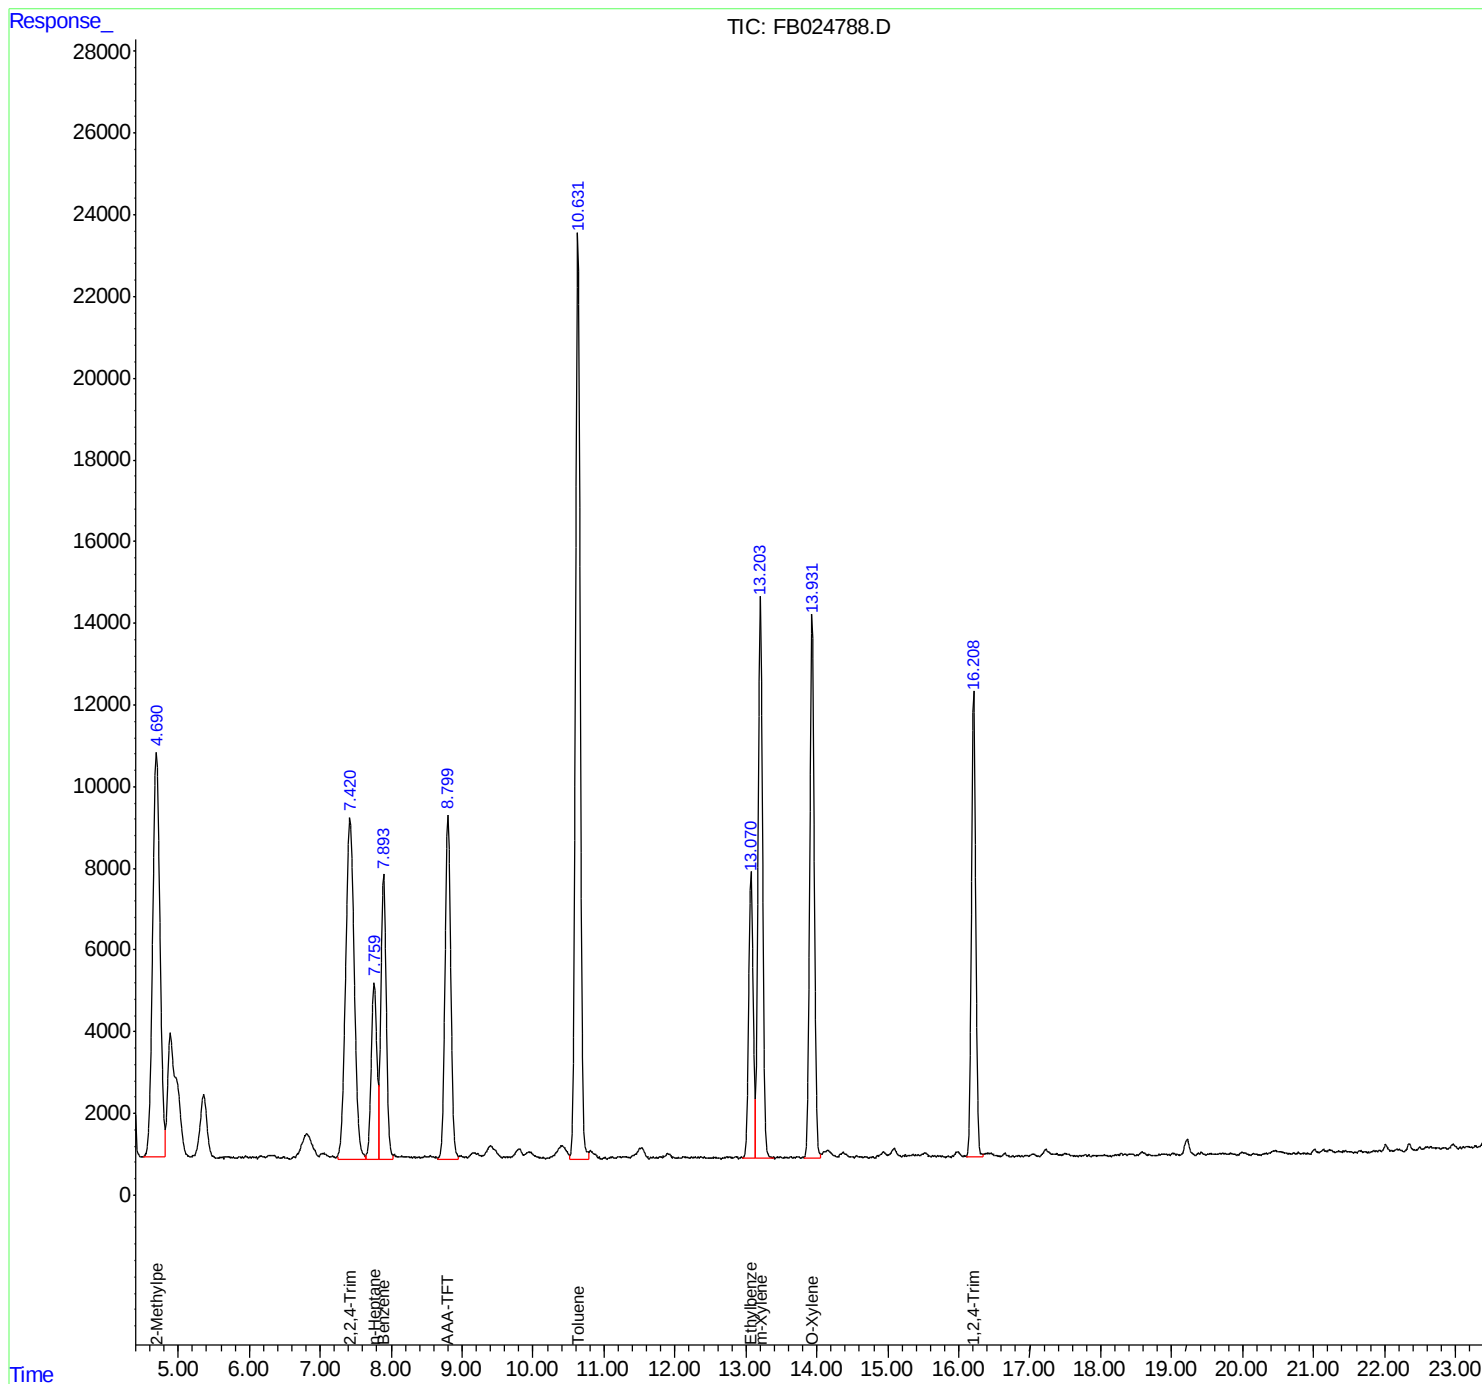

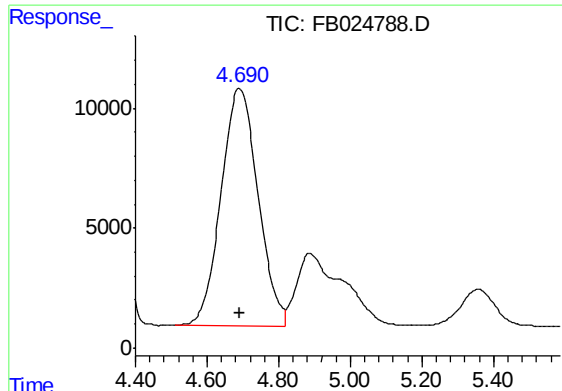


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 712593
Conc: 29.61 ng/ml

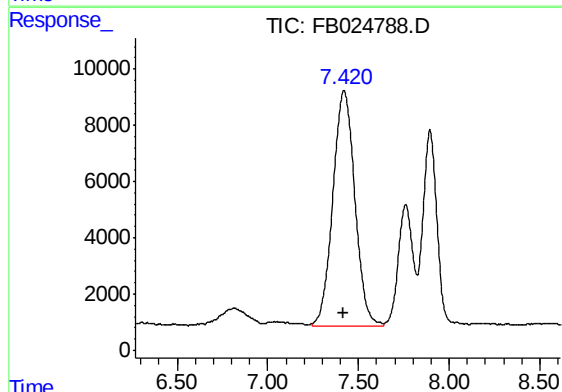


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.003 min
Response: 702853
Conc: 25.36 ng/ml

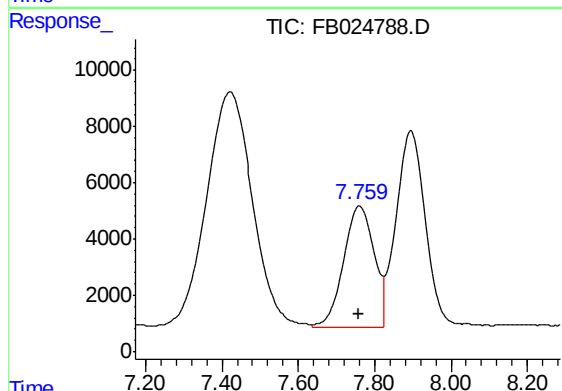


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.003 min
Response: 236909
Conc: 8.71 ng/ml

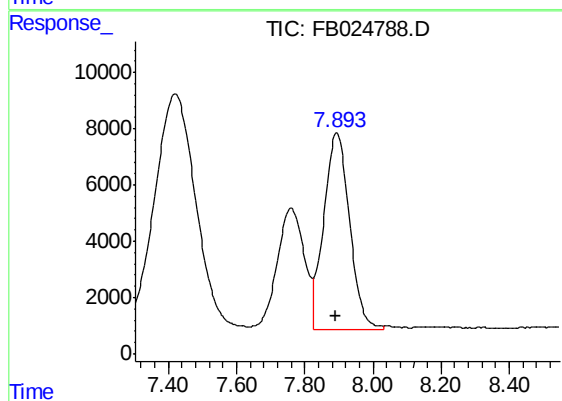


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 368526
Conc: 10.50 ng/ml

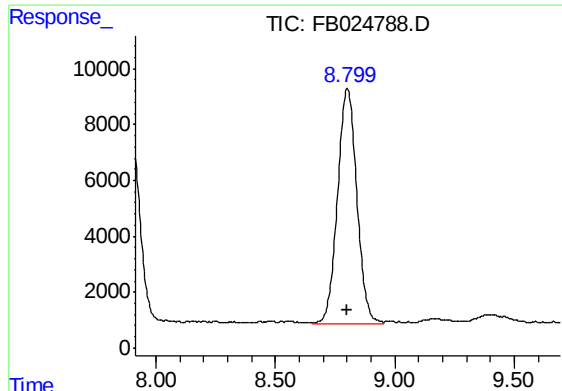


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 472089
Conc: 22.86 ng/ml

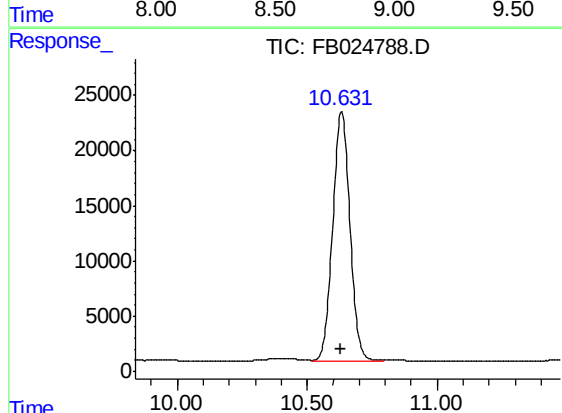


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.003 min
Response: 1053332
Conc: 30.58 ng/ml

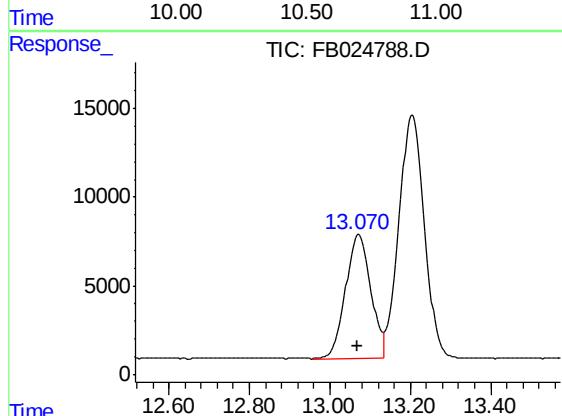


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 306190
Conc: 9.56 ng/ml

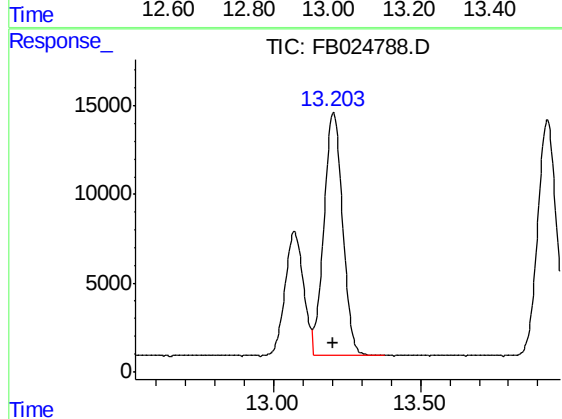


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.003 min
Response: 606971
Conc: 19.45 ng/ml

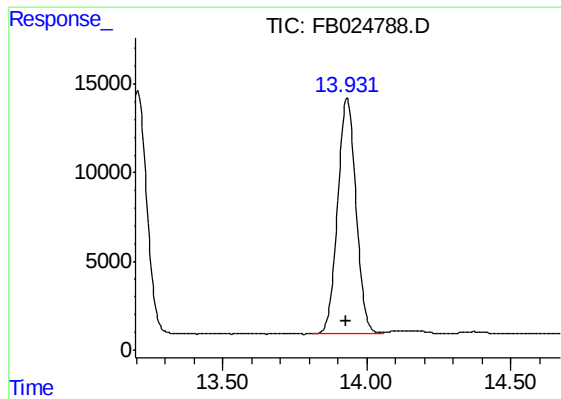

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.003 min
Response: 589461
Conc: 19.49 ng/ml

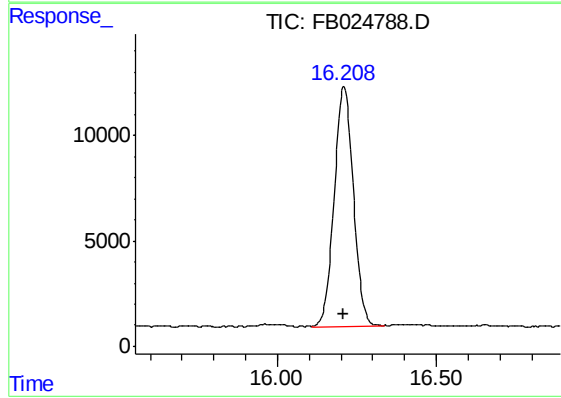

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 479526
Conc: 19.53 ng/ml