

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082420\
 Data File : FB024790.D
 Signal(s) : FID2B.CH
 Acq On : 24 Aug 2020 16:13
 Operator : DD/AJ
 Sample : L3780-10
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 25 00:54:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	388588	18.819 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.702	4063	0.169 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	1647	0.059 ng/ml
3) t	n-Heptane	7.753	707	0.026 ng/ml
4) t	Benzene	7.896	78522	2.237 ng/ml
6) t	Toluene	10.636	11547	0.335 ng/ml
7) t	Ethylbenzene	13.071	20306	0.634 ng/ml
8) t	m-Xylene	13.206	9067	0.291 ng/ml
9) t	O-Xylene	13.929	16815	0.556 ng/ml
10) t	1,2,4-Trimethylbenzene	16.224	6107	0.249 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082420\
Data File : FB024790.D
Signal(s) : FID2B.CH
Acq On : 24 Aug 2020 16:13
Operator : DD/AJ
Sample : L3780-10
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 25 00:54:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

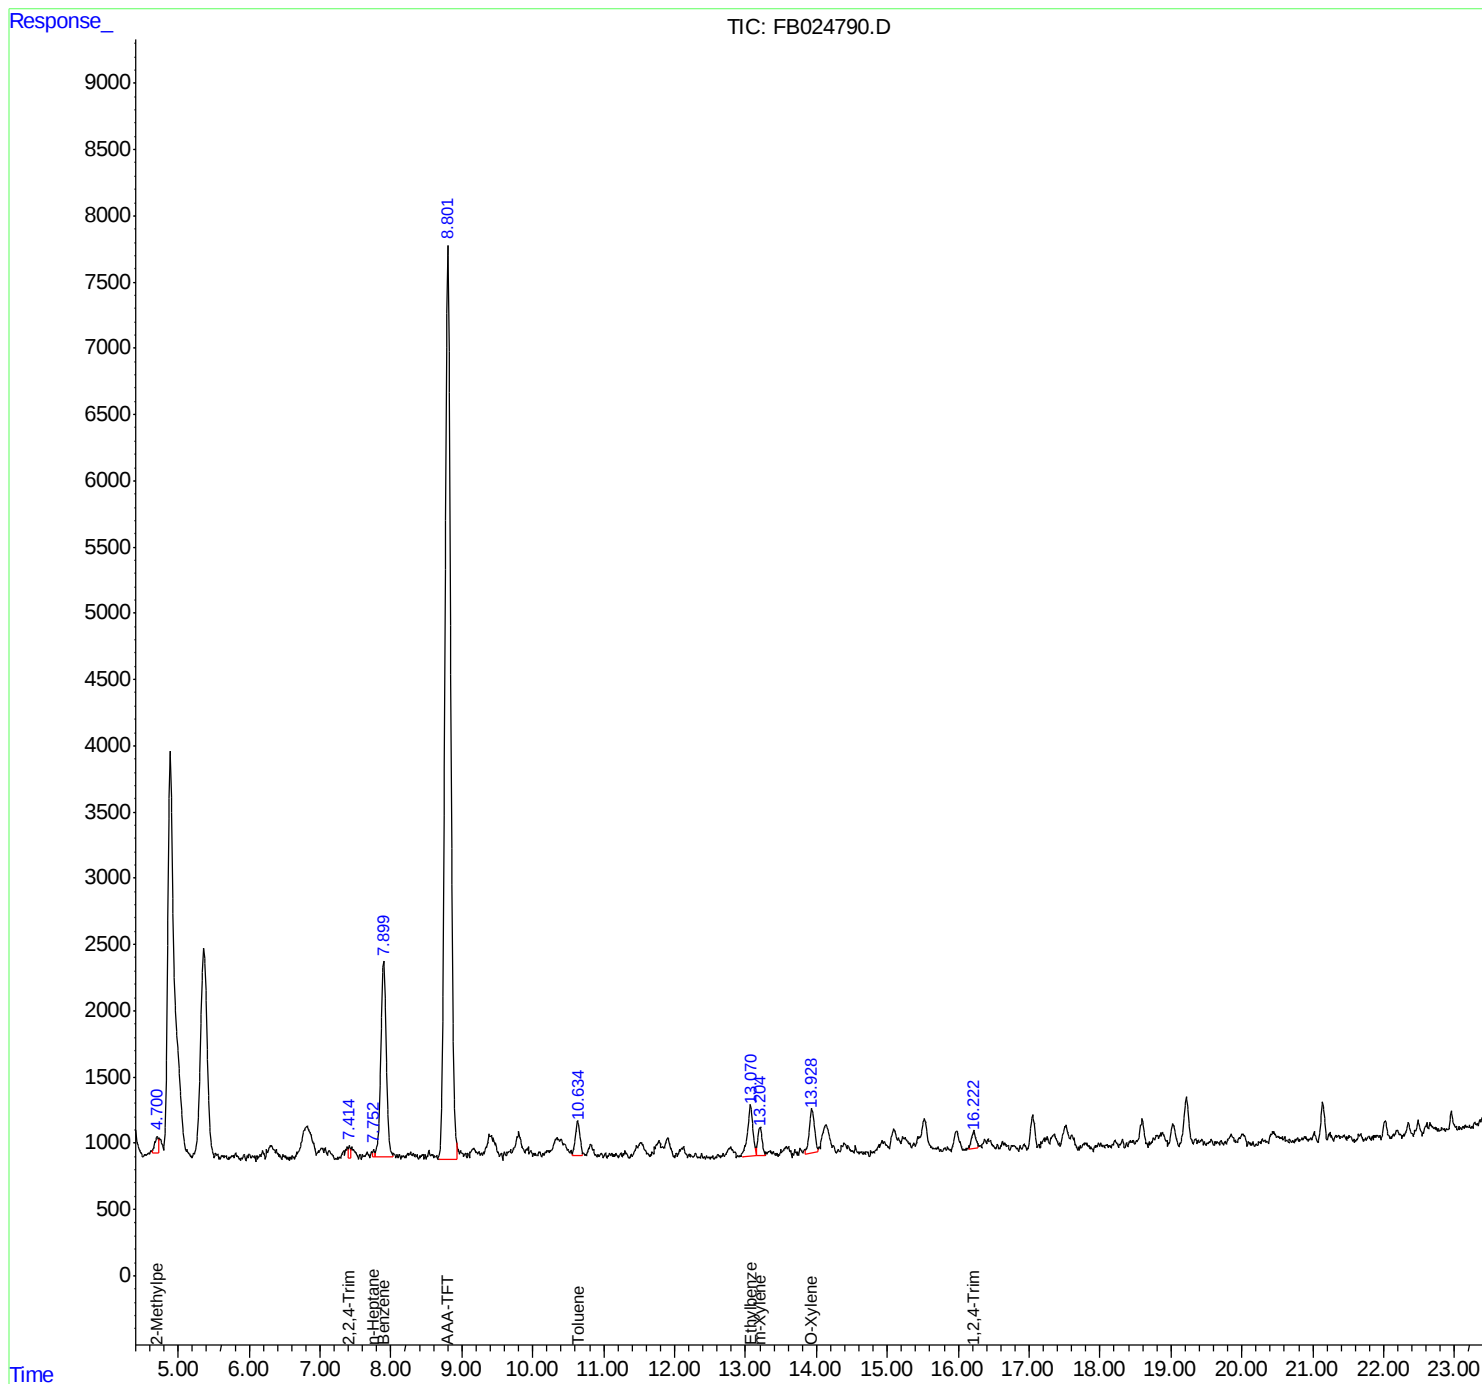

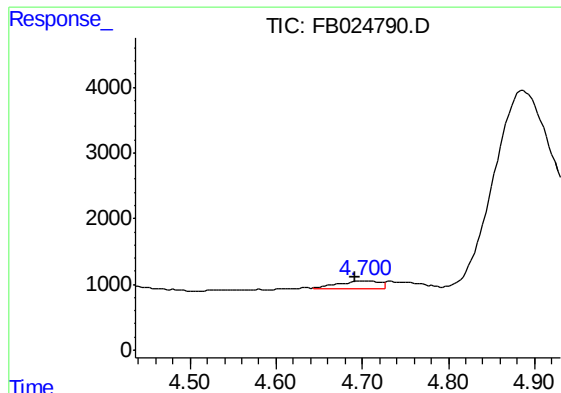


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: 0.011 min
Response: 4063
Conc: 0.17 ng/ml

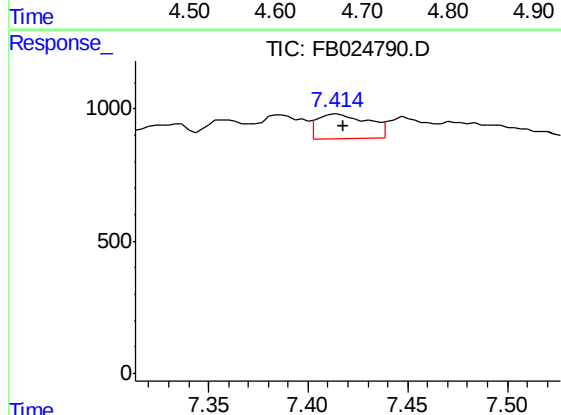


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 1647
Conc: 0.06 ng/ml

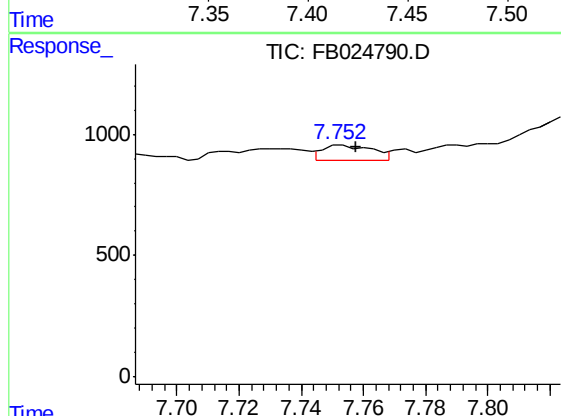


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.004 min
Response: 707
Conc: 0.03 ng/ml

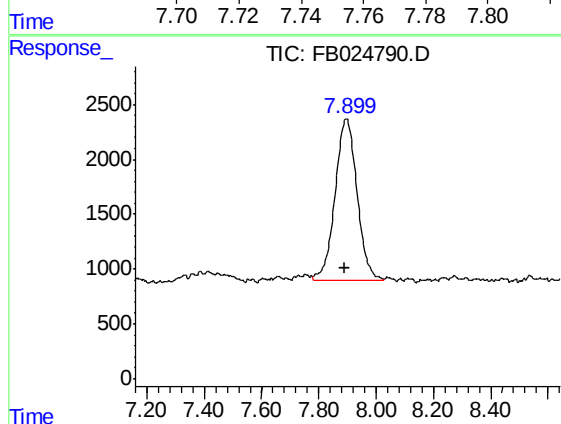


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.004 min
Response: 78522
Conc: 2.24 ng/ml

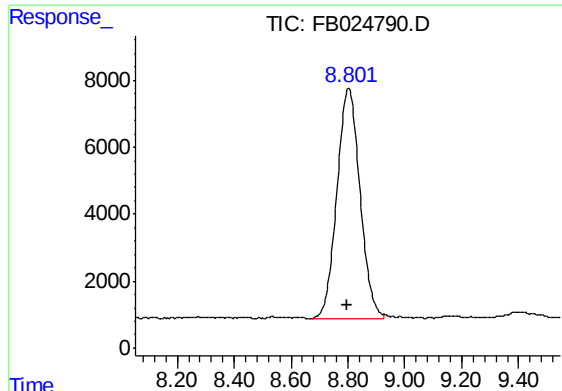


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 388588
Conc: 18.82 ng/ml

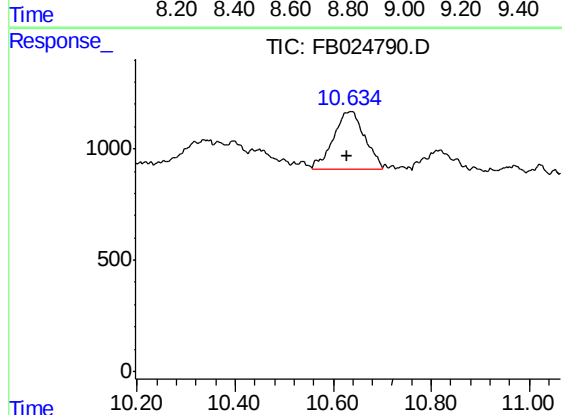


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.006 min
Response: 11547
Conc: 0.34 ng/ml

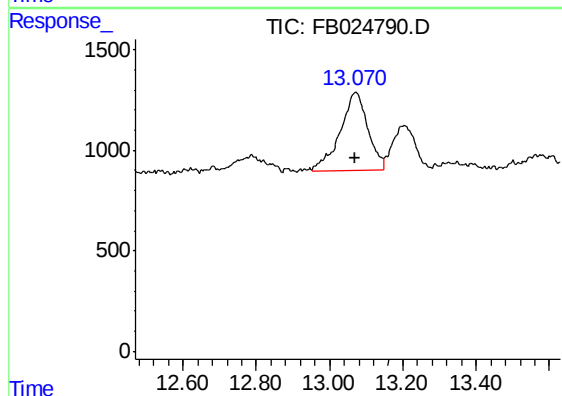


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.002 min
Response: 20306
Conc: 0.63 ng/ml

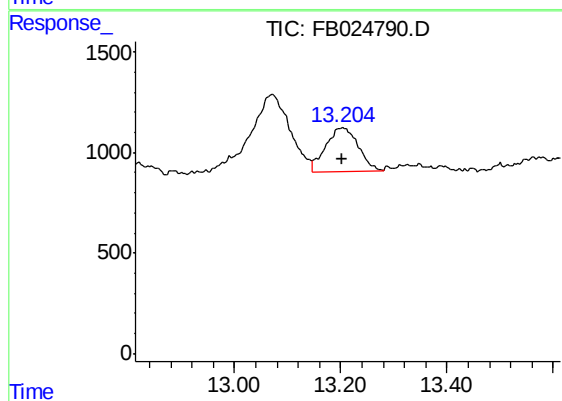


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.004 min
Response: 9067
Conc: 0.29 ng/ml

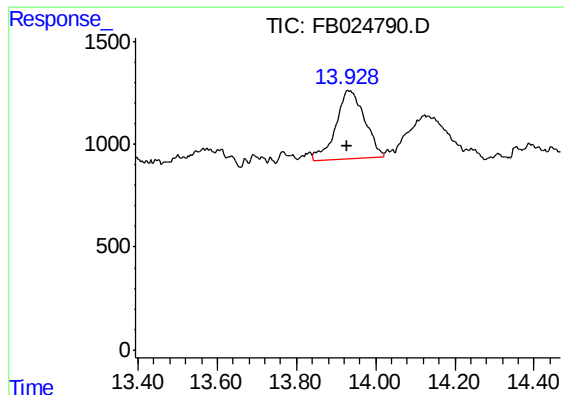

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 16815
Conc: 0.56 ng/ml

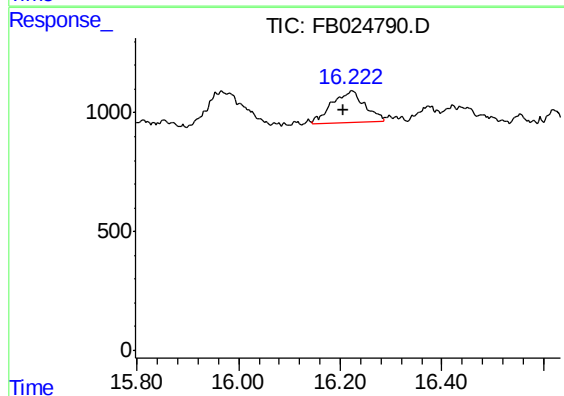

#10 1,2,4-Trimethylbenzene

R.T.: 16.224 min
Delta R.T.: 0.017 min
Response: 6107
Conc: 0.25 ng/ml