

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
 Data File : FB022176.D
 Signal(s) : FID2B.CH
 Acq On : 26 Aug 2019 9:53
 Operator : DD/AJ
 Sample : BSF0826S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0826S1

Integration File: Calibration.e
 Quant Time: Aug 27 01:10:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.981	431623	20.321 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.852	1184166	29.588 ng/ml
2) t 2,2,4-Trimethylpentane	7.600	1200036	29.794 ng/ml
3) t n-Heptane	7.940	381093	9.976 ng/ml
4) t Benzene	8.074	442021	9.846 ng/ml
6) t Toluene	10.821	899610	29.263 ng/ml
7) t Ethylbenzene	13.268	217996	10.683 ng/ml
8) t m-Xylene	13.400	459490	21.818 ng/ml
9) t O-Xylene	14.129	478908	21.413 ng/ml
10) t 1,2,4-Trimethylbenzene	16.409	530602	20.690 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
Data File : FB022176.D
Signal(s) : FID2B.CH
Acq On : 26 Aug 2019 9:53
Operator : DD/AJ
Sample : BSF0826S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0826S1

Integration File: Calibration.e
Quant Time: Aug 27 01:10:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

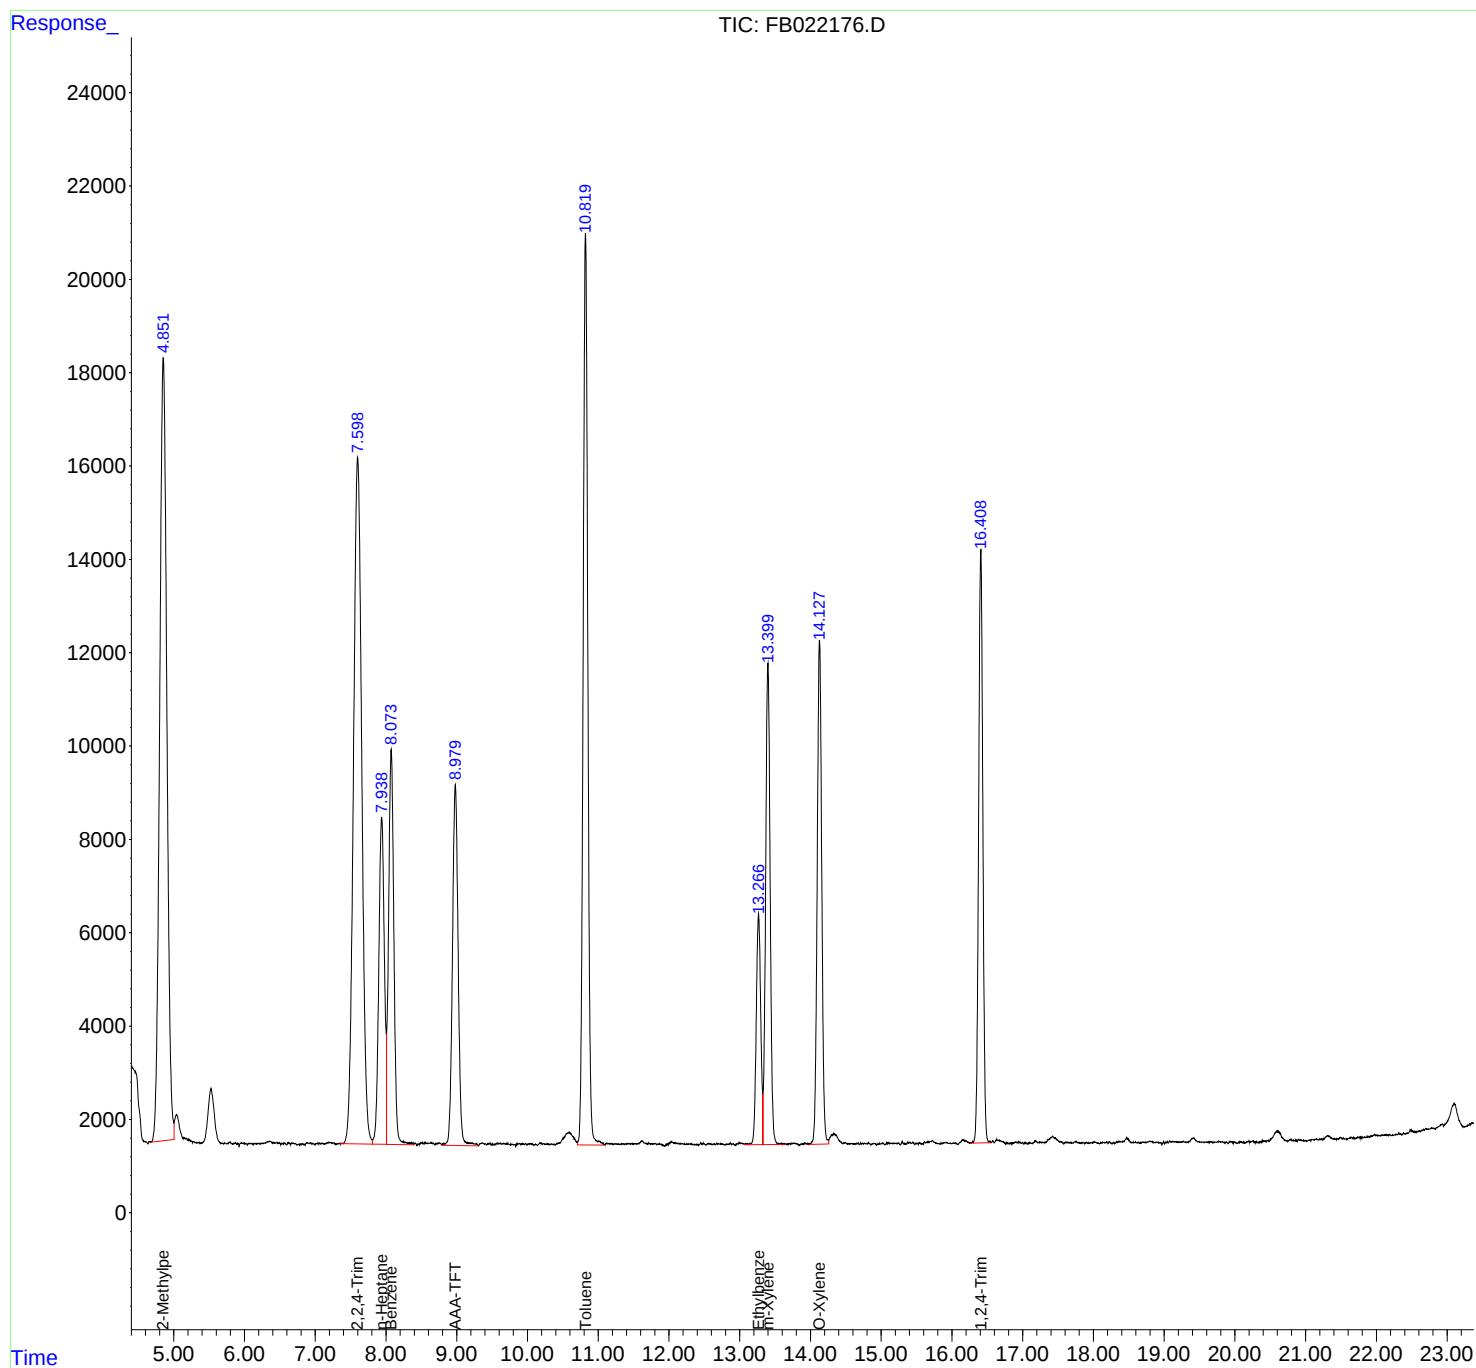


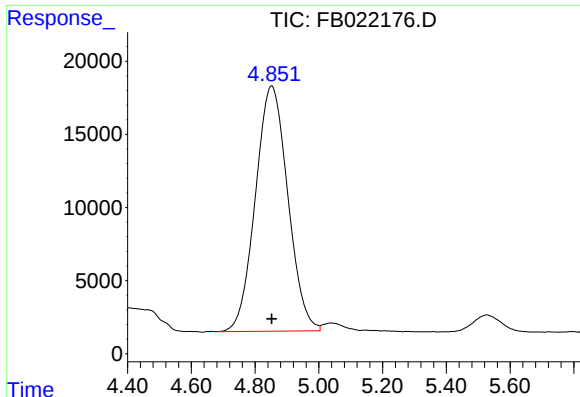

#1 2-Methylpentane


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 1184166
Conc: 29.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0826S1

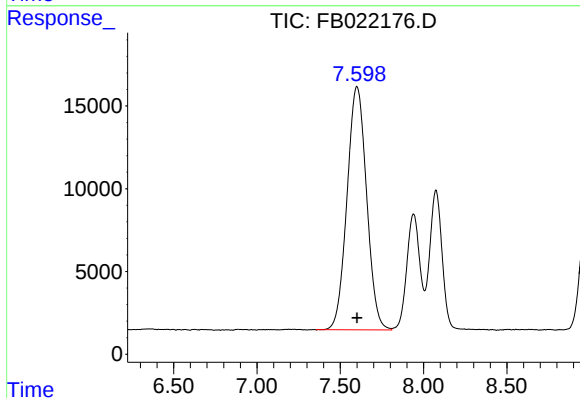


#2 2,2,4-Trimethylpentane

R.T.: 7.600 min
Delta R.T.: 0.000 min
Response: 1200036
Conc: 29.79 ng/ml

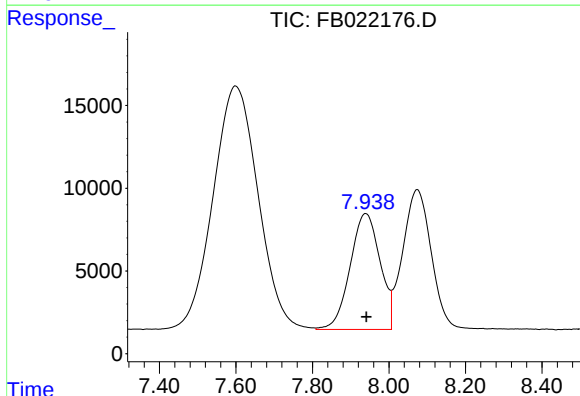


#3 n-Heptane

R.T.: 7.940 min
Delta R.T.: -0.001 min
Response: 381093
Conc: 9.98 ng/ml

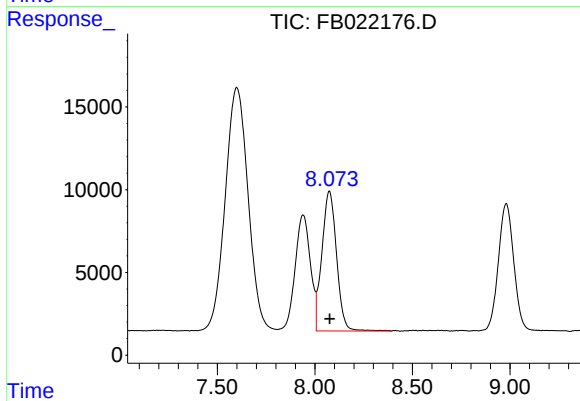

#4 Benzene


R.T.: 8.074 min
Delta R.T.: -0.002 min
Response: 442021
Conc: 9.85 ng/ml

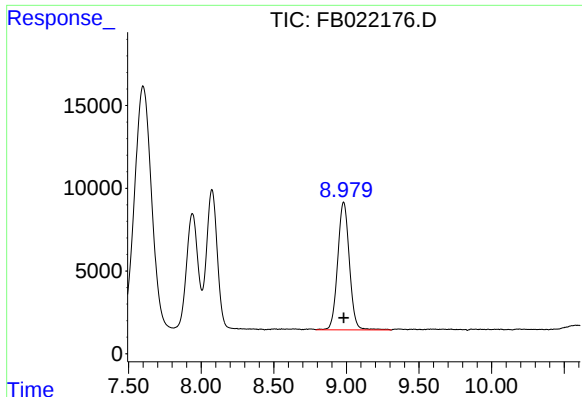

#5 AAA-TFT


R.T.: 8.981 min
Delta R.T.: -0.001 min
Response: 431623
Conc: 20.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0826S1

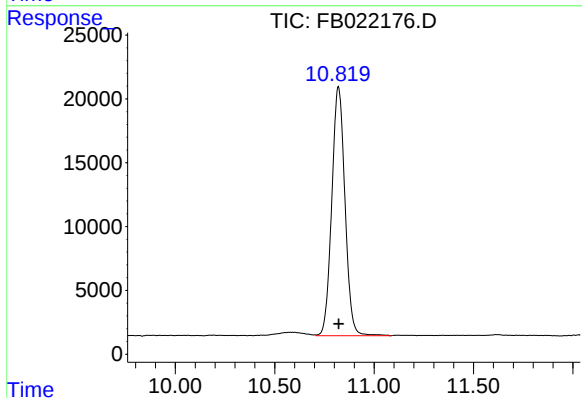


#6 Toluene

R.T.: 10.821 min
Delta R.T.: -0.002 min
Response: 899610
Conc: 29.26 ng/ml

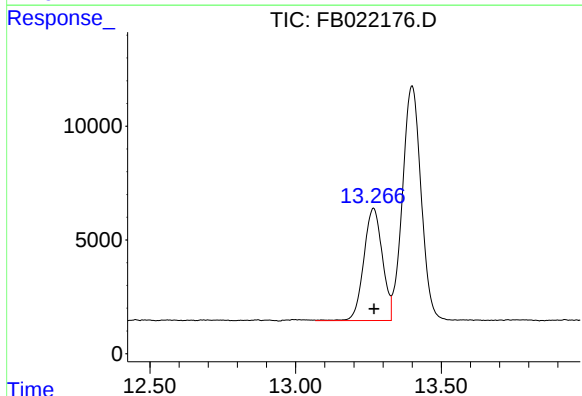


#7 Ethylbenzene

R.T.: 13.268 min
Delta R.T.: -0.002 min
Response: 217996
Conc: 10.68 ng/ml

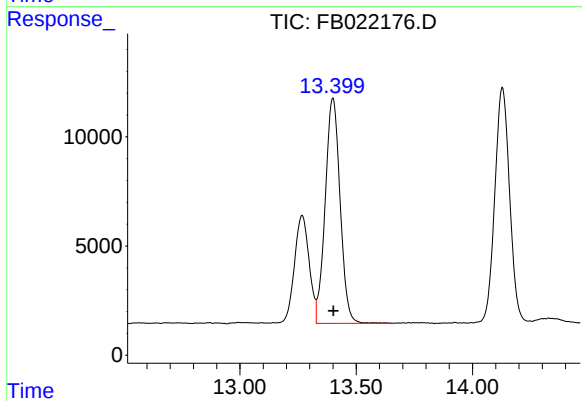

#8 m-Xylene

R.T.: 13.400 min
Delta R.T.: -0.002 min
Response: 459490
Conc: 21.82 ng/ml

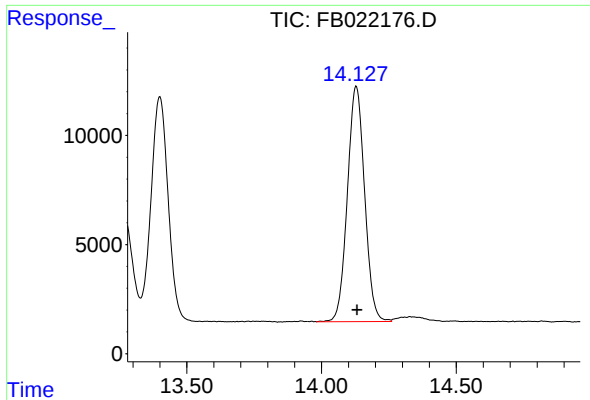

#9 O-Xylene


R.T.: 14.129 min

Delta R.T.: -0.003 min

Response: 478908

Conc: 21.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0826S1

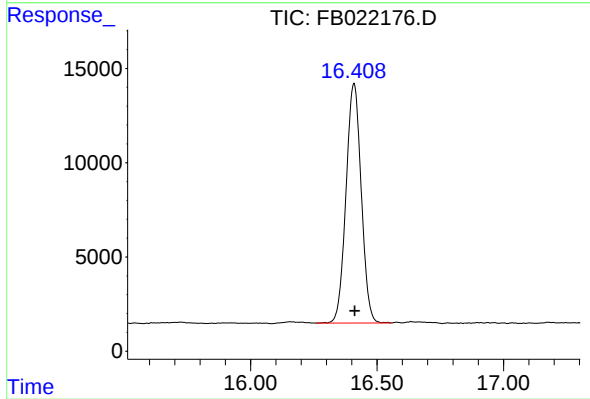

#10 1,2,4-Trimethylbenzene

R.T.: 16.409 min

Delta R.T.: -0.003 min

Response: 530602

Conc: 20.69 ng/ml