

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082619\  
Data File : FB022192.D  
Signal(s) : FID2B.CH  
Acq On : 26 Aug 2019 17:59  
Operator : DD/AJ  
Sample : K4461-08  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP

Integration File: Calibration.e  
Quant Time: Aug 27 01:14:21 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.987  | 502244   | 23.646 ng/ml |
| Target Compounds            |        |          |              |
| 6) t Toluene                | 10.847 | 3406     | 0.111 ng/ml  |
| 7) t Ethylbenzene           | 13.210 | 1218     | 0.060 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082619\  
Data File : FB022192.D  
Signal(s) : FID2B.CH  
Acq On : 26 Aug 2019 17:59  
Operator : DD/AJ  
Sample : K4461-08  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP

Integration File: Calibration.e  
Quant Time: Aug 27 01:14:21 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

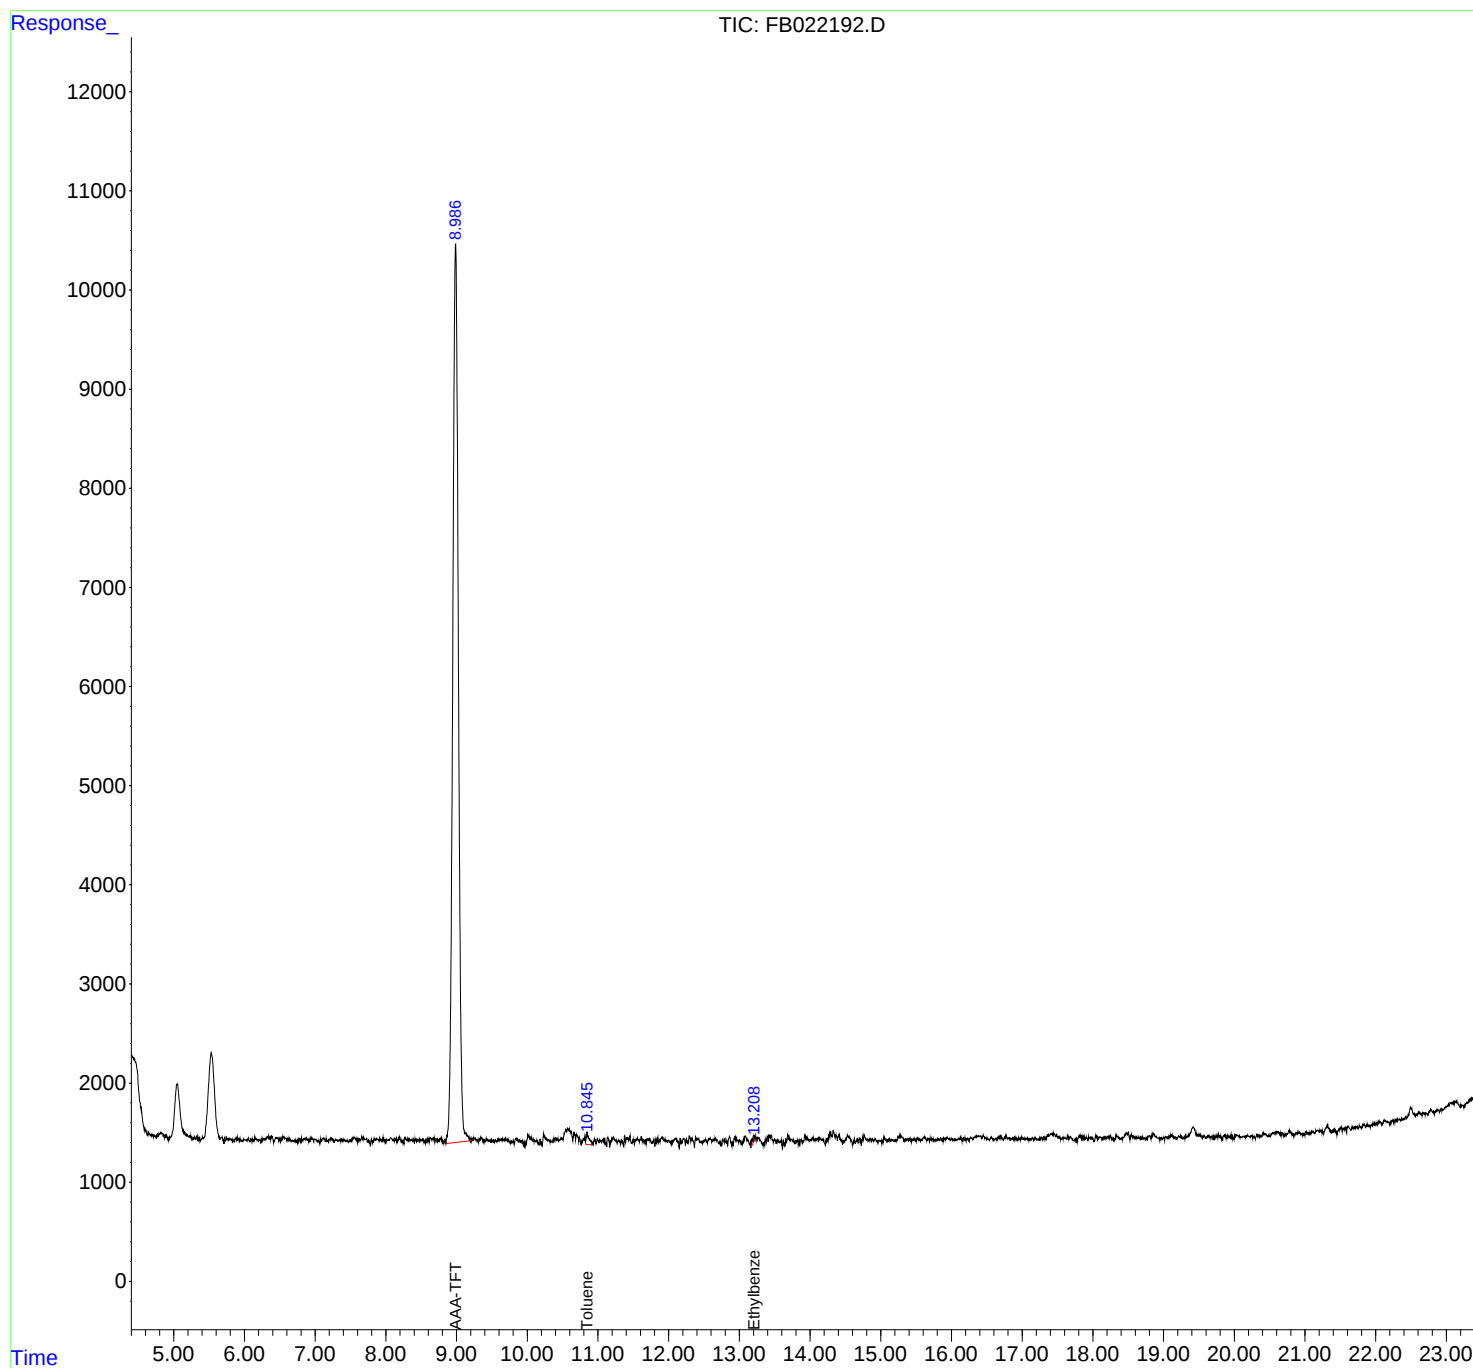


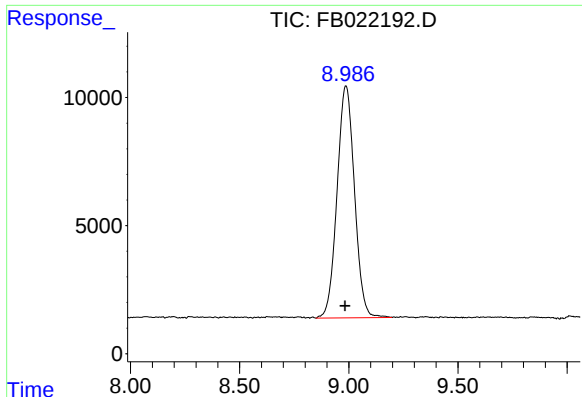

#5 AAA-TFT


R.T.: 8.987 min  
Delta R.T.: 0.005 min  
Response: 502244  
Conc: 23.65 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP

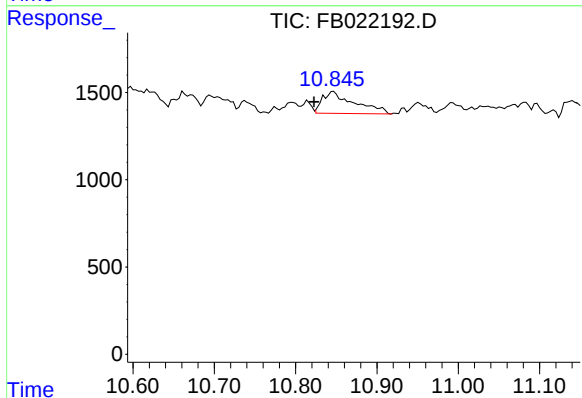

#6 Toluene

R.T.: 10.847 min  
Delta R.T.: 0.024 min  
Response: 3406  
Conc: 0.11 ng/ml

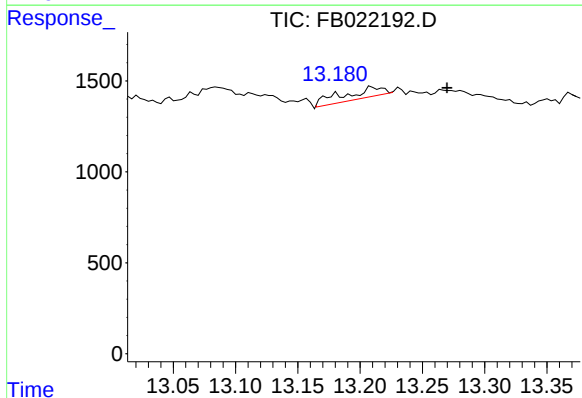

#7 Ethylbenzene

R.T.: 13.210 min  
Delta R.T.: -0.059 min  
Response: 1218  
Conc: 0.06 ng/ml