

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
 Data File : FB022188.D
 Signal(s) : FID2B.CH
 Acq On : 26 Aug 2019 15:57
 Operator : DD/AJ
 Sample : K4514-03MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S602-M-1.0-1.5-082319MS

Integration File: Calibration.e
 Quant Time: Aug 27 01:13:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.985	437282	20.587 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.854	1054076	26.337 ng/ml
2) t	2,2,4-Trimethylpentane	7.603	841684	20.897 ng/ml
3) t	n-Heptane	7.943	263640	6.902 ng/ml
4) t	Benzene	8.079	425072	9.468 ng/ml
6) t	Toluene	10.826	835852	27.189 ng/ml
7) t	Ethylbenzene	13.272	200308	9.816 ng/ml
8) t	m-Xylene	13.405	429114	20.375 ng/ml
9) t	O-Xylene	14.134	453202	20.264 ng/ml
10) t	1,2,4-Trimethylbenzene	16.413	468247	18.258 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
Data File : FB022188.D
Signal(s) : FID2B.CH
Acq On : 26 Aug 2019 15:57
Operator : DD/AJ
Sample : K4514-03MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MS

Integration File: Calibration.e
Quant Time: Aug 27 01:13:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

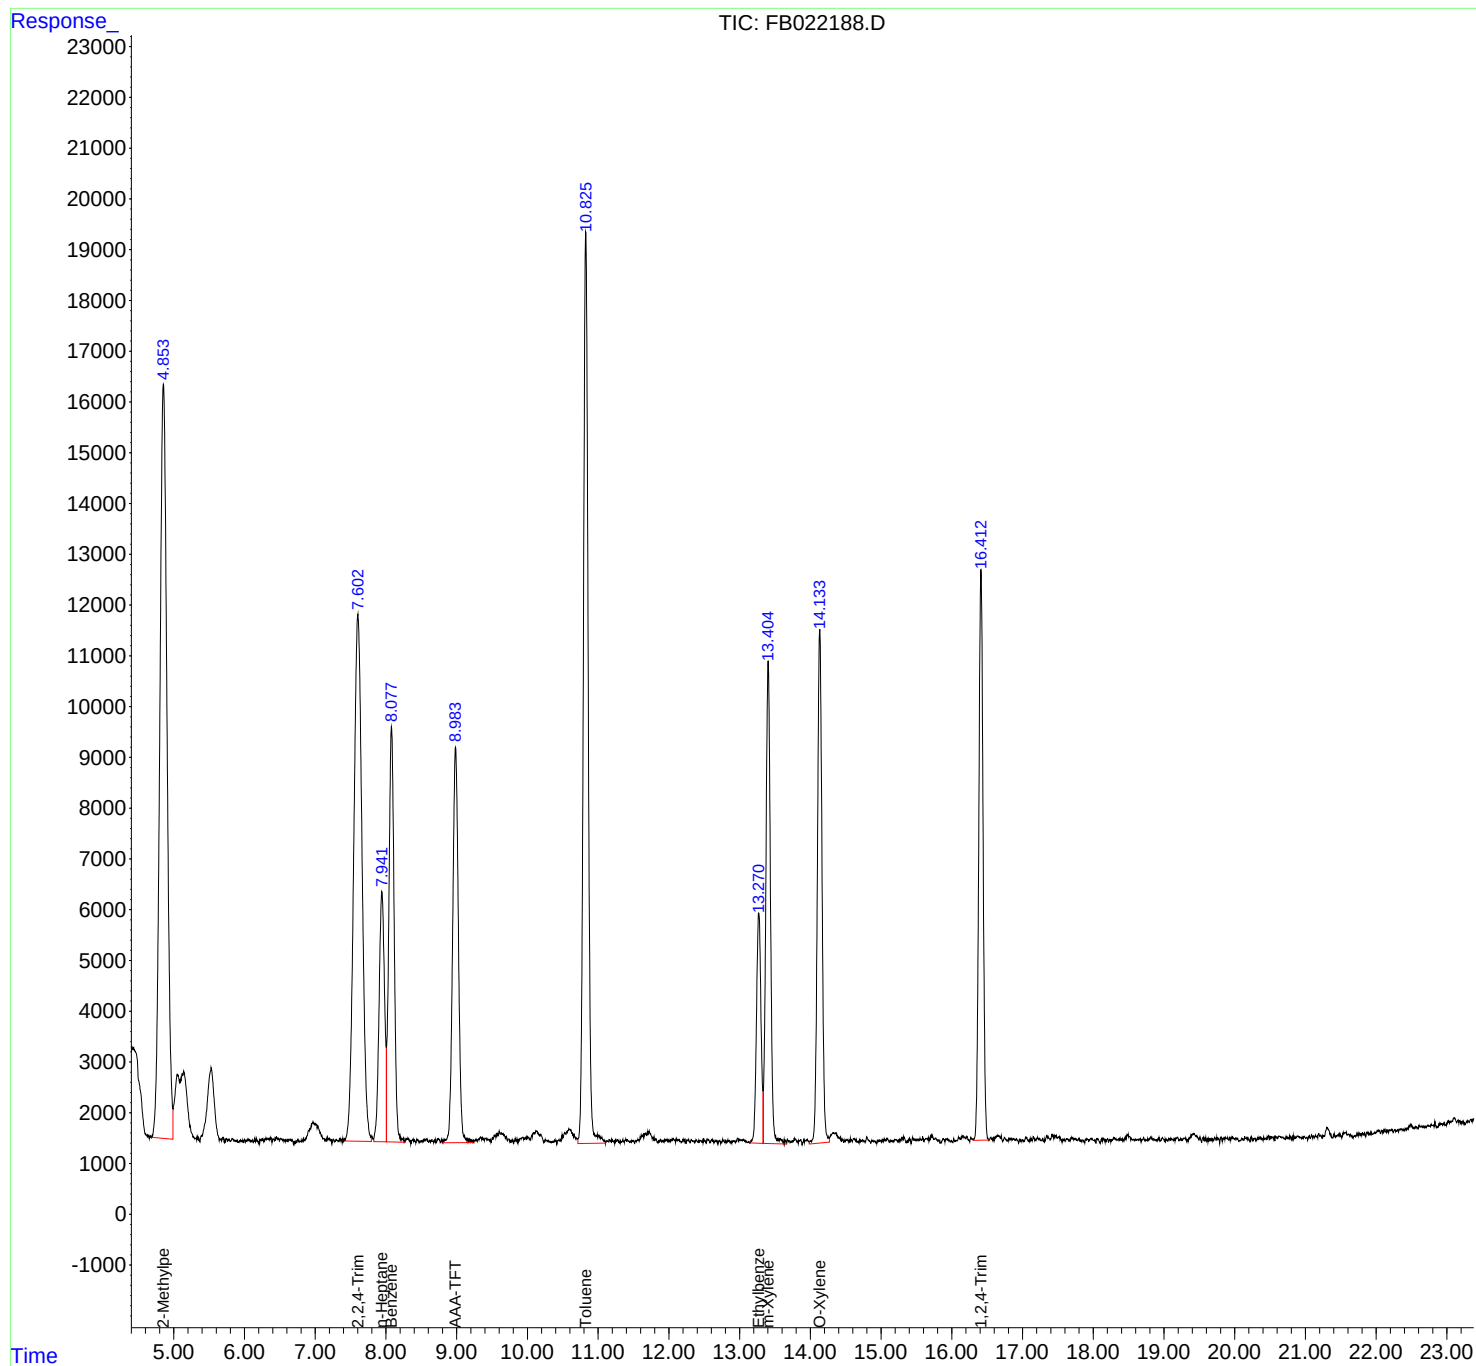


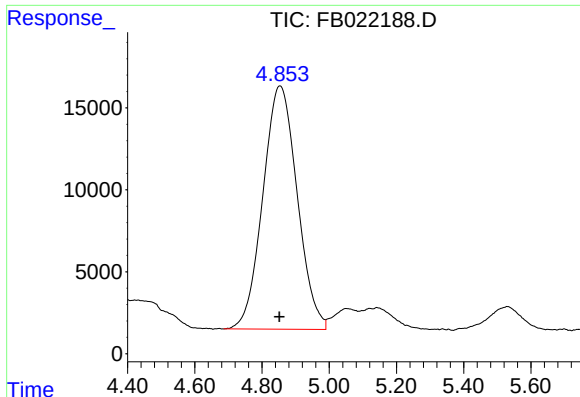

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: 0.002 min
Response: 1054076
Conc: 26.34 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MS

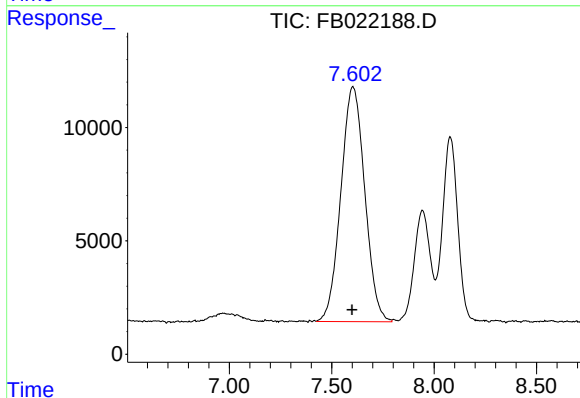


#2 2,2,4-Trimethylpentane

R.T.: 7.603 min
Delta R.T.: 0.004 min
Response: 841684
Conc: 20.90 ng/ml

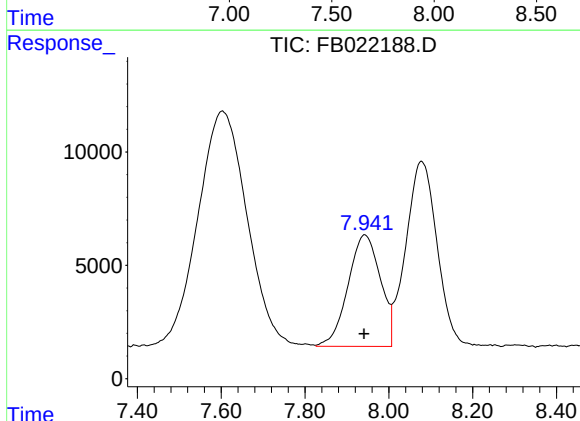


#3 n-Heptane

R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 263640
Conc: 6.90 ng/ml

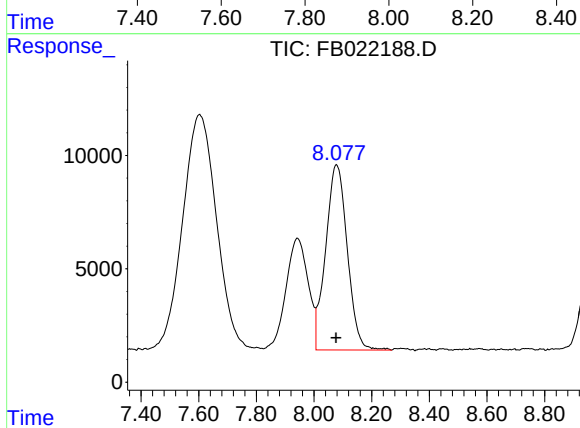

#4 Benzene


R.T.: 8.079 min
Delta R.T.: 0.003 min
Response: 425072
Conc: 9.47 ng/ml

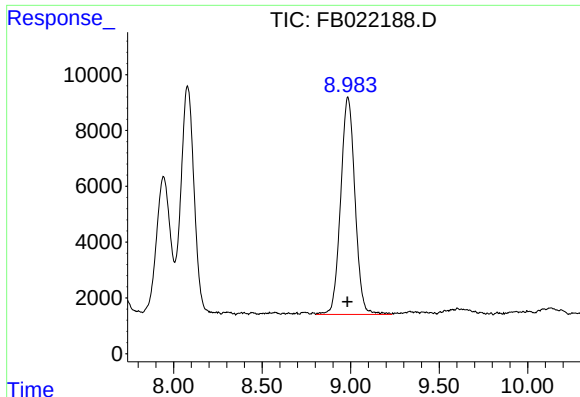

#5 AAA-TFT


R.T.: 8.985 min
Delta R.T.: 0.002 min
Response: 437282
Conc: 20.59 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MS

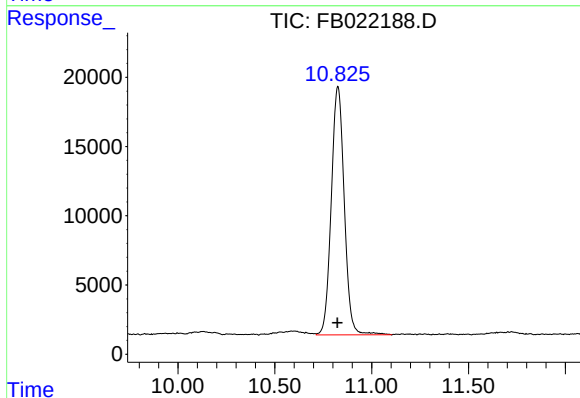


#6 Toluene

R.T.: 10.826 min
Delta R.T.: 0.003 min
Response: 835852
Conc: 27.19 ng/ml

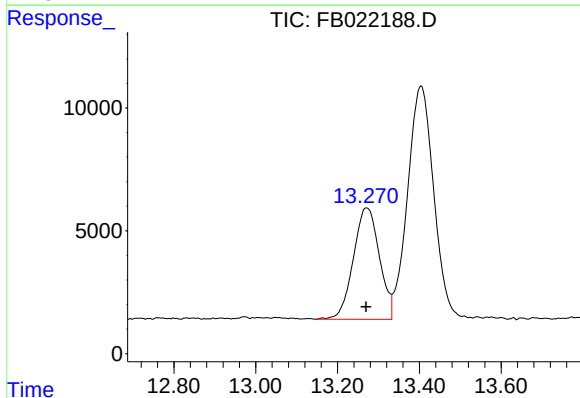


#7 Ethylbenzene

R.T.: 13.272 min
Delta R.T.: 0.002 min
Response: 200308
Conc: 9.82 ng/ml

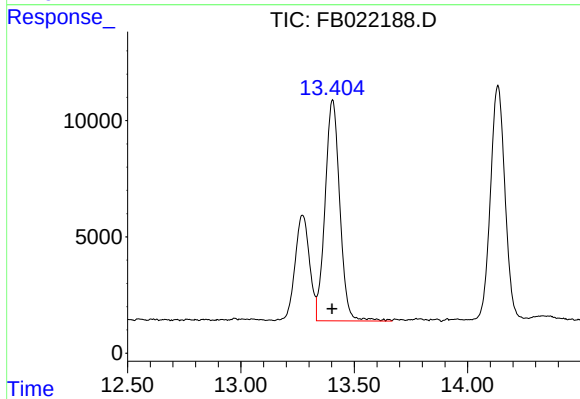

#8 m-Xylene

R.T.: 13.405 min
Delta R.T.: 0.003 min
Response: 429114
Conc: 20.38 ng/ml

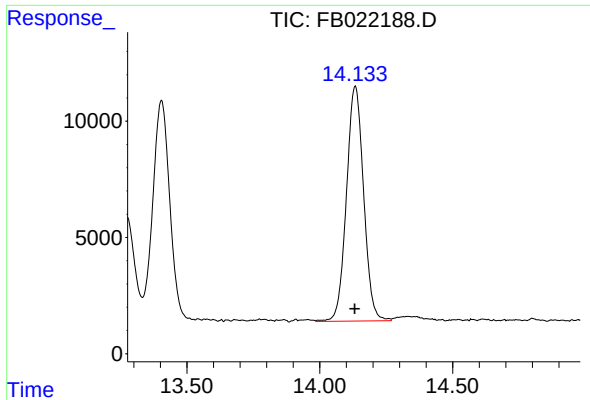

#9 O-Xylene


R.T.: 14.134 min

Delta R.T.: 0.002 min

Response: 453202

Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MS

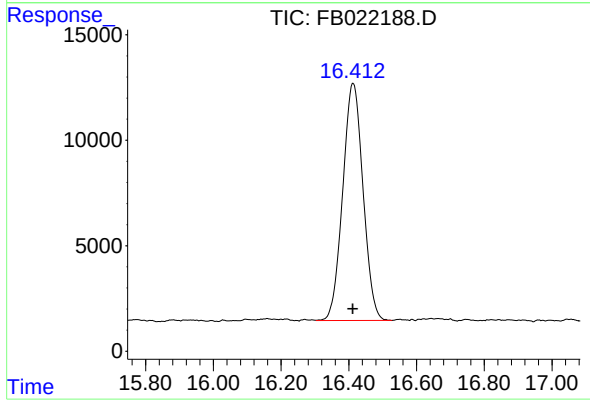

#10 1,2,4-Trimethylbenzene

R.T.: 16.413 min

Delta R.T.: 0.002 min

Response: 468247

Conc: 18.26 ng/ml