

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
 Data File : FB022189.D
 Signal(s) : FID2B.CH
 Acq On : 26 Aug 2019 16:28
 Operator : DD/AJ
 Sample : K4514-04MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S602-M-1.0-1.5-082319MSD

Integration File: Calibration.e
 Quant Time: Aug 27 01:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	393769	18.539 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	888675	22.204 ng/ml
2) t 2,2,4-Trimethylpentane	7.604	757321	18.802 ng/ml
3) t n-Heptane	7.944	231006	6.047 ng/ml
4) t Benzene	8.080	389238	8.670 ng/ml
6) t Toluene	10.826	783711	25.493 ng/ml
7) t Ethylbenzene	13.273	184080	9.021 ng/ml
8) t m-Xylene	13.405	371903	17.659 ng/ml
9) t O-Xylene	14.135	400453	17.905 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	434473	16.941 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082619\
Data File : FB022189.D
Signal(s) : FID2B.CH
Acq On : 26 Aug 2019 16:28
Operator : DD/AJ
Sample : K4514-04MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MSD

Integration File: Calibration.e
Quant Time: Aug 27 01:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

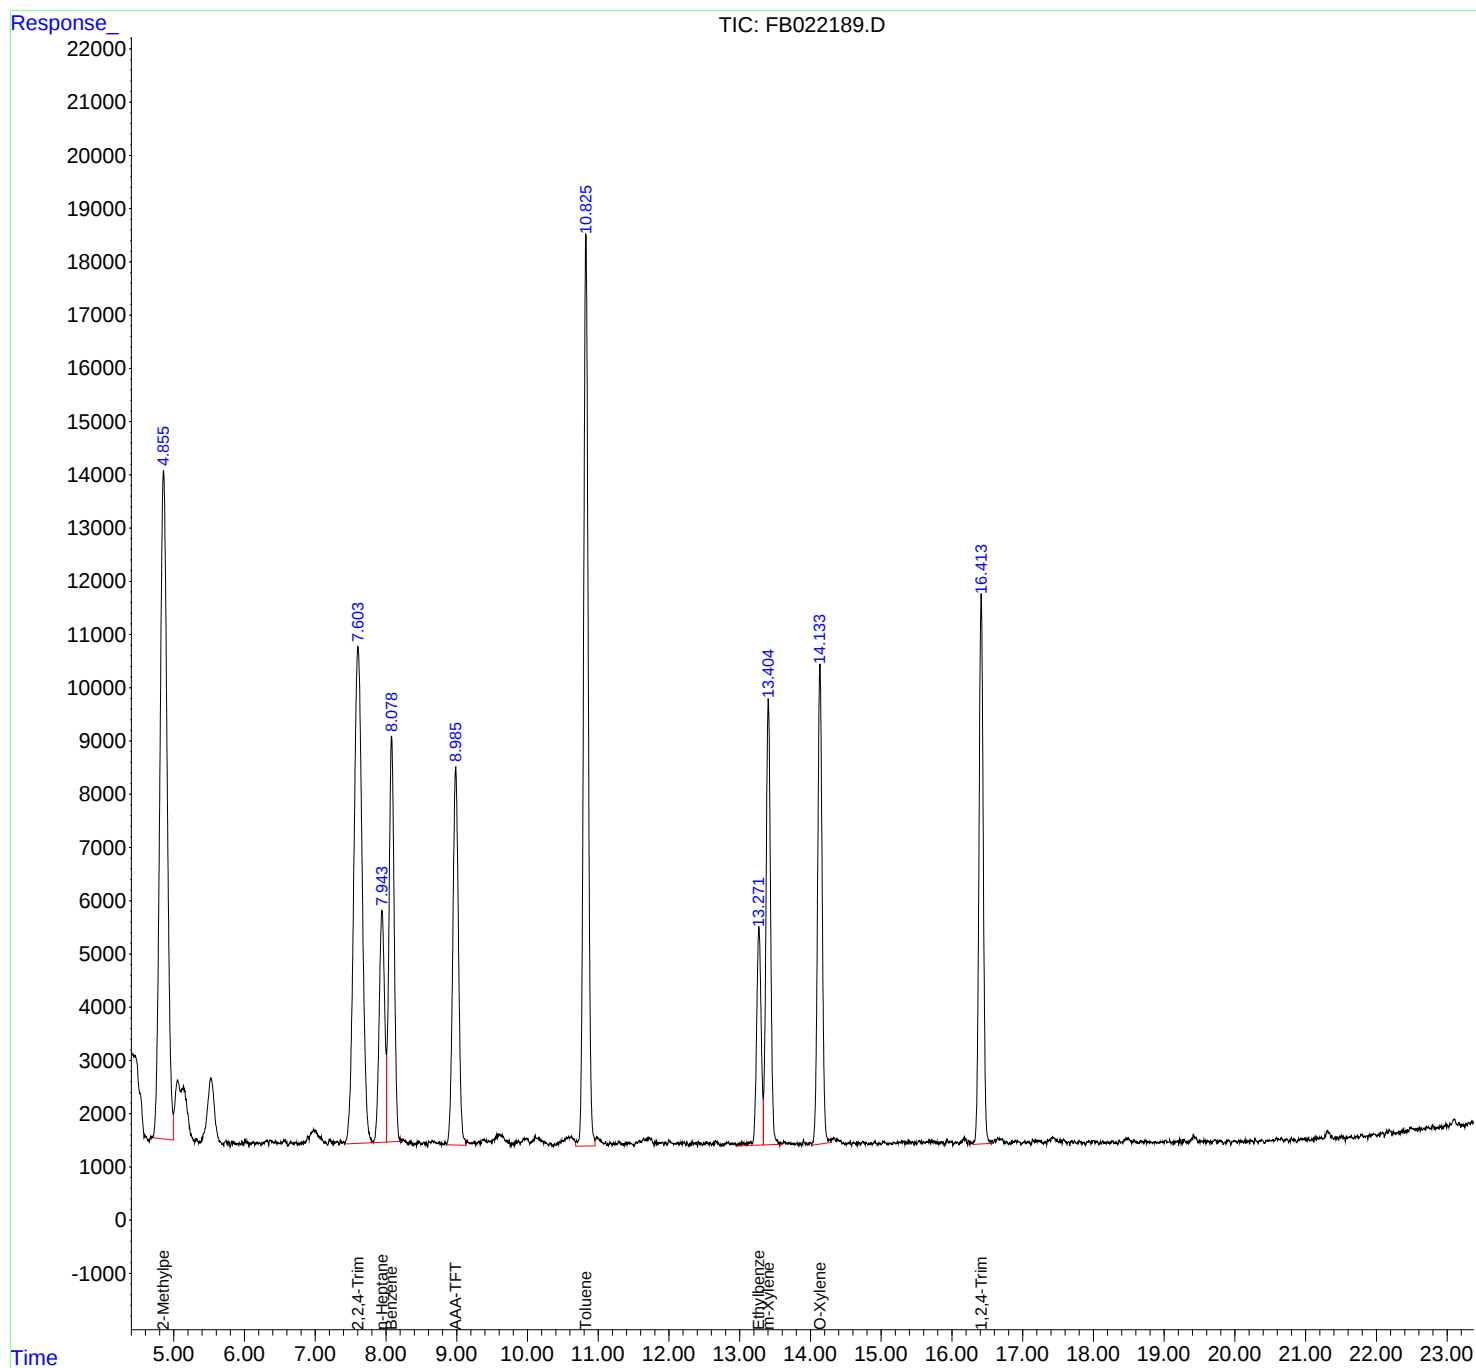


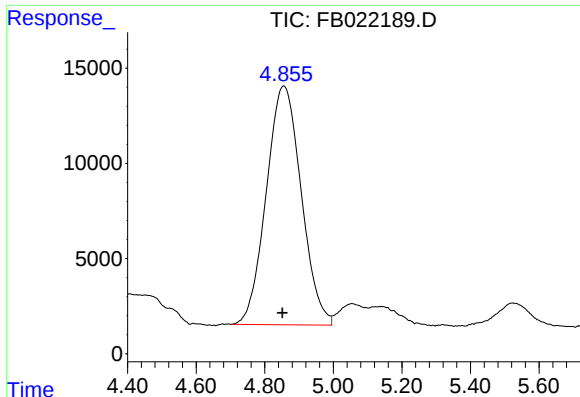

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 888675
Conc: 22.20 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MSD

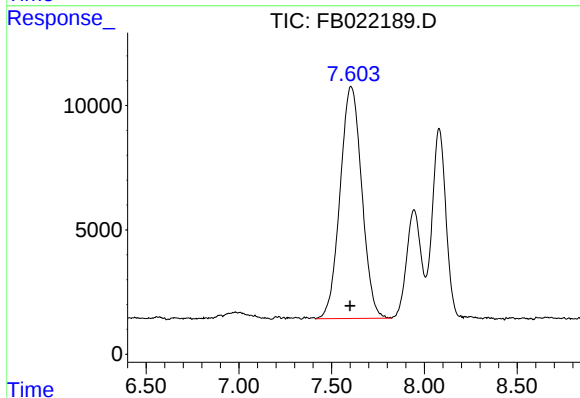


#2 2,2,4-Trimethylpentane

R.T.: 7.604 min
Delta R.T.: 0.005 min
Response: 757321
Conc: 18.80 ng/ml

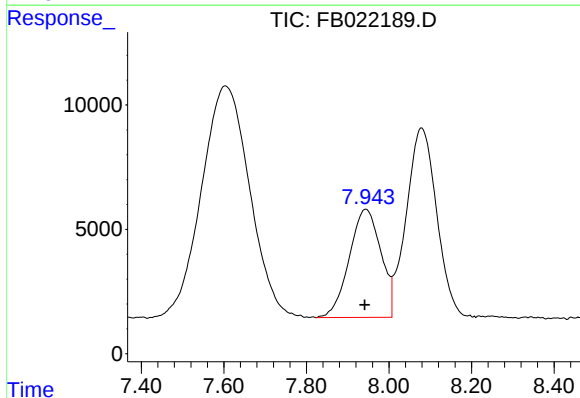


#3 n-Heptane

R.T.: 7.944 min
Delta R.T.: 0.003 min
Response: 231006
Conc: 6.05 ng/ml

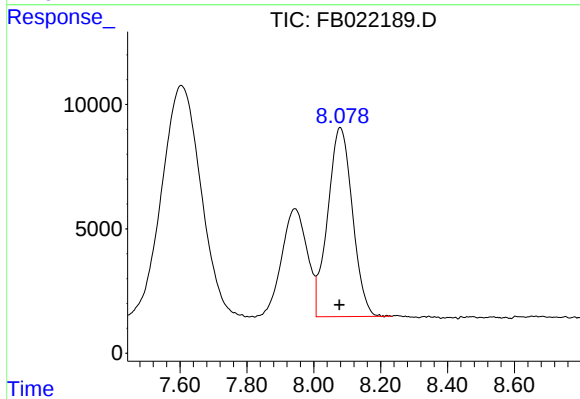

#4 Benzene


R.T.: 8.080 min
Delta R.T.: 0.003 min
Response: 389238
Conc: 8.67 ng/ml

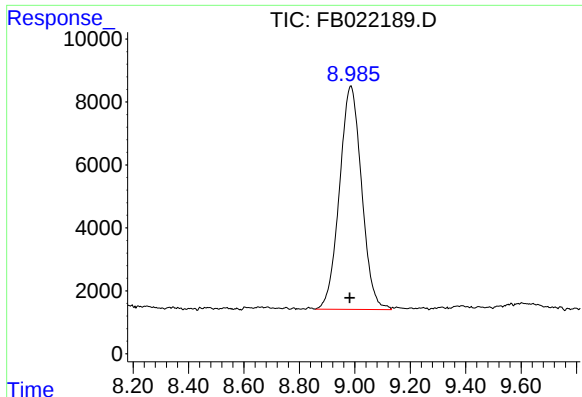

#5 AAA-TFT


R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 393769
Conc: 18.54 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MSD

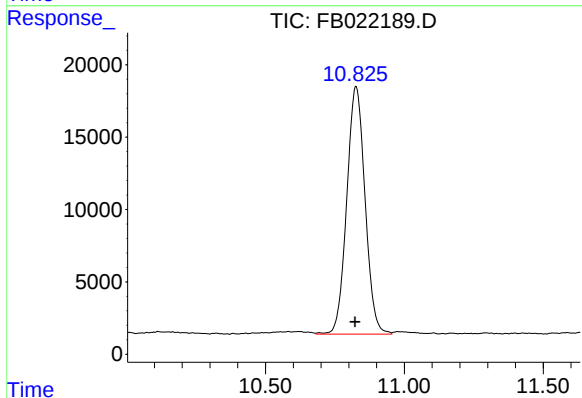


#6 Toluene

R.T.: 10.826 min
Delta R.T.: 0.004 min
Response: 783711
Conc: 25.49 ng/ml

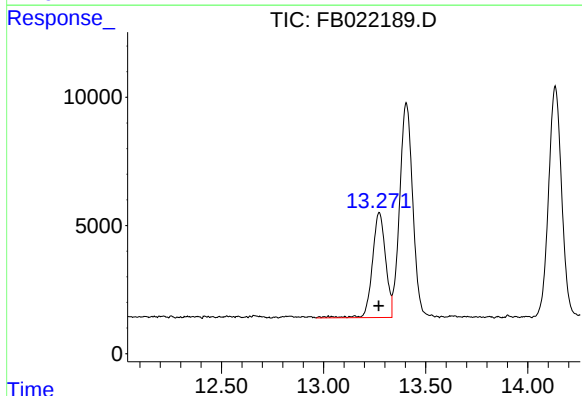


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.003 min
Response: 184080
Conc: 9.02 ng/ml

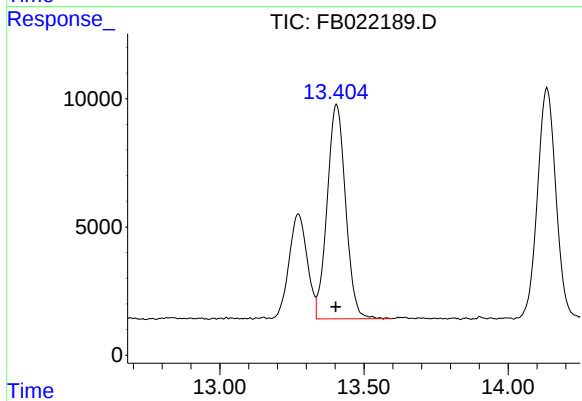

#8 m-Xylene


R.T.: 13.405 min
Delta R.T.: 0.004 min
Response: 371903
Conc: 17.66 ng/ml

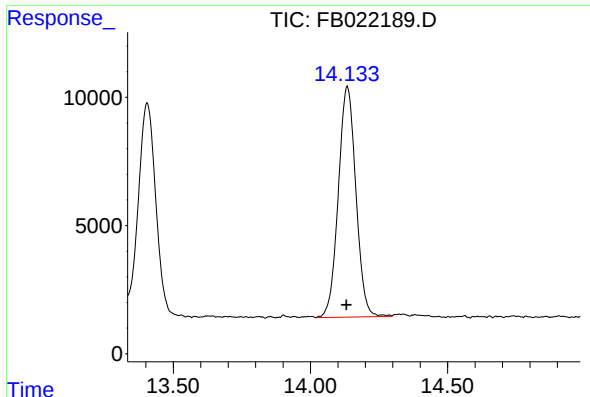

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.003 min
Response: 400453
Conc: 17.91 ng/ml

Instrument :
FID_B
ClientSampleId :
S602-M-1.0-1.5-082319MSD

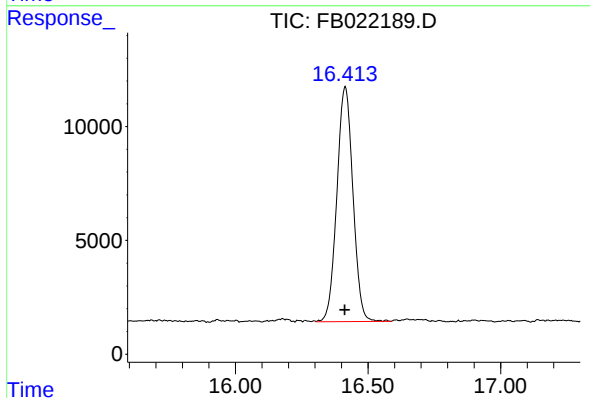

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.003 min
Response: 434473
Conc: 16.94 ng/ml