

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082718\
 Data File : FB017544.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2018 9:57
 Operator : MJ/SJ
 Sample : BSF0827S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 27 13:38:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.108	159130	19.301 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	356900	25.471 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	310145	22.009 ng/ml
3) t n-Heptane	8.066	95897	6.958 ng/ml
4) t Benzene	8.204	163958	9.300 ng/ml
6) t Toluene	10.957	386862	26.892 ng/ml
7) t Ethylbenzene	13.408	132834	9.007 ng/ml
8) t m-Xylene	13.540	282324	18.161 ng/ml
9) t O-Xylene	14.272	296004	18.032 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	324930	16.683 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082718\
Data File : FB017544.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2018 9:57
Operator : MJ/SJ
Sample : BSF0827S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 27 13:38:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

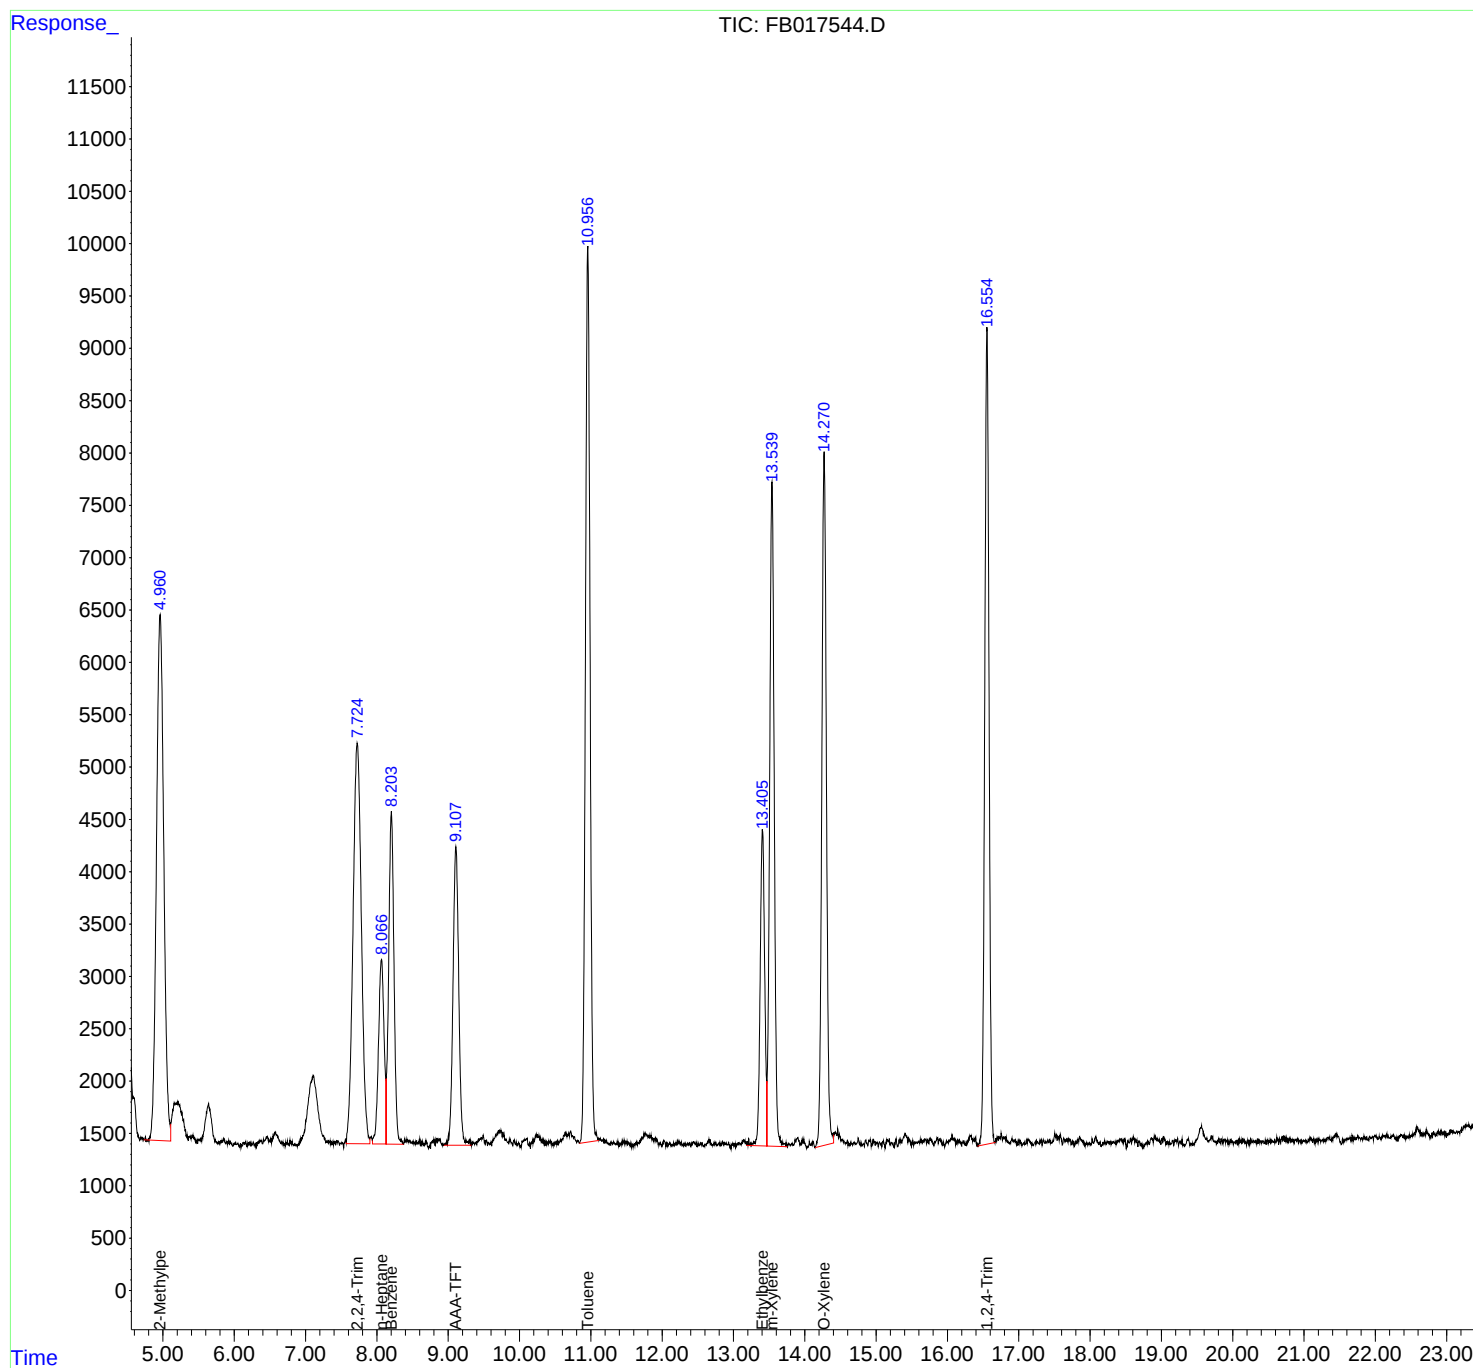

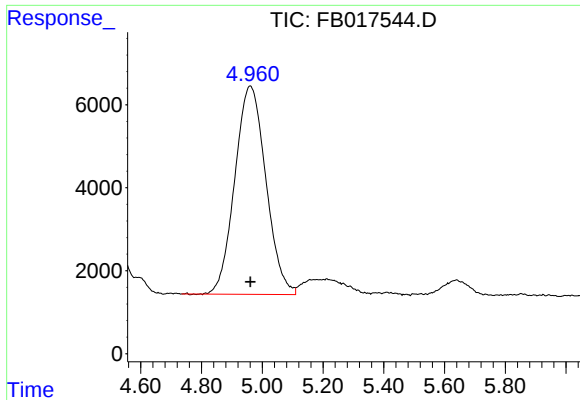


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 356900
Conc: 25.47 ng/ml

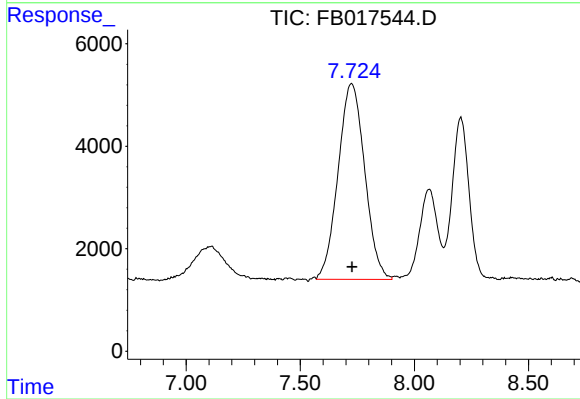


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 310145
Conc: 22.01 ng/ml

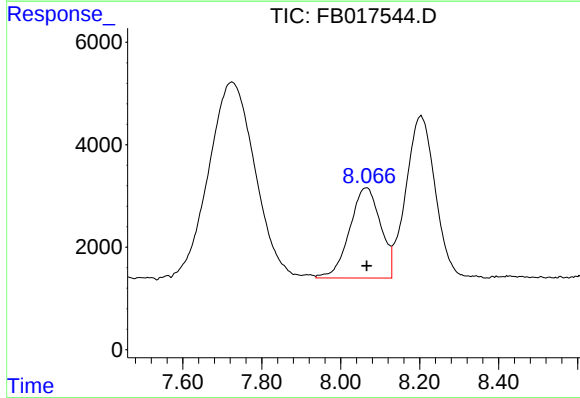


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 95897
Conc: 6.96 ng/ml

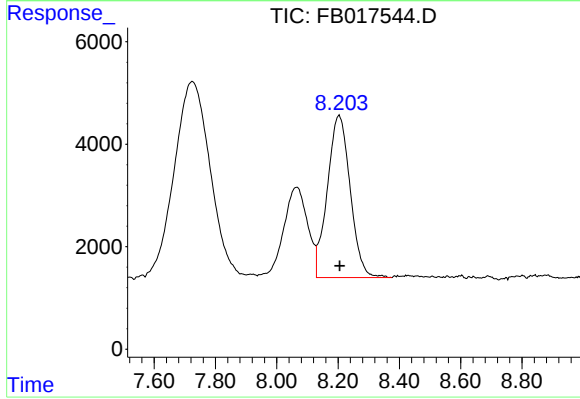


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.002 min
Response: 163958
Conc: 9.30 ng/ml

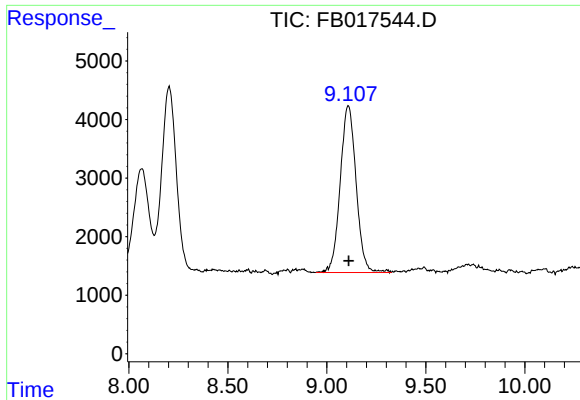


#5 AAA-TFT

R.T.: 9.108 min
Delta R.T.: -0.003 min
Response: 159130
Conc: 19.30 ng/ml

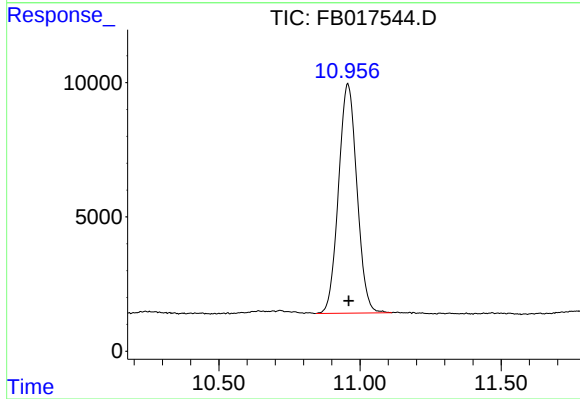


#6 Toluene

R.T.: 10.957 min
Delta R.T.: -0.003 min
Response: 386862
Conc: 26.89 ng/ml

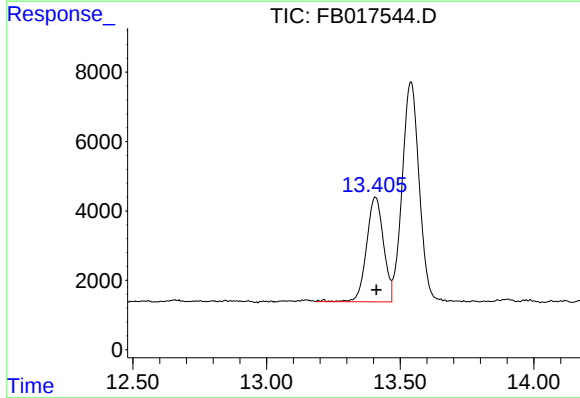


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 132834
Conc: 9.01 ng/ml

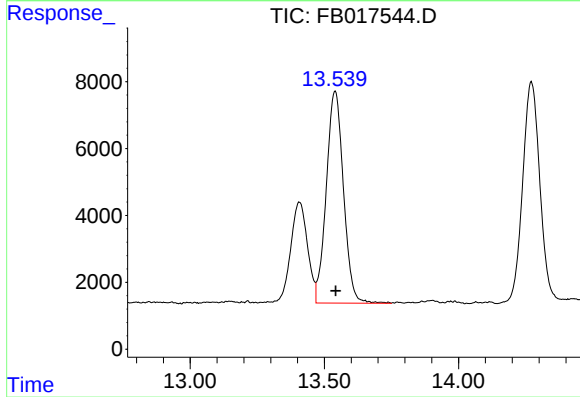


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.002 min
Response: 282324
Conc: 18.16 ng/ml

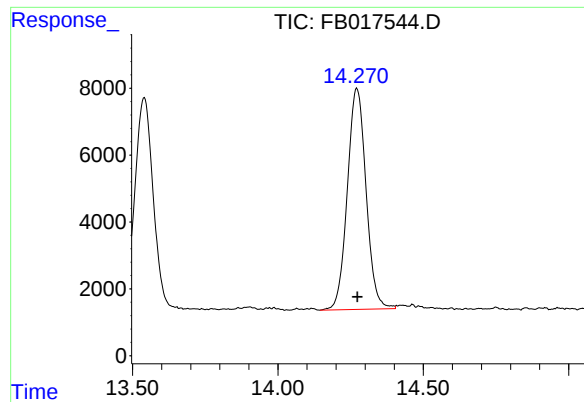

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 296004
Conc: 18.03 ng/ml

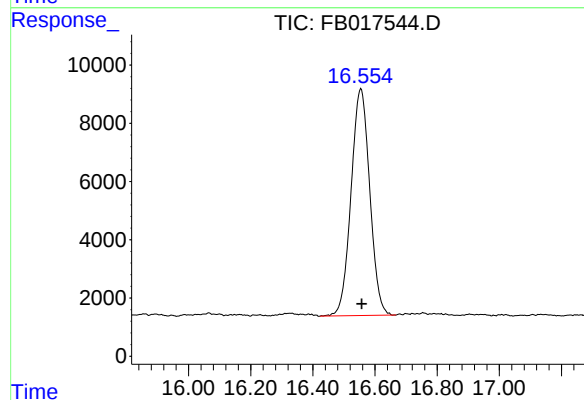

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min
Delta R.T.: -0.003 min
Response: 324930
Conc: 16.68 ng/ml