

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022200.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 9:12
 Operator : DD/AJ
 Sample : BSF0827S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0827S1

Integration File: Calibration.e
 Quant Time: Aug 27 23:15:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.982	437764	20.610 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	1215437	30.369 ng/ml
2) t 2,2,4-Trimethylpentane	7.602	1214835	30.161 ng/ml
3) t n-Heptane	7.941	385250	10.085 ng/ml
4) t Benzene	8.076	444086	9.892 ng/ml
6) t Toluene	10.823	912121	29.670 ng/ml
7) t Ethylbenzene	13.268	222220	10.890 ng/ml
8) t m-Xylene	13.401	462485	21.960 ng/ml
9) t O-Xylene	14.130	486053	21.733 ng/ml
10) t 1,2,4-Trimethylbenzene	16.410	536464	20.918 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022200.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 9:12
Operator : DD/AJ
Sample : BSF0827S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0827S1

Integration File: Calibration.e
Quant Time: Aug 27 23:15:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

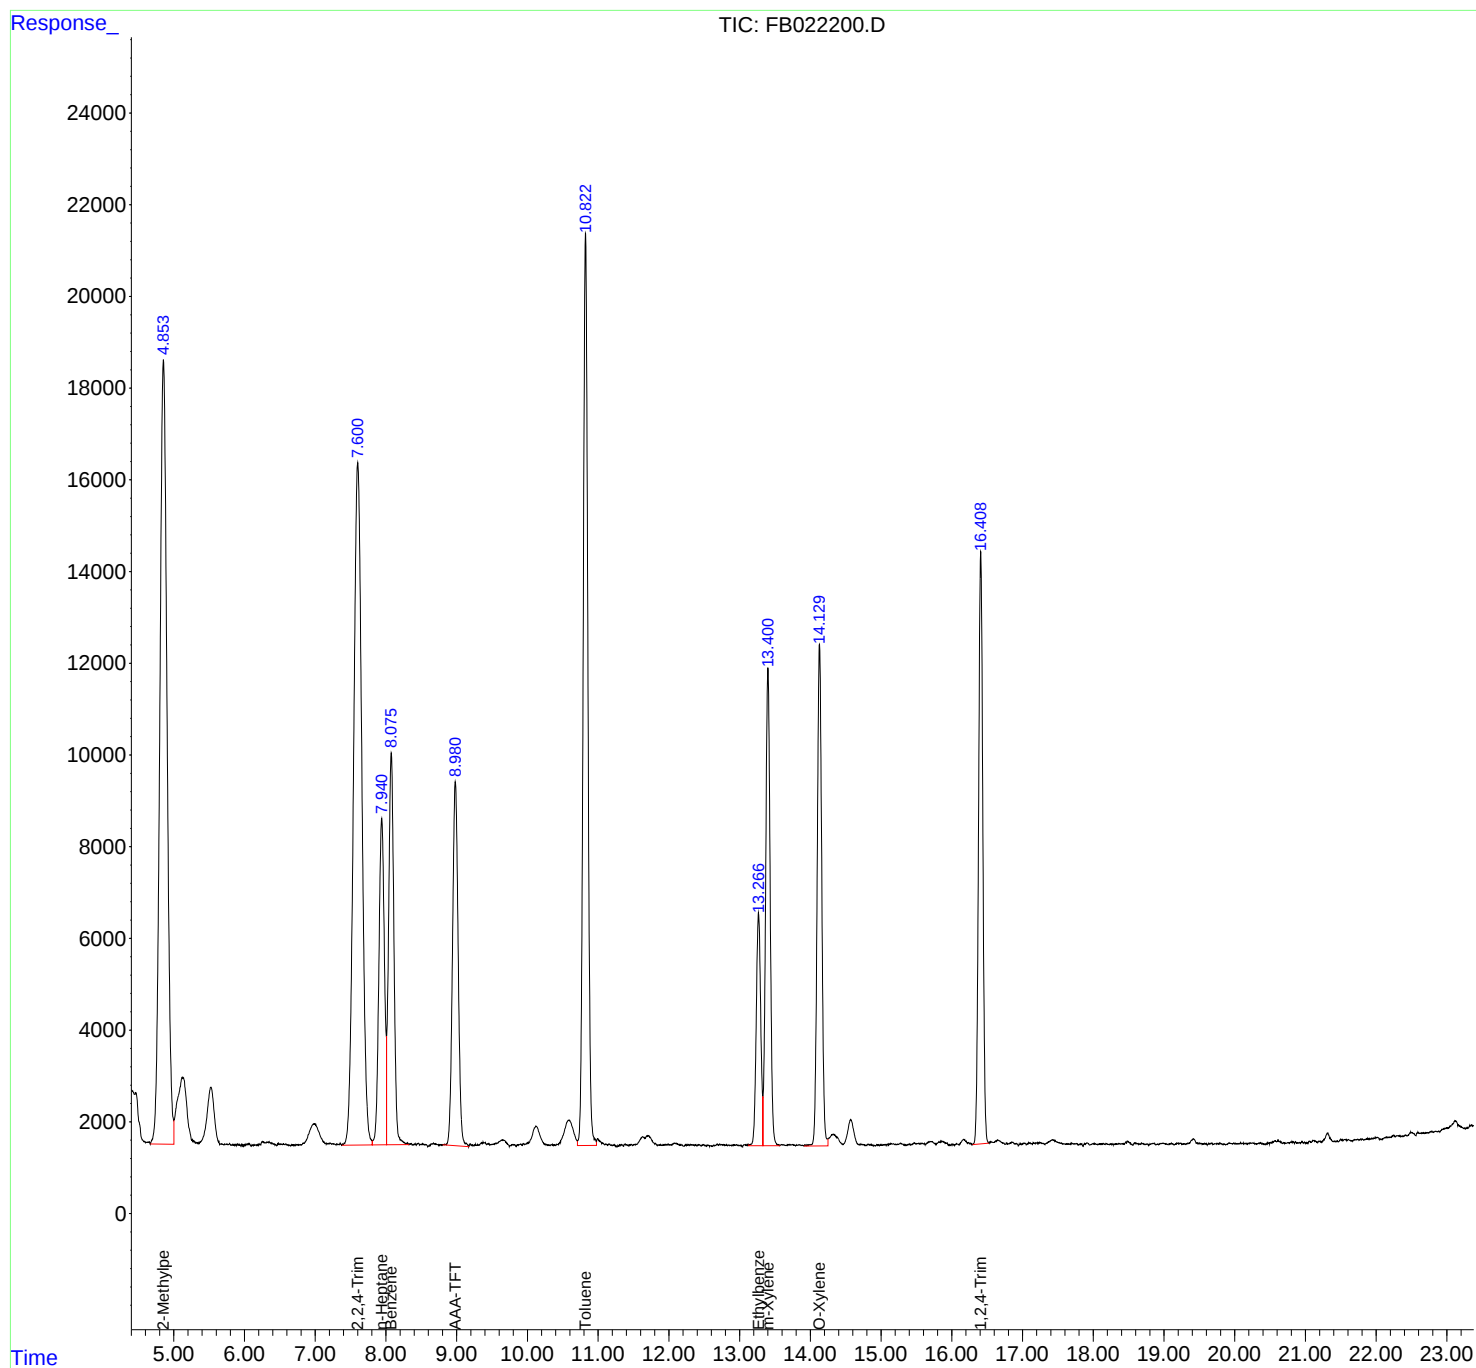


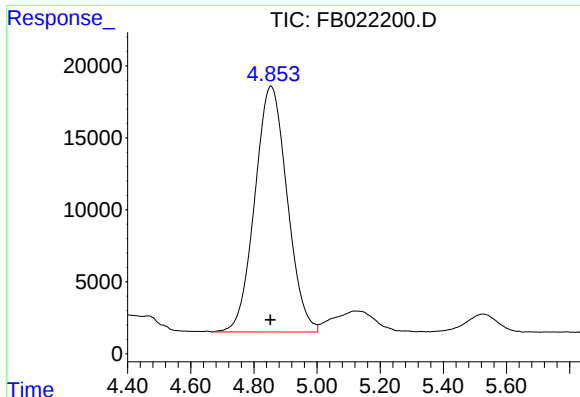

#1 2-Methylpentane


R.T.: 4.855 min
Delta R.T.: 0.003 min
Response: 1215437
Conc: 30.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827S1

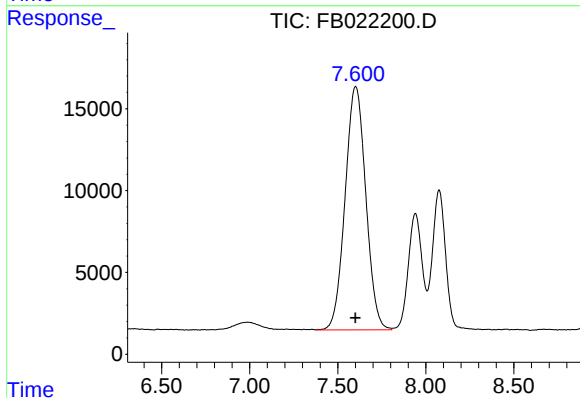


#2 2,2,4-Trimethylpentane

R.T.: 7.602 min
Delta R.T.: 0.002 min
Response: 1214835
Conc: 30.16 ng/ml

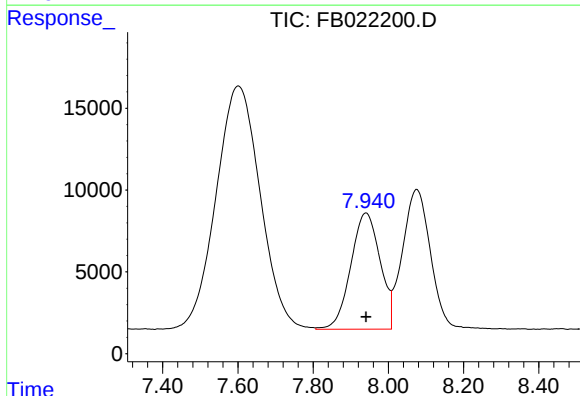


#3 n-Heptane

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 385250
Conc: 10.09 ng/ml

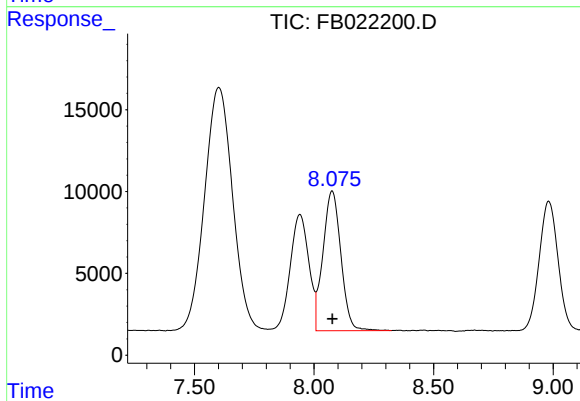

#4 Benzene


R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 444086
Conc: 9.89 ng/ml

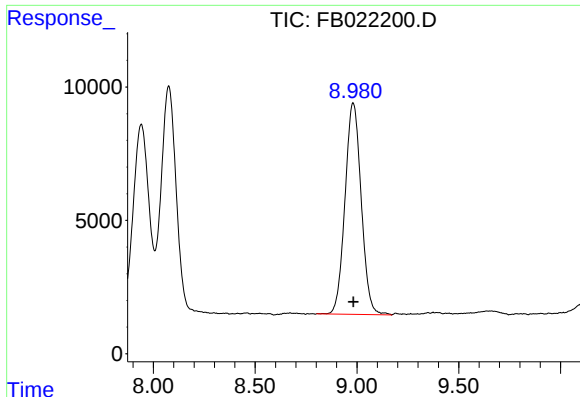

#5 AAA-TFT


R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 437764
Conc: 20.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827S1

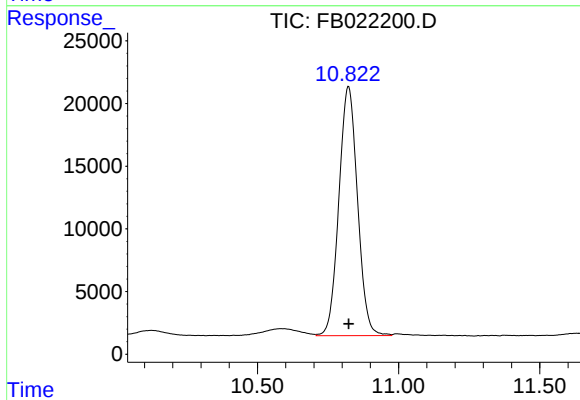


#6 Toluene

R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 912121
Conc: 29.67 ng/ml

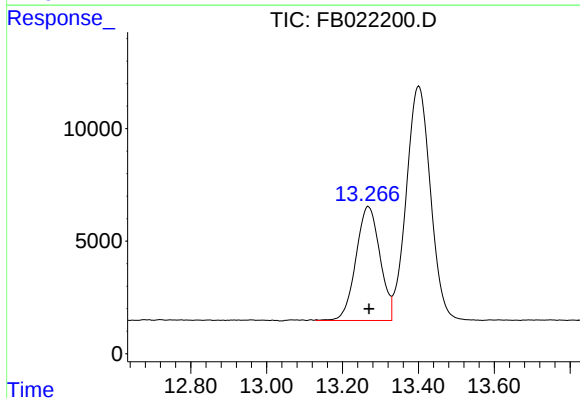


#7 Ethylbenzene

R.T.: 13.268 min
Delta R.T.: -0.001 min
Response: 222220
Conc: 10.89 ng/ml

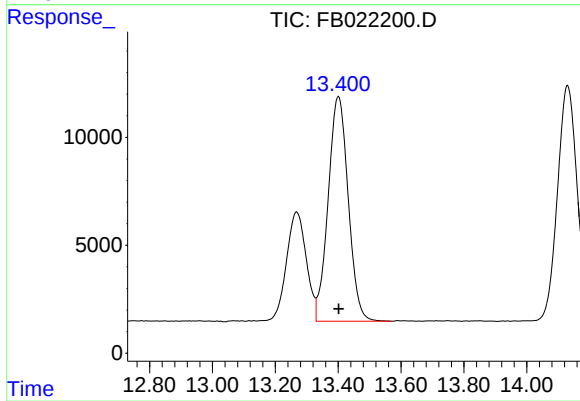

#8 m-Xylene


R.T.: 13.401 min
Delta R.T.: 0.000 min
Response: 462485
Conc: 21.96 ng/ml

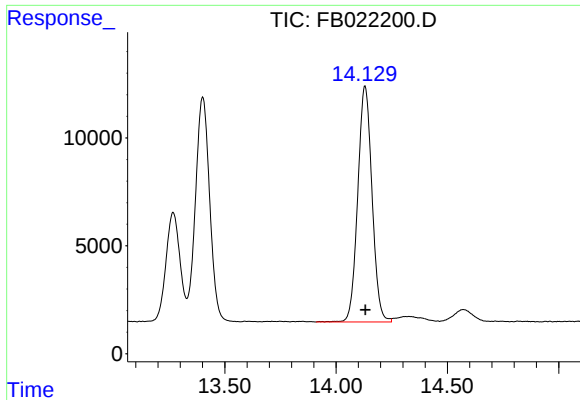

#9 O-Xylene

R.T.: 14.130 min
Delta R.T.: -0.001 min
Response: 486053
Conc: 21.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0827S1

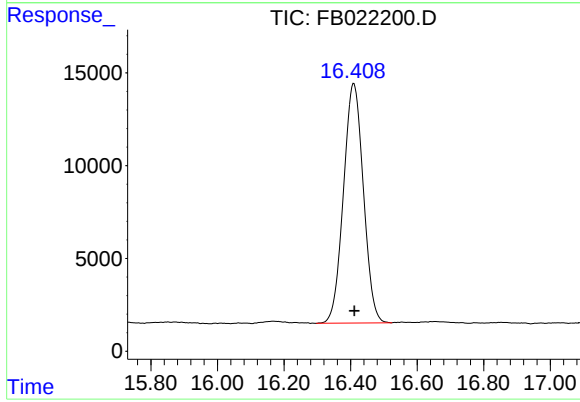

#10 1,2,4-Trimethylbenzene

R.T.: 16.410 min
Delta R.T.: -0.002 min
Response: 536464
Conc: 20.92 ng/ml