

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082719\  
 Data File : FB022201.D  
 Signal(s) : FID2B.CH  
 Acq On : 27 Aug 2019 10:31  
 Operator : DD/AJ  
 Sample : K4088-09  
 Misc : 5.04/5.00ml DI WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Aug 27 23:16:02 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
 Quant Title :  
 QLast Update : Wed Aug 21 07:59:08 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.980  | 427966   | 20.149 ng/ml |
| Target Compounds             |        |          |              |
| 2) t 2,2,4-Trimethylpentane  | 7.608  | 5985     | 0.149 ng/ml  |
| 9) t O-Xylene                | 14.075 | 1867     | 0.083 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.404 | 6785     | 0.265 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082719\  
Data File : FB022201.D  
Signal(s) : FID2B.CH  
Acq On : 27 Aug 2019 10:31  
Operator : DD/AJ  
Sample : K4088-09  
Misc : 5.04/5.00ml DI WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Aug 27 23:16:02 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

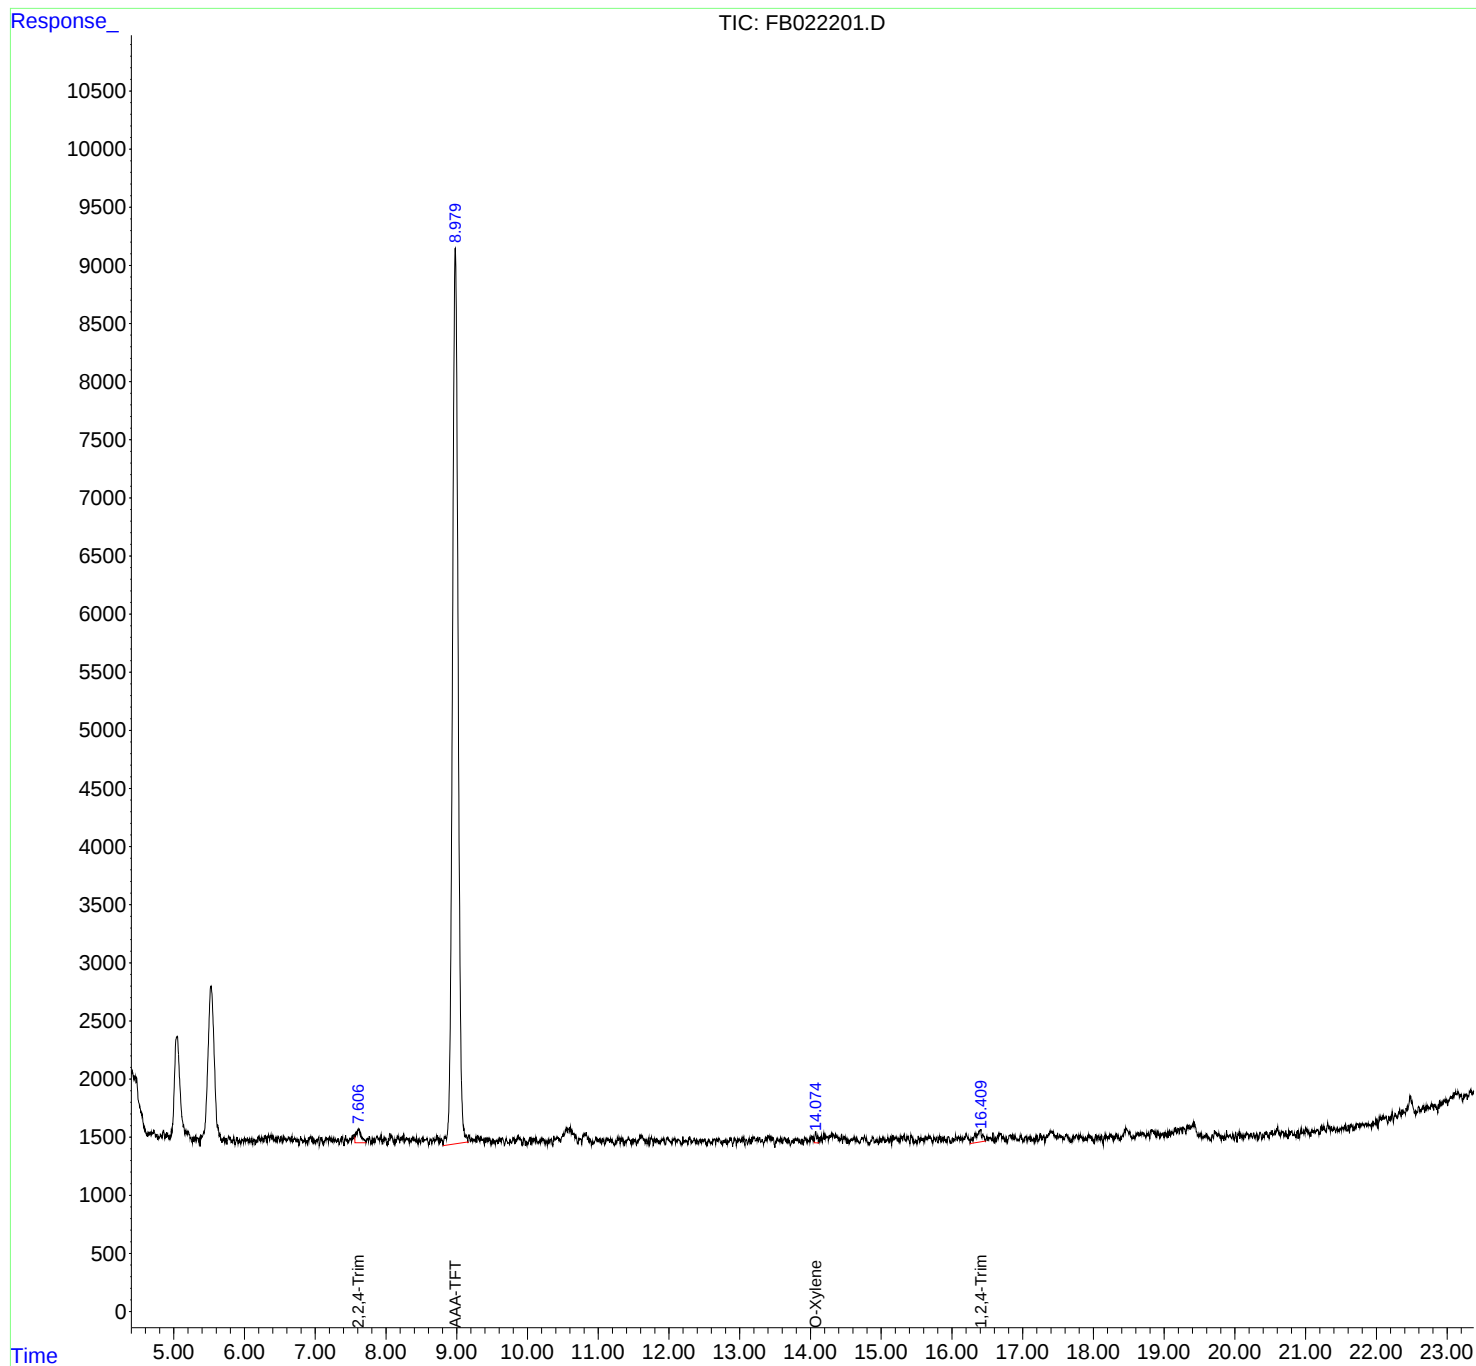


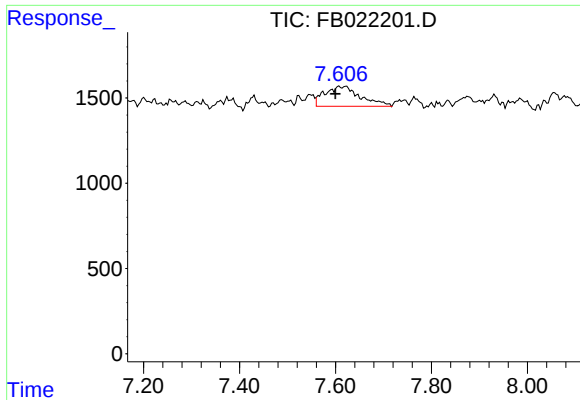

#2 2,2,4-Trimethylpentane


R.T.: 7.608 min  
Delta R.T.: 0.008 min  
Response: 5985  
Conc: 0.15 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

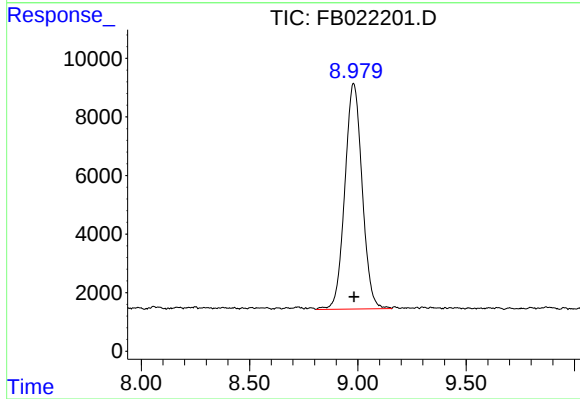


#5 AAA-TFT

R.T.: 8.980 min  
Delta R.T.: -0.002 min  
Response: 427966  
Conc: 20.15 ng/ml

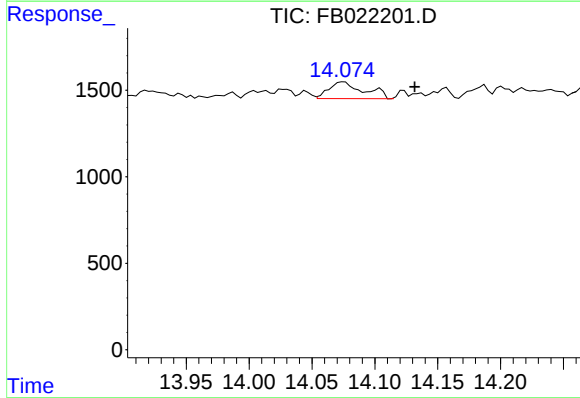

#9 O-Xylene

R.T.: 14.075 min  
Delta R.T.: -0.057 min  
Response: 1867  
Conc: 0.08 ng/ml

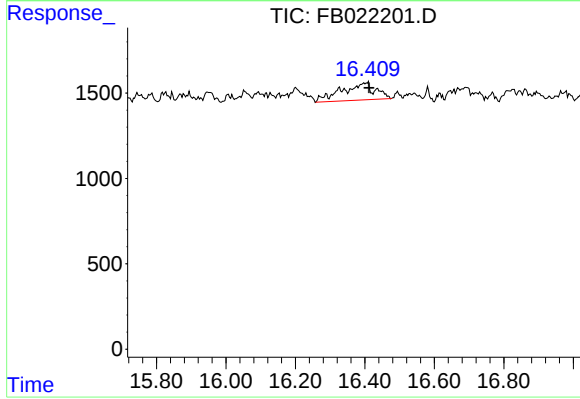

#10 1,2,4-Trimethylbenzene

R.T.: 16.404 min  
Delta R.T.: -0.008 min  
Response: 6785  
Conc: 0.26 ng/ml