

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022201.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 10:31
Operator : DD/AJ
Sample : K4088-09
Misc : 5.04/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CL-02-082619-1

Integration File: Calibration.e
Quant Time: Aug 27 23:16:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.980	427966	20.149 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.608	5985	0.149 ng/ml
9) t O-Xylene	14.075	1867	0.083 ng/ml
10) t 1,2,4-Trimethylbenzene	16.404	6785	0.265 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022201.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 10:31
Operator : DD/AJ
Sample : K4088-09
Misc : 5.04/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CL-02-082619-1

Integration File: Calibration.e
Quant Time: Aug 27 23:16:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

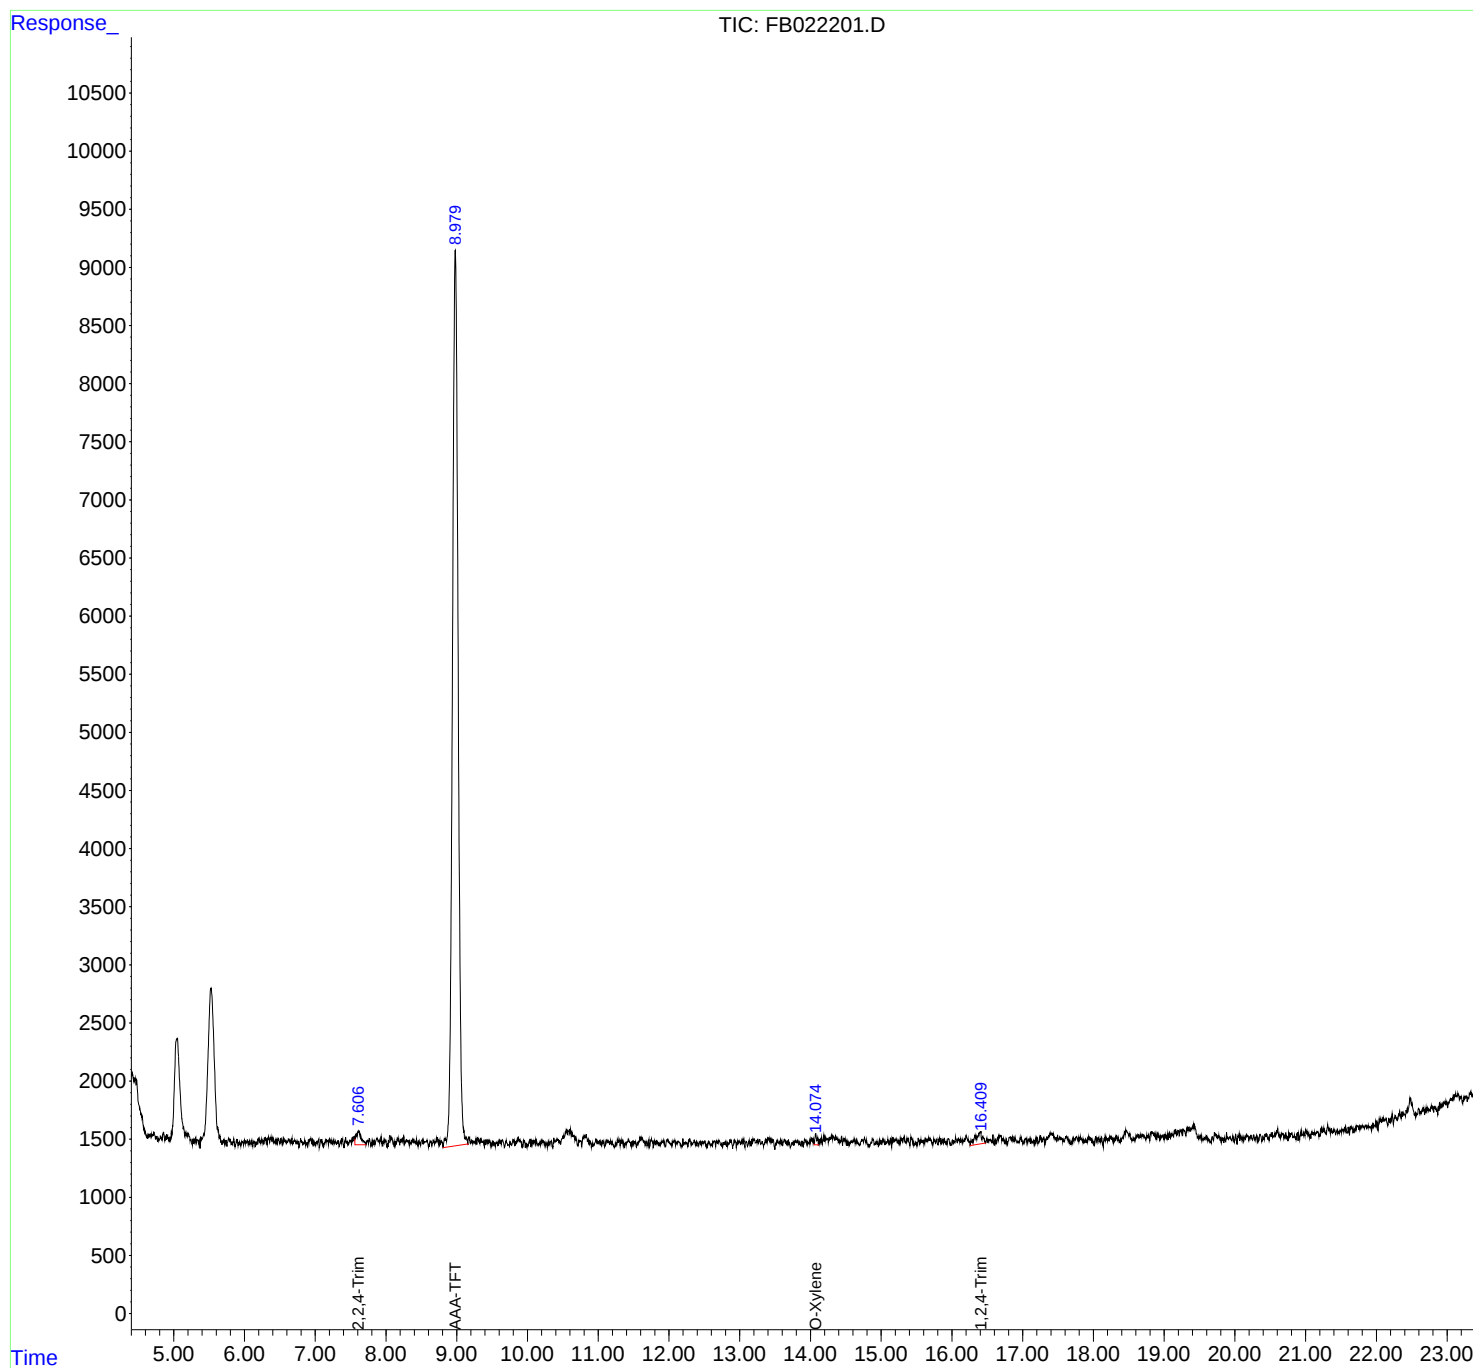


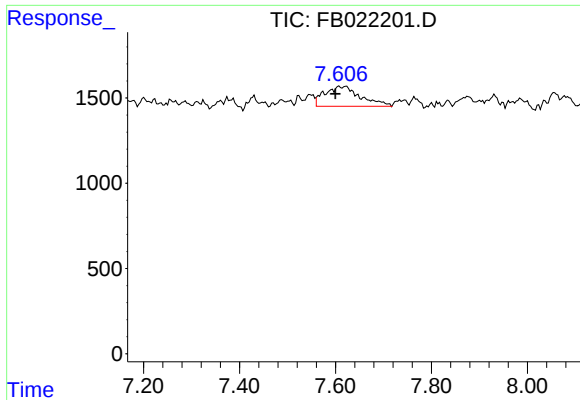

#2 2,2,4-Trimethylpentane


R.T.: 7.608 min
Delta R.T.: 0.008 min
Response: 5985
Conc: 0.15 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-02-082619-1

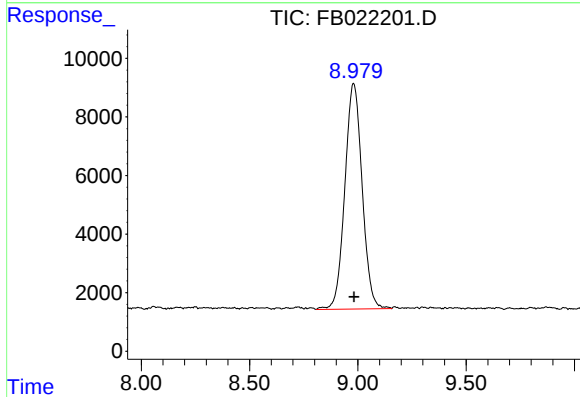


#5 AAA-TFT

R.T.: 8.980 min
Delta R.T.: -0.002 min
Response: 427966
Conc: 20.15 ng/ml

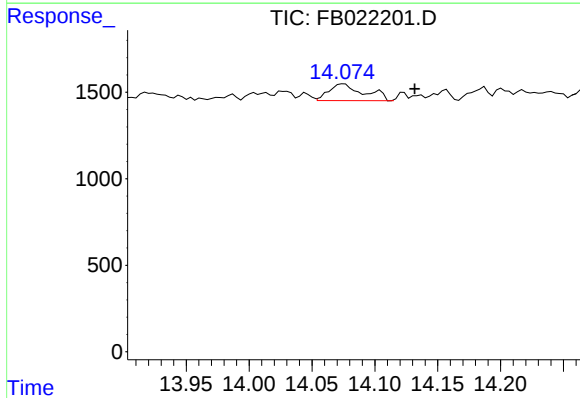

#9 O-Xylene

R.T.: 14.075 min
Delta R.T.: -0.057 min
Response: 1867
Conc: 0.08 ng/ml

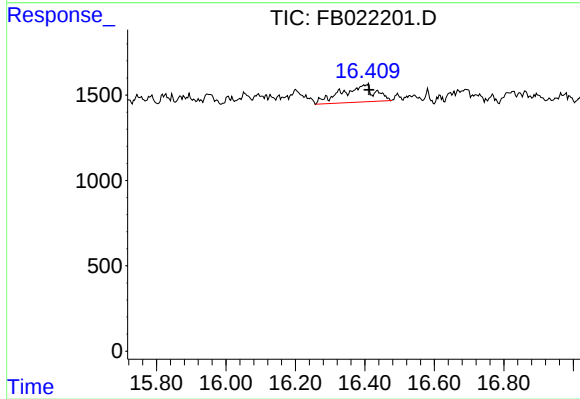

#10 1,2,4-Trimethylbenzene

R.T.: 16.404 min
Delta R.T.: -0.008 min
Response: 6785
Conc: 0.26 ng/ml