

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022205.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 12:32
 Operator : DD/AJ
 Sample : K4093-04MS
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PL-02-082619-1MS

Integration File: Calibration.e
 Quant Time: Aug 27 23:17:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.985	438455	20.643 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	1035338	25.869 ng/ml
2) t 2,2,4-Trimethylpentane	7.605	897295	22.278 ng/ml
3) t n-Heptane	7.944	276499	7.238 ng/ml
4) t Benzene	8.079	426227	9.494 ng/ml
6) t Toluene	10.826	839180	27.297 ng/ml
7) t Ethylbenzene	13.272	195295	9.570 ng/ml
8) t m-Xylene	13.405	400728	19.028 ng/ml
9) t O-Xylene	14.134	415253	18.567 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	439165	17.124 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022205.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 12:32
Operator : DD/AJ
Sample : K4093-04MS
Misc : 5.04/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MS

Integration File: Calibration.e
Quant Time: Aug 27 23:17:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

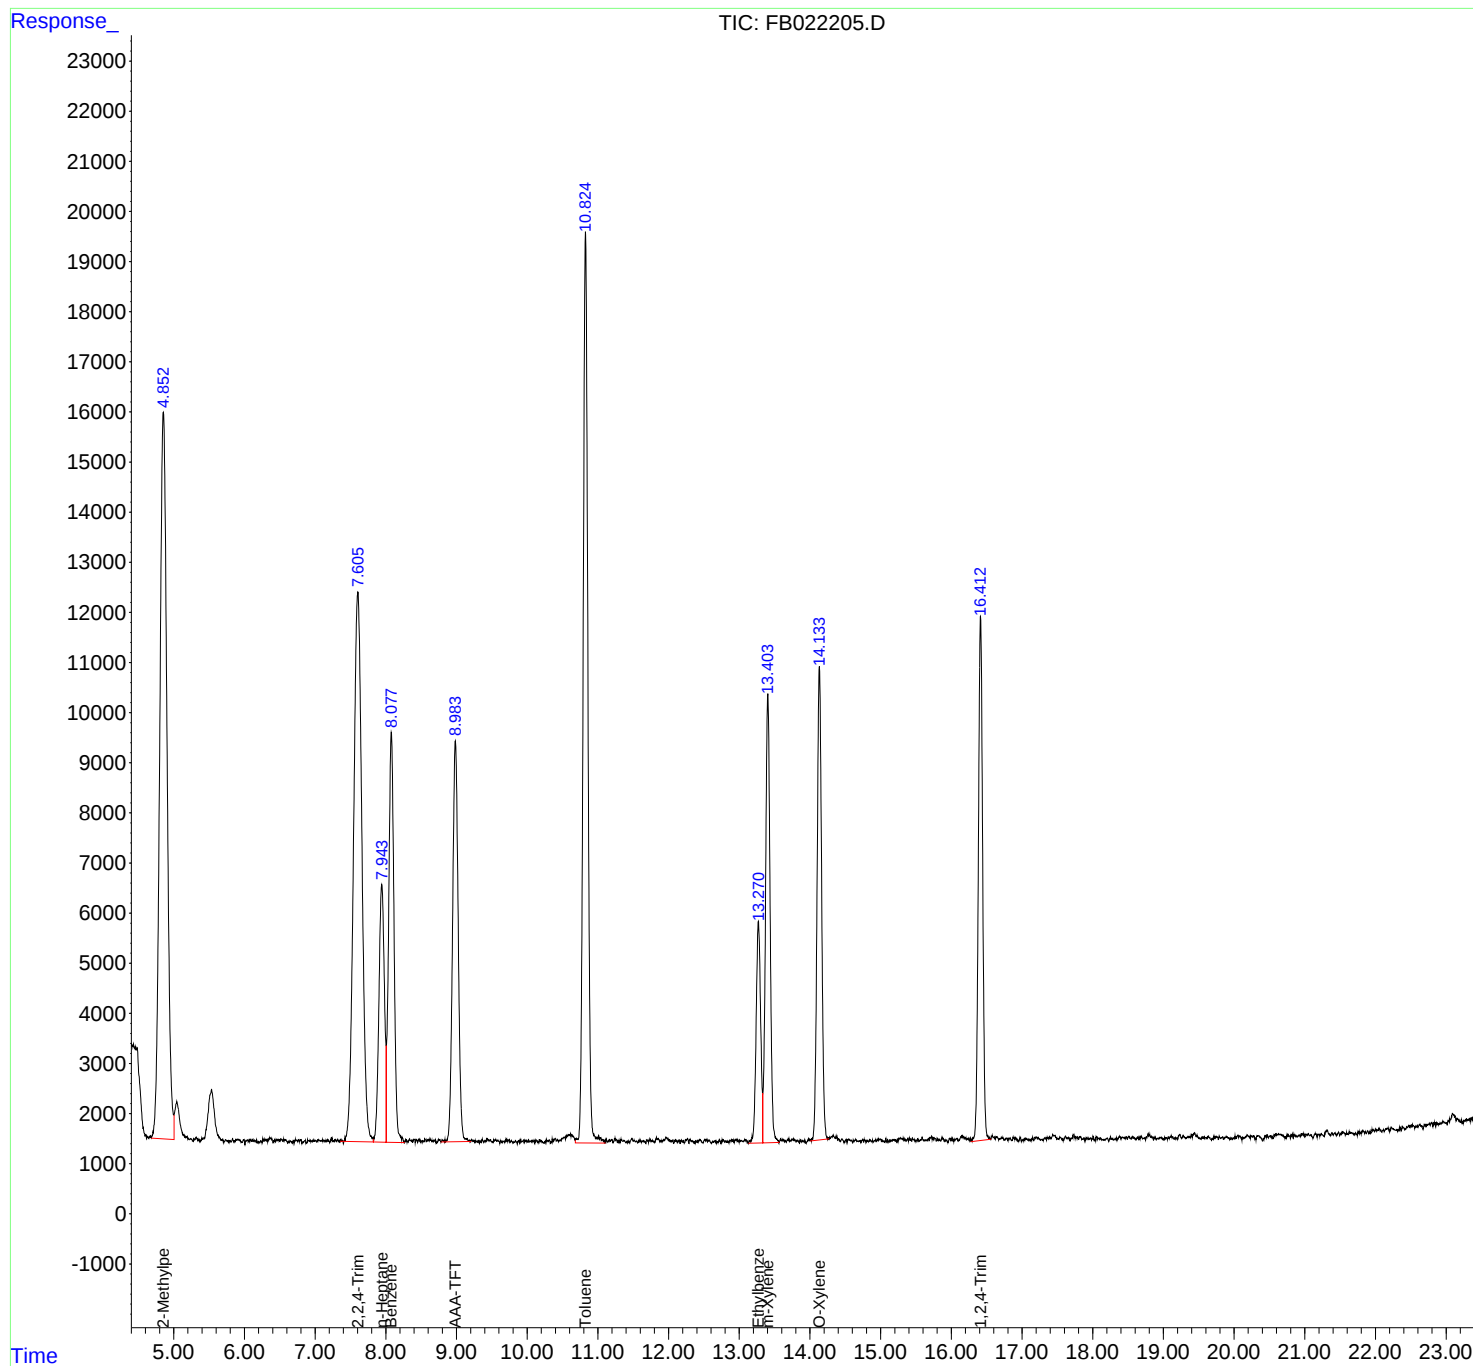


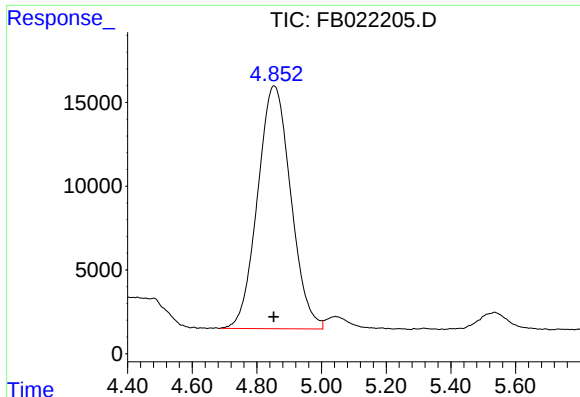

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: 0.002 min
Response: 1035338
Conc: 25.87 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MS

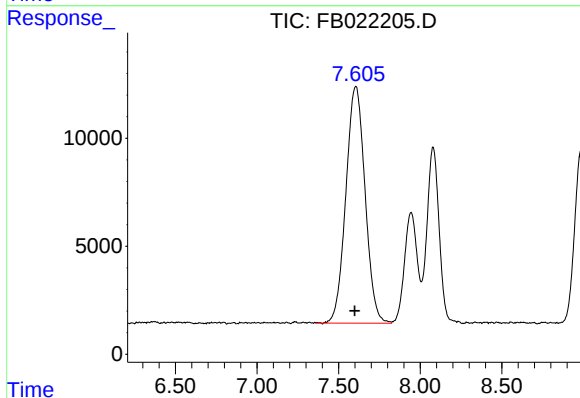


#2 2,2,4-Trimethylpentane

R.T.: 7.605 min
Delta R.T.: 0.006 min
Response: 897295
Conc: 22.28 ng/ml

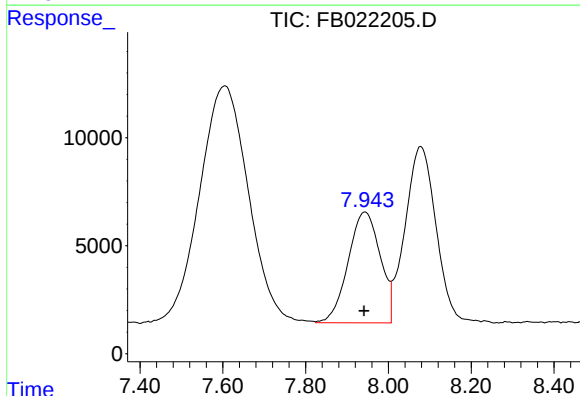


#3 n-Heptane

R.T.: 7.944 min
Delta R.T.: 0.003 min
Response: 276499
Conc: 7.24 ng/ml

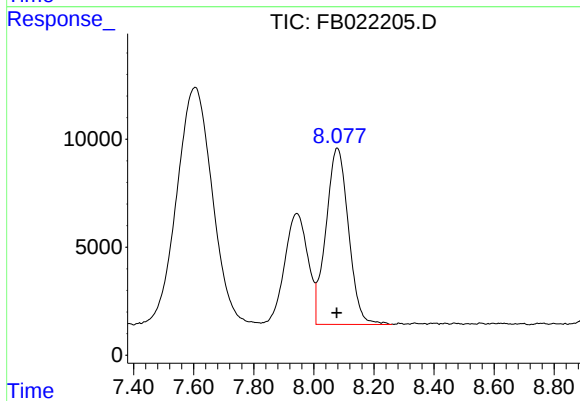

#4 Benzene


R.T.: 8.079 min
Delta R.T.: 0.002 min
Response: 426227
Conc: 9.49 ng/ml

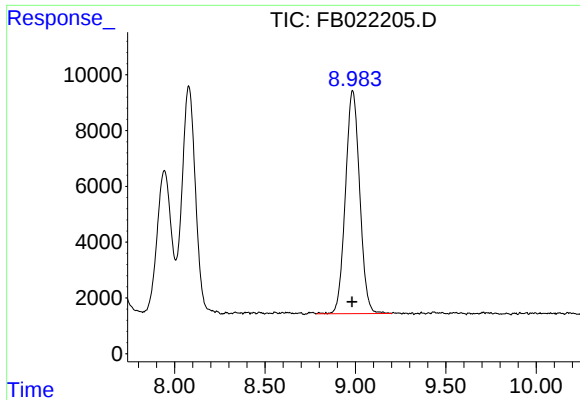

#5 AAA-TFT


R.T.: 8.985 min
Delta R.T.: 0.003 min
Response: 438455
Conc: 20.64 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MS

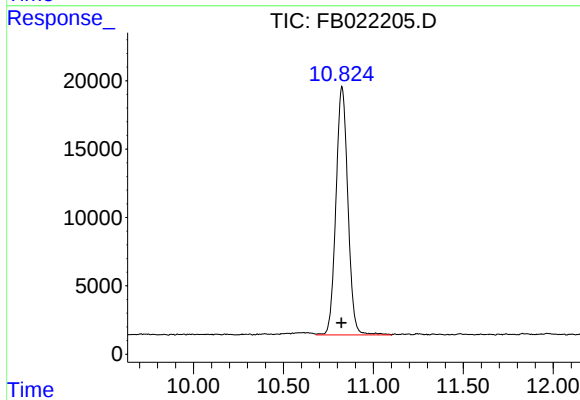


#6 Toluene

R.T.: 10.826 min
Delta R.T.: 0.003 min
Response: 839180
Conc: 27.30 ng/ml

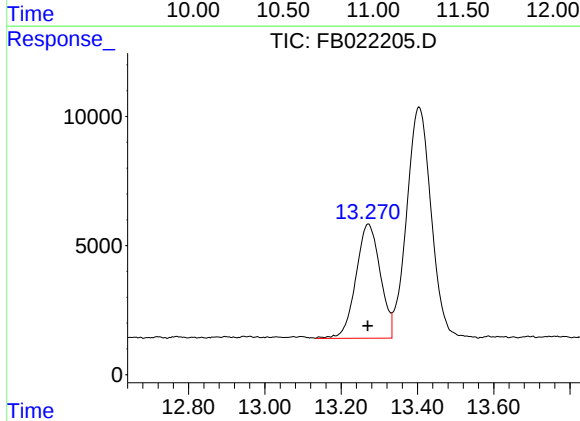


#7 Ethylbenzene

R.T.: 13.272 min
Delta R.T.: 0.002 min
Response: 195295
Conc: 9.57 ng/ml

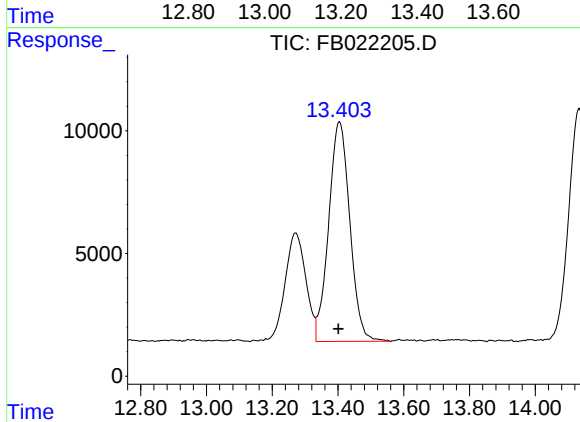

#8 m-Xylene


R.T.: 13.405 min
Delta R.T.: 0.003 min
Response: 400728
Conc: 19.03 ng/ml

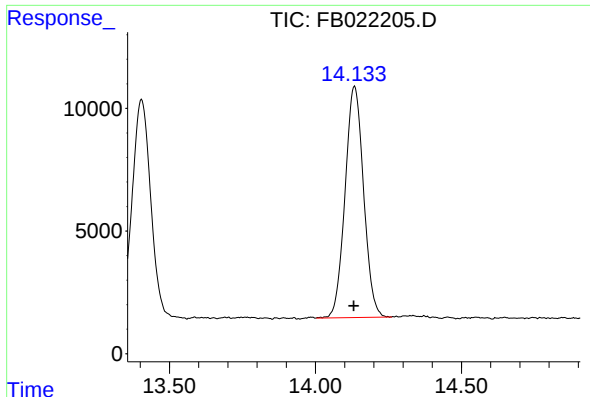

#9 O-Xylene

R.T.: 14.134 min
Delta R.T.: 0.002 min
Response: 415253
Conc: 18.57 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MS

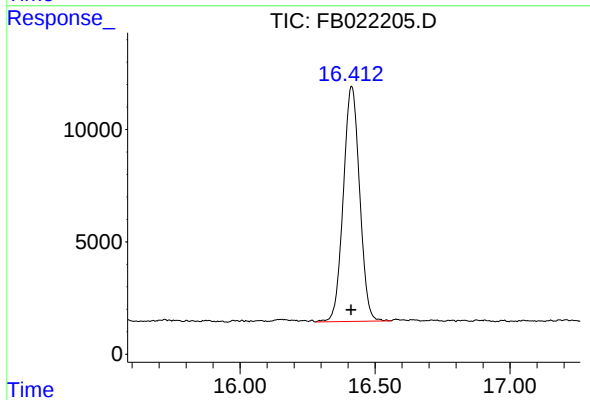

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.002 min
Response: 439165
Conc: 17.12 ng/ml