

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022206.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 13:03
 Operator : DD/AJ
 Sample : K4093-04MSD
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PL-02-082619-1MSD

Integration File: Calibration.e
 Quant Time: Aug 27 23:17:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.985	400262	18.845 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.852	967197	24.166 ng/ml
2) t 2,2,4-Trimethylpentane	7.602	853883	21.200 ng/ml
3) t n-Heptane	7.943	255709	6.694 ng/ml
4) t Benzene	8.078	395431	8.808 ng/ml
6) t Toluene	10.826	777293	25.284 ng/ml
7) t Ethylbenzene	13.272	183990	9.016 ng/ml
8) t m-Xylene	13.405	372939	17.708 ng/ml
9) t O-Xylene	14.135	394246	17.628 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	406281	15.842 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022206.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 13:03
Operator : DD/AJ
Sample : K4093-04MSD
Misc : 5.06/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MSD

Integration File: Calibration.e
Quant Time: Aug 27 23:17:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

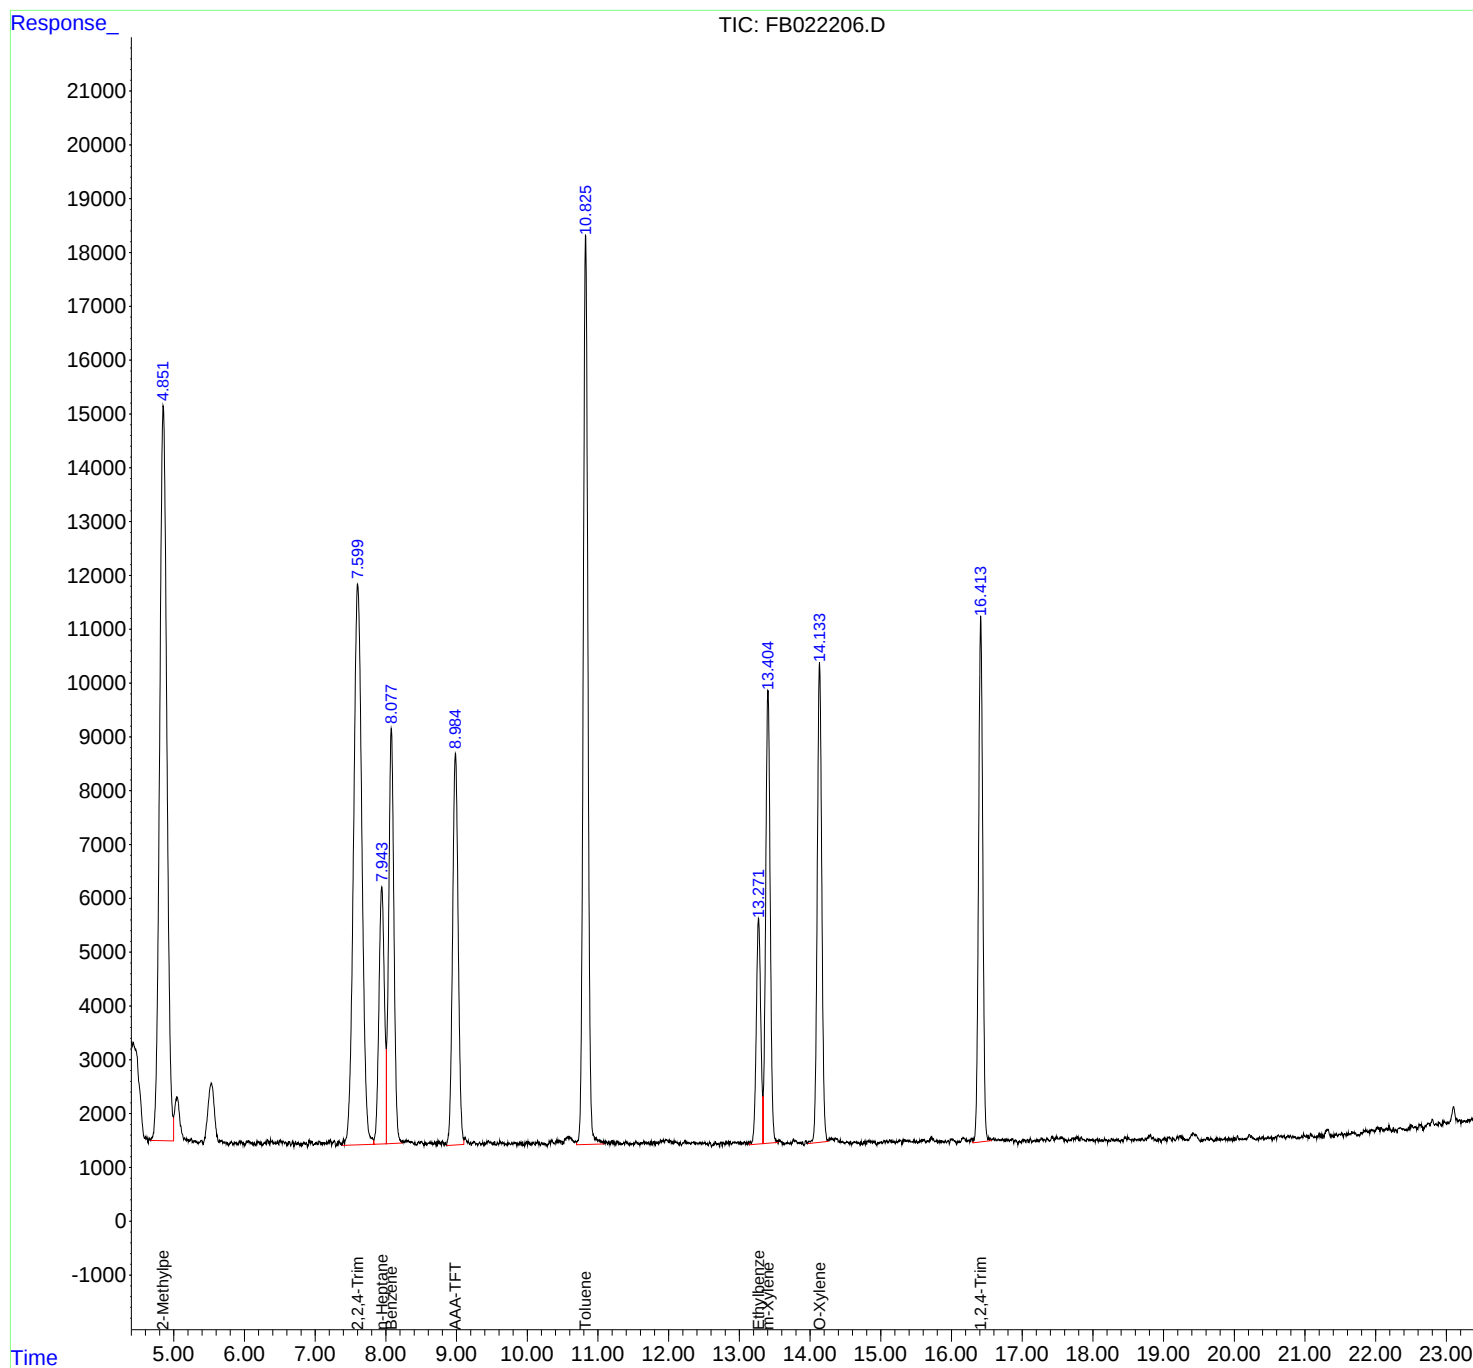


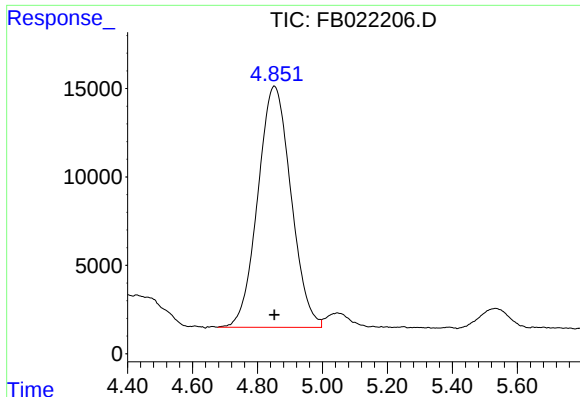

#1 2-Methylpentane


R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 967197
Conc: 24.17 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MSD

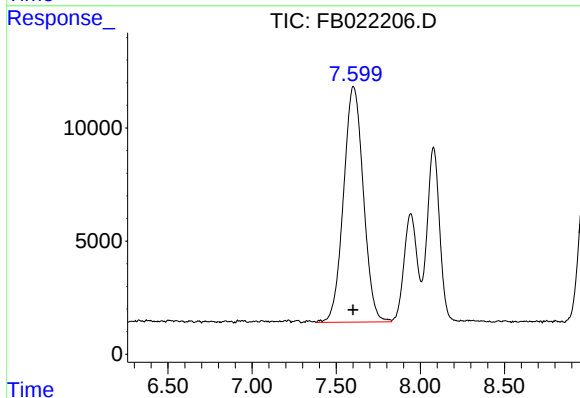


#2 2,2,4-Trimethylpentane

R.T.: 7.602 min
Delta R.T.: 0.002 min
Response: 853883
Conc: 21.20 ng/ml

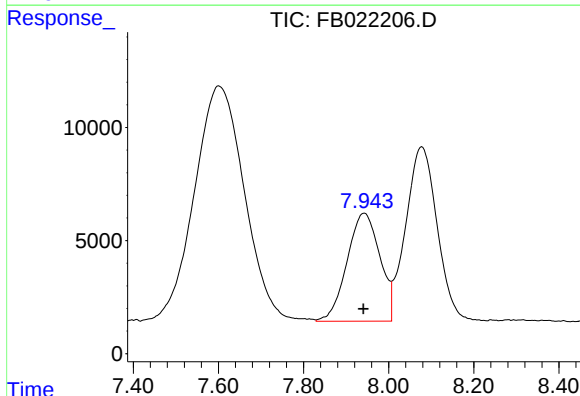


#3 n-Heptane

R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 255709
Conc: 6.69 ng/ml

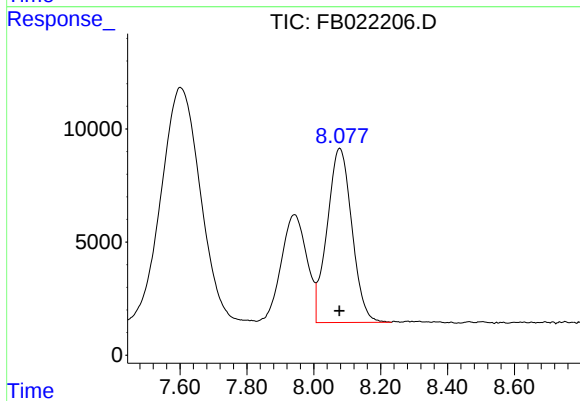

#4 Benzene


R.T.: 8.078 min
Delta R.T.: 0.002 min
Response: 395431
Conc: 8.81 ng/ml

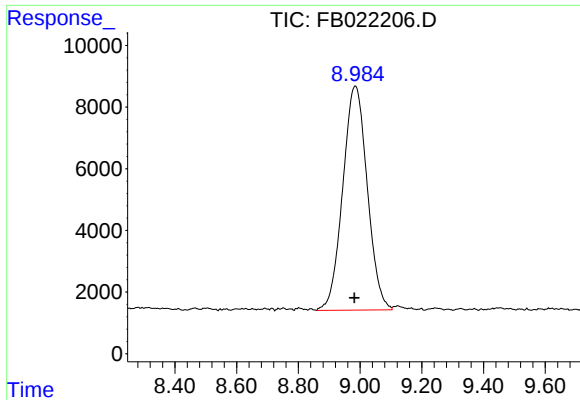

#5 AAA-TFT


R.T.: 8.985 min
Delta R.T.: 0.003 min
Response: 400262
Conc: 18.84 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MSD

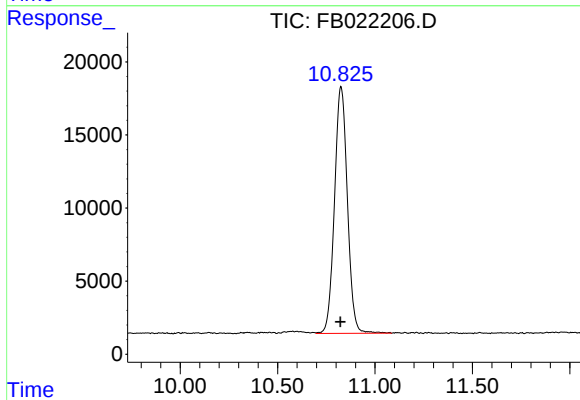


#6 Toluene

R.T.: 10.826 min
Delta R.T.: 0.003 min
Response: 777293
Conc: 25.28 ng/ml

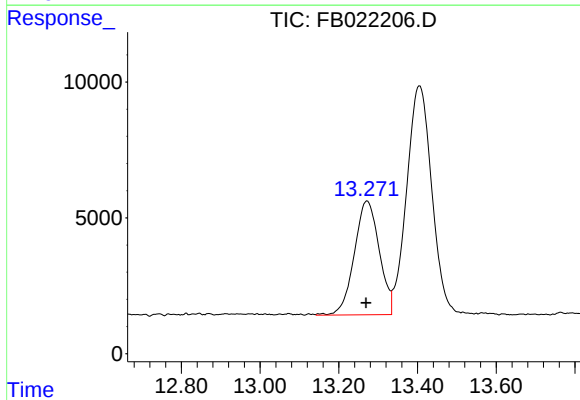


#7 Ethylbenzene

R.T.: 13.272 min
Delta R.T.: 0.002 min
Response: 183990
Conc: 9.02 ng/ml

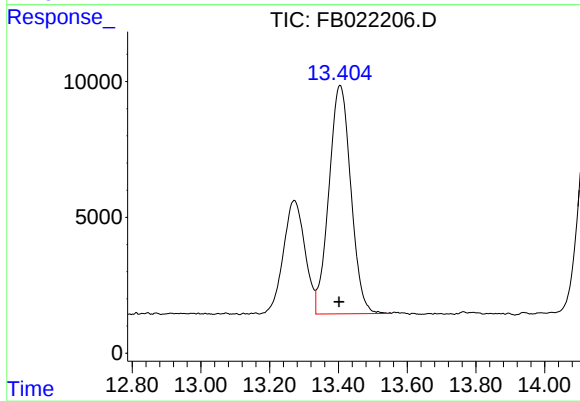

#8 m-Xylene


R.T.: 13.405 min
Delta R.T.: 0.004 min
Response: 372939
Conc: 17.71 ng/ml

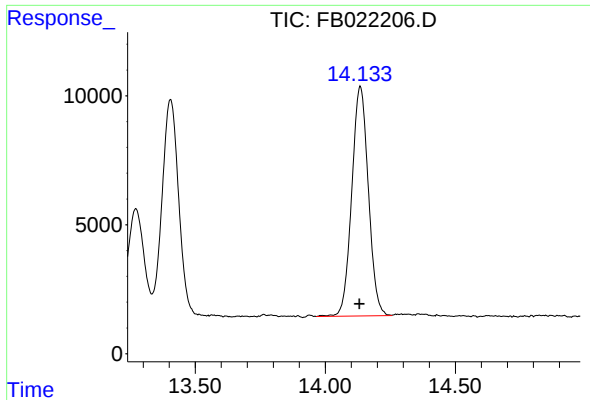

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.003 min
Response: 394246
Conc: 17.63 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-082619-1MSD

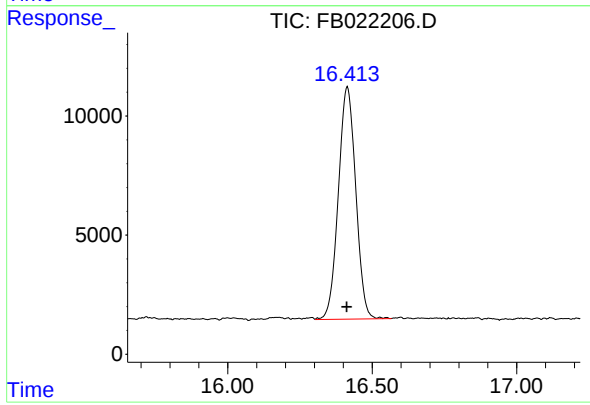

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.003 min
Response: 406281
Conc: 15.84 ng/ml