

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022210.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 15:15
 Operator : DD/AJ
 Sample : K4551-17
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S402-K1-1.0-1.5-082619

Integration File: Calibration.e
 Quant Time: Aug 27 23:18:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	473747	22.304 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	7260	0.181 ng/ml
6) t Toluene	10.817	2132	0.069 ng/ml
9) t O-Xylene	14.144	2227	0.100 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022210.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 15:15
Operator : DD/AJ
Sample : K4551-17
Misc : 5.02/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619

Integration File: Calibration.e
Quant Time: Aug 27 23:18:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

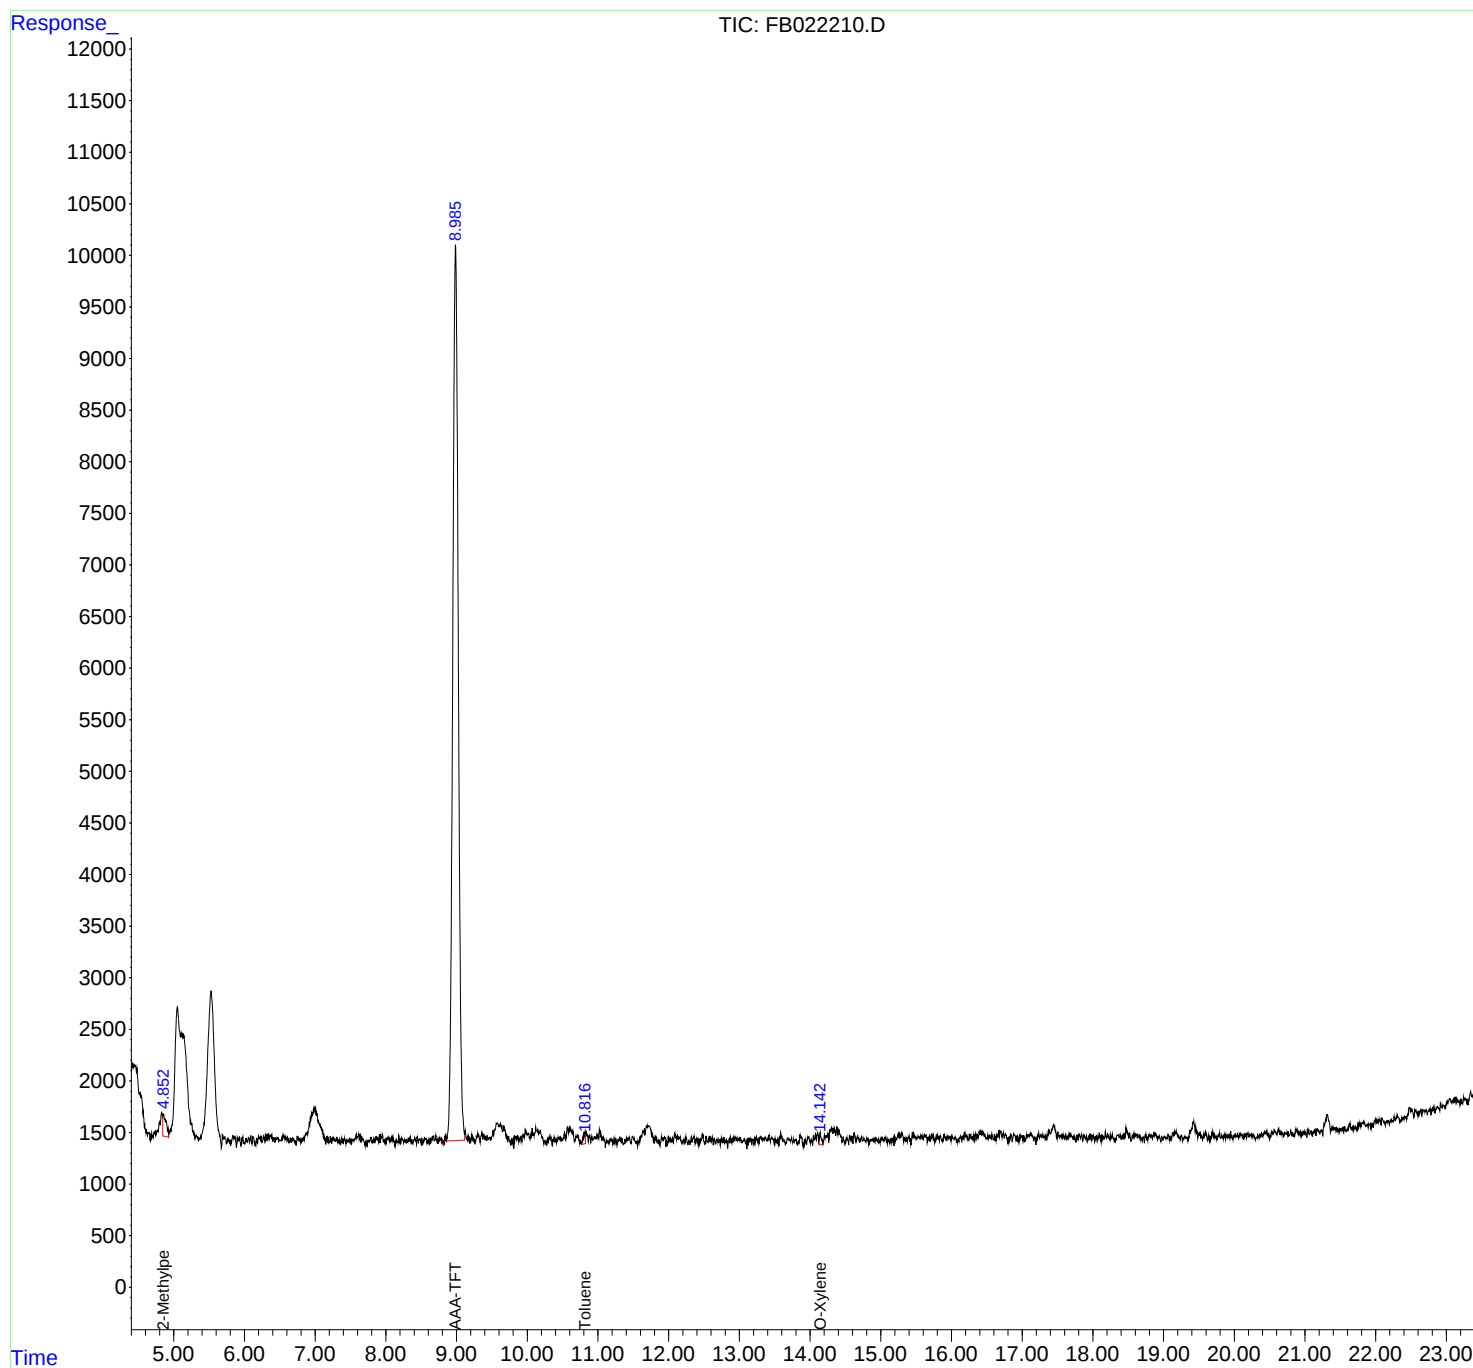


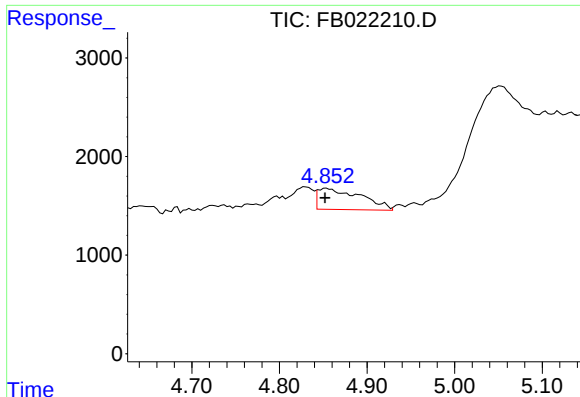

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: 0.002 min
Response: 7260
Conc: 0.18 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619

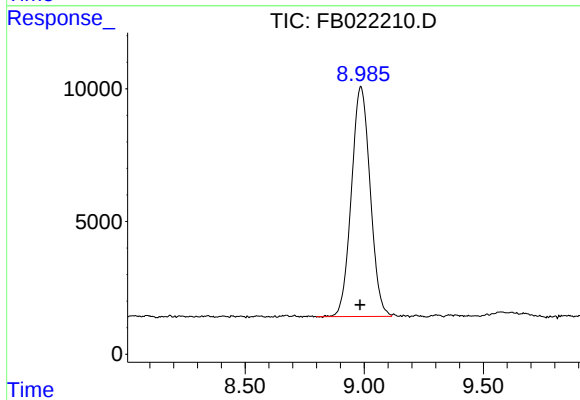


#5 AAA-TFT

R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 473747
Conc: 22.30 ng/ml

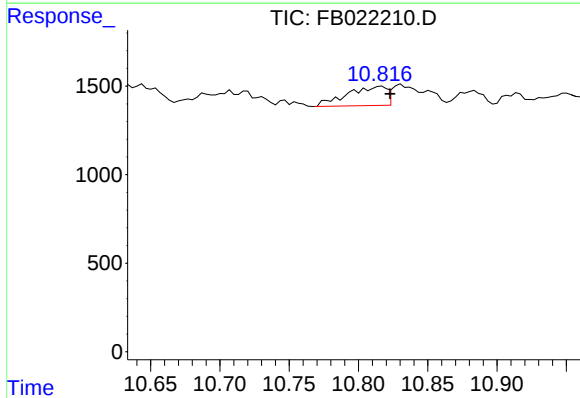

#6 Toluene

R.T.: 10.817 min
Delta R.T.: -0.006 min
Response: 2132
Conc: 0.07 ng/ml

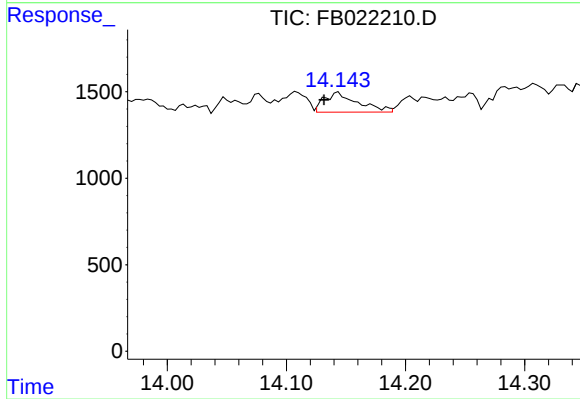

#9 O-Xylene

R.T.: 14.144 min
Delta R.T.: 0.012 min
Response: 2227
Conc: 0.10 ng/ml