

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022211.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 15:46
 Operator : DD/AJ
 Sample : K4551-18MS
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S402-K1-1.0-1.5-082619MS

Integration File: Calibration.e
 Quant Time: Aug 27 23:18:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	414348	19.508 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1041297	26.018 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	992853	24.650 ng/ml
3) t n-Heptane	7.946	308609	8.079 ng/ml
4) t Benzene	8.082	409680	9.126 ng/ml
6) t Toluene	10.829	820569	26.692 ng/ml
7) t Ethylbenzene	13.275	200400	9.820 ng/ml
8) t m-Xylene	13.407	423696	20.118 ng/ml
9) t O-Xylene	14.136	453515	20.278 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	504916	19.688 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022211.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 15:46
Operator : DD/AJ
Sample : K4551-18MS
Misc : 5.01/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MS

Integration File: Calibration.e
Quant Time: Aug 27 23:18:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

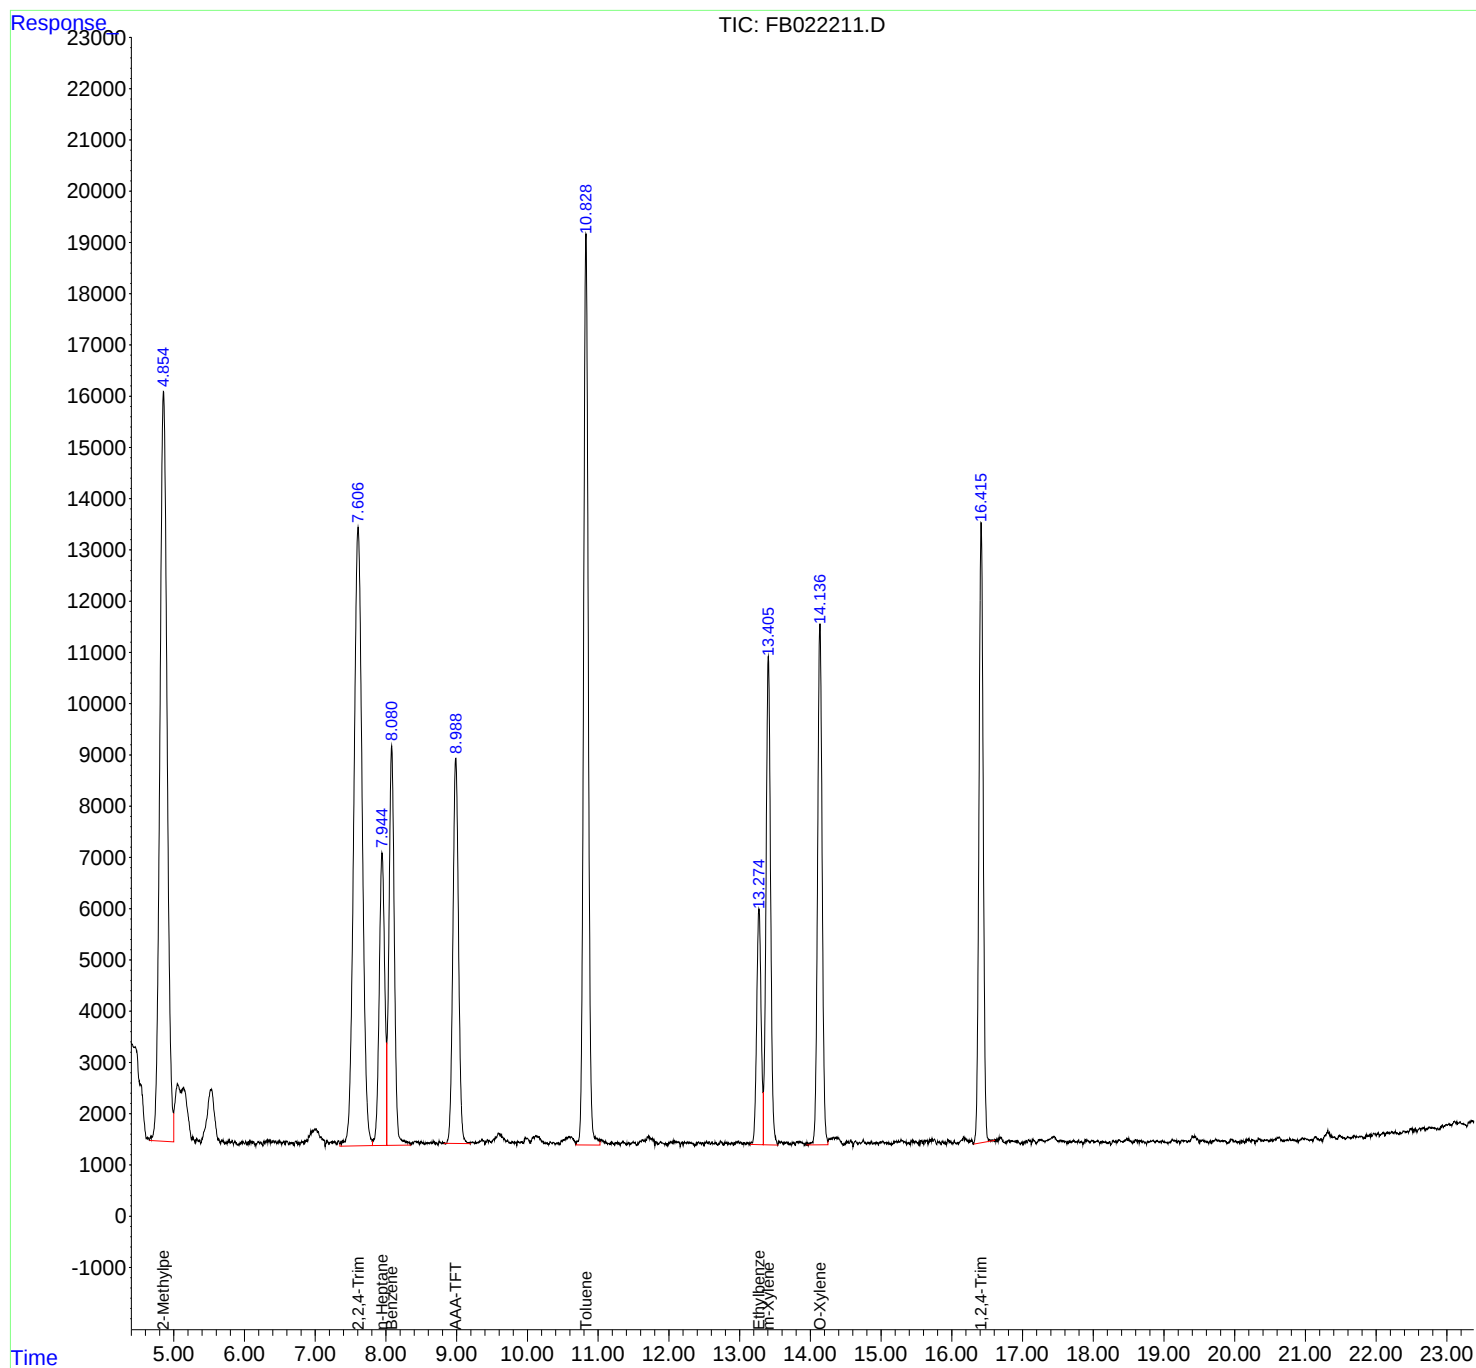


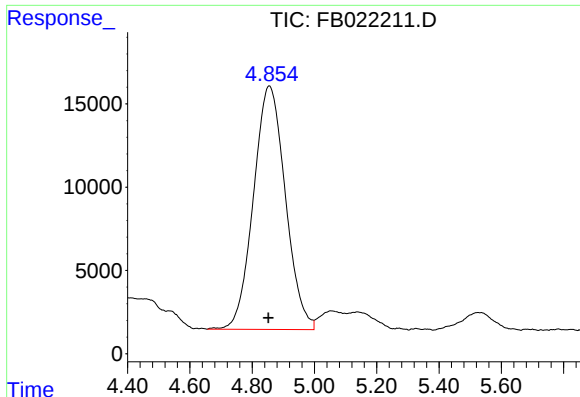

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 1041297
Conc: 26.02 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MS

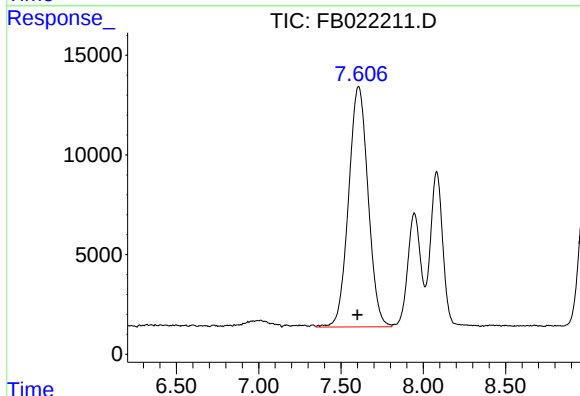


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: 0.007 min
Response: 992853
Conc: 24.65 ng/ml

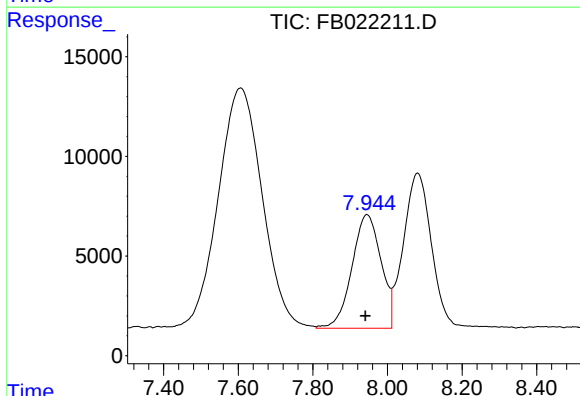


#3 n-Heptane

R.T.: 7.946 min
Delta R.T.: 0.005 min
Response: 308609
Conc: 8.08 ng/ml

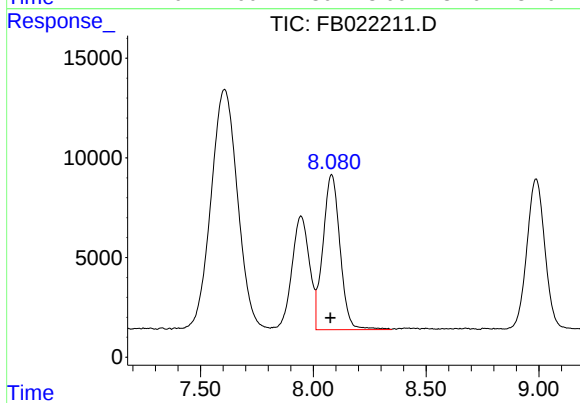

#4 Benzene


R.T.: 8.082 min
Delta R.T.: 0.005 min
Response: 409680
Conc: 9.13 ng/ml

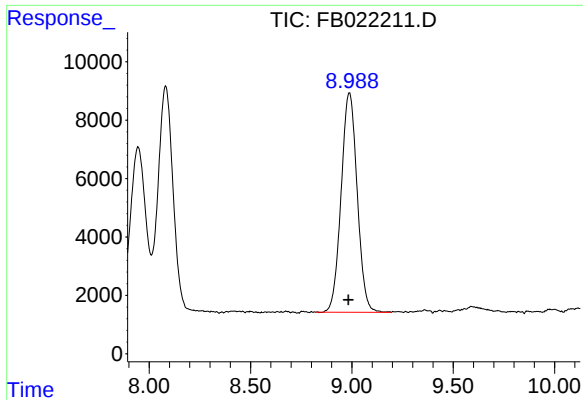

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 414348
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MS

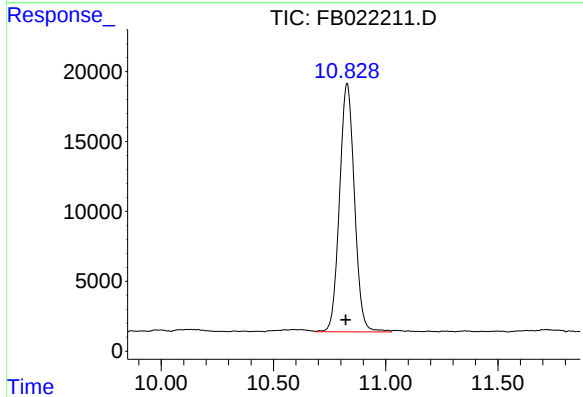


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.006 min
Response: 820569
Conc: 26.69 ng/ml

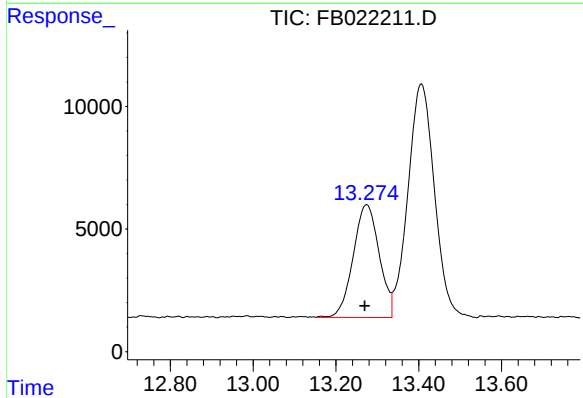


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.005 min
Response: 200400
Conc: 9.82 ng/ml

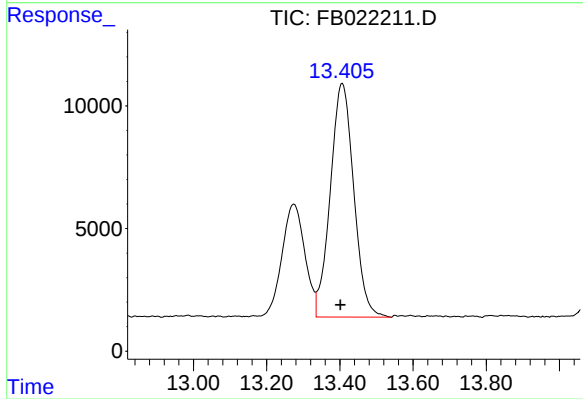

#8 m-Xylene


R.T.: 13.407 min
Delta R.T.: 0.005 min
Response: 423696
Conc: 20.12 ng/ml

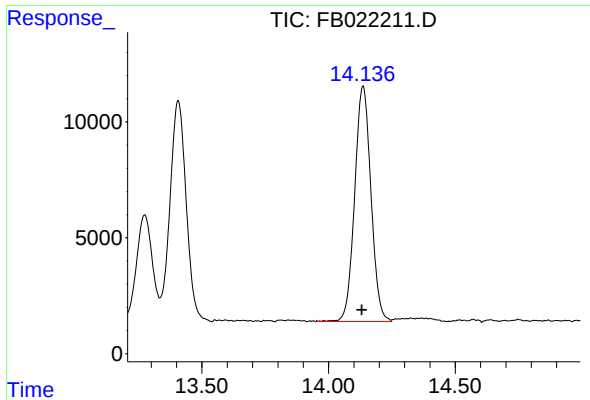

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: 0.005 min
Response: 453515
Conc: 20.28 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MS

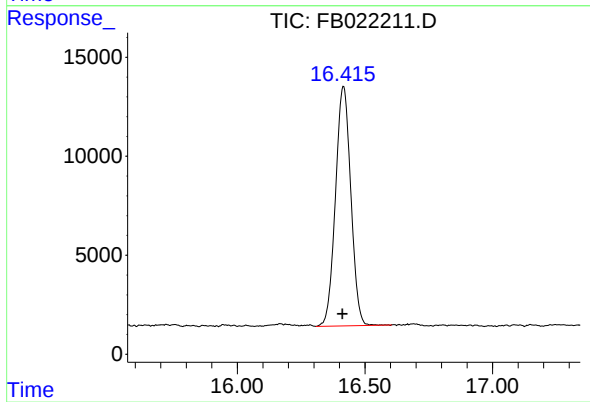

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: 0.004 min
Response: 504916
Conc: 19.69 ng/ml