

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
 Data File : FB022212.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2019 16:17
 Operator : DD/AJ
 Sample : K4551-20MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S402-K1-1.0-1.5-082619MSD

Integration File: Calibration.e
 Quant Time: Aug 27 23:18:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	449273	21.152 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1084906	27.107 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	902210	22.400 ng/ml
3) t n-Heptane	7.945	283651	7.426 ng/ml
4) t Benzene	8.081	427329	9.519 ng/ml
6) t Toluene	10.828	852111	27.718 ng/ml
7) t Ethylbenzene	13.274	210530	10.317 ng/ml
8) t m-Xylene	13.407	433571	20.587 ng/ml
9) t O-Xylene	14.137	457682	20.464 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	489511	19.087 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082719\
Data File : FB022212.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2019 16:17
Operator : DD/AJ
Sample : K4551-20MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MSD

Integration File: Calibration.e
Quant Time: Aug 27 23:18:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

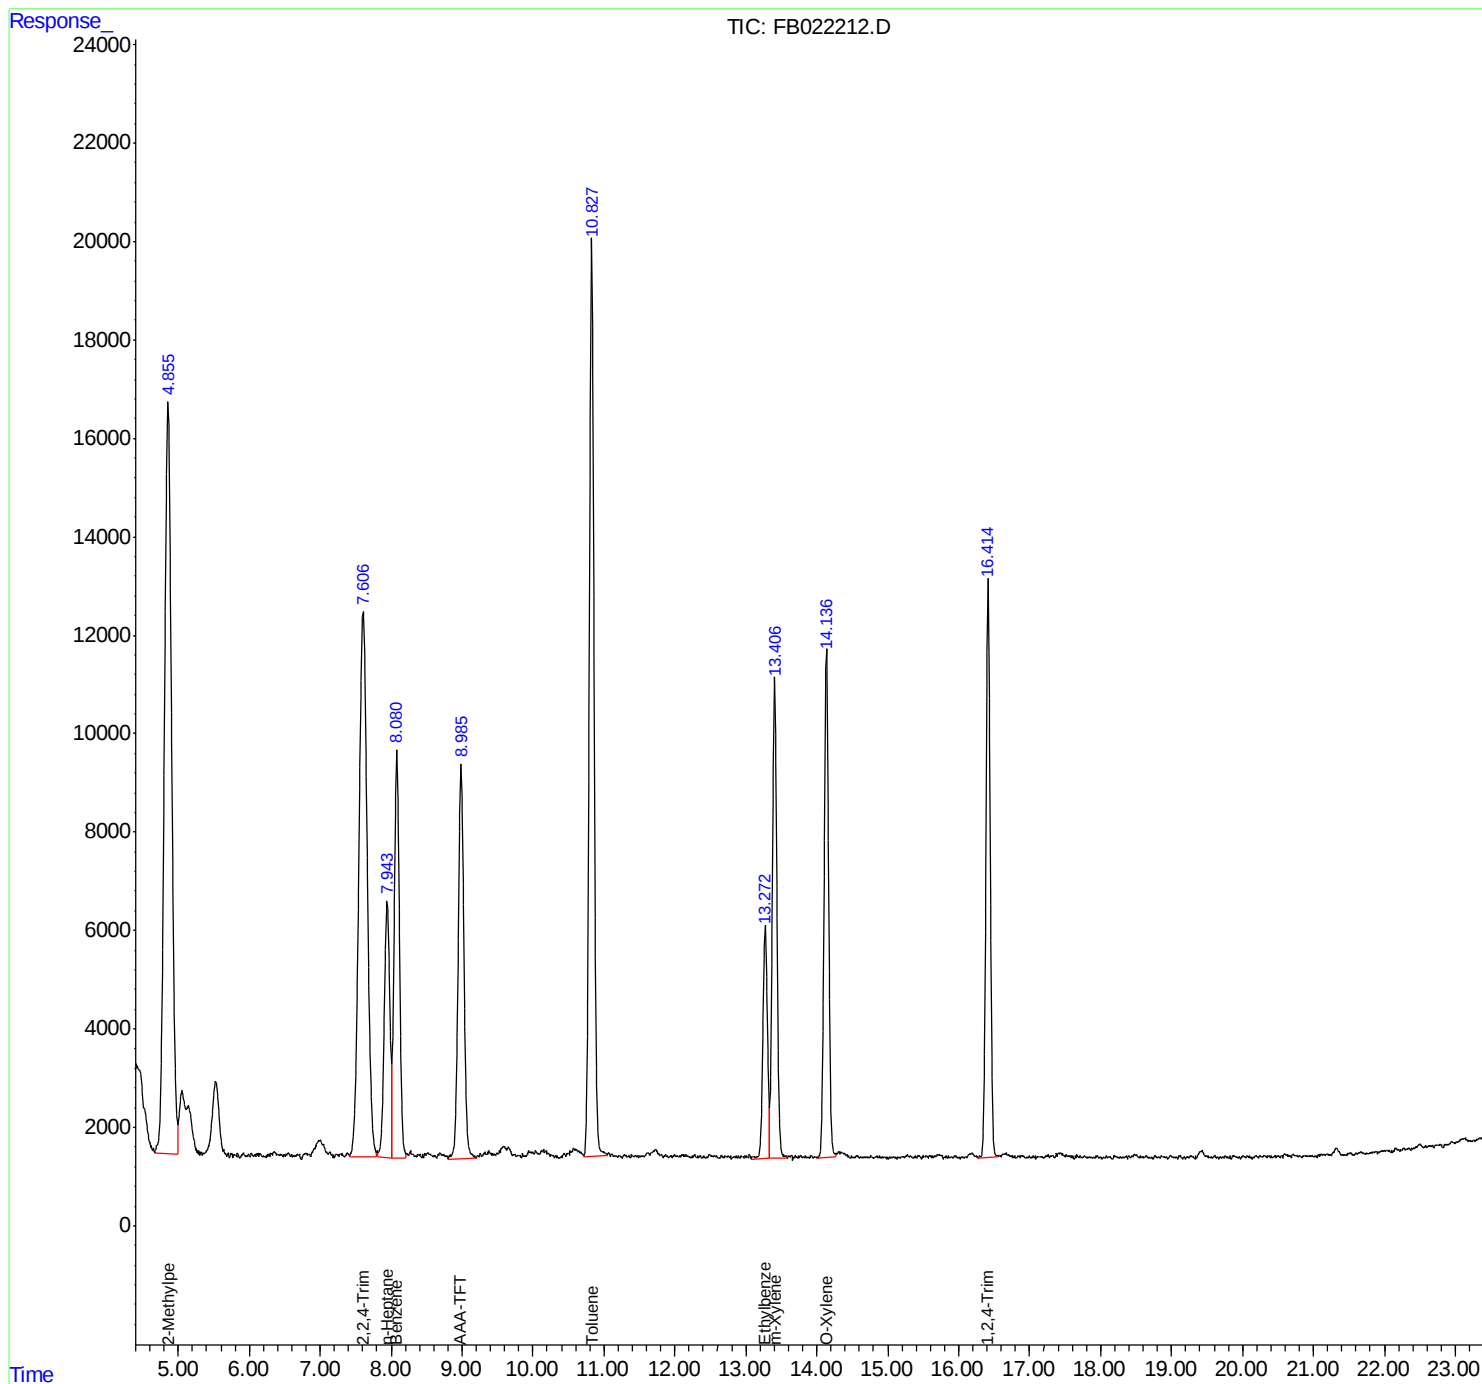


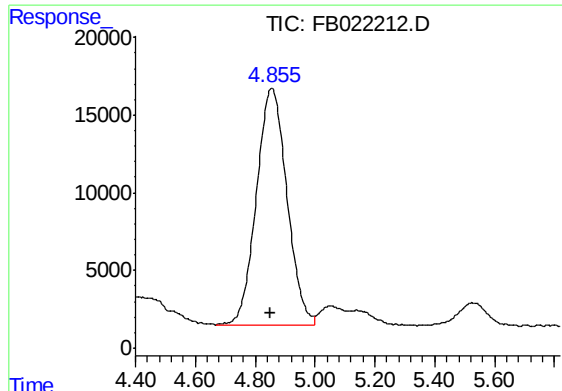

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 1084906
Conc: 27.11 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MSD

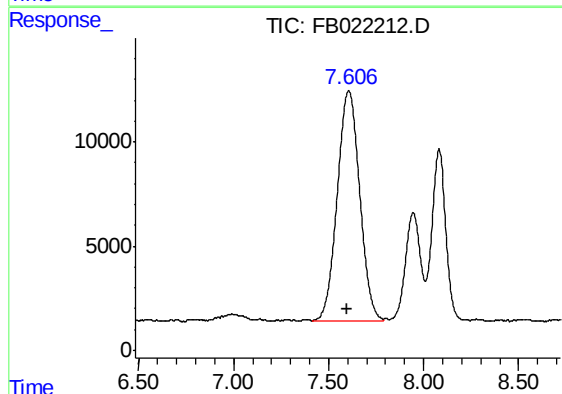


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: 0.007 min
Response: 902210
Conc: 22.40 ng/ml

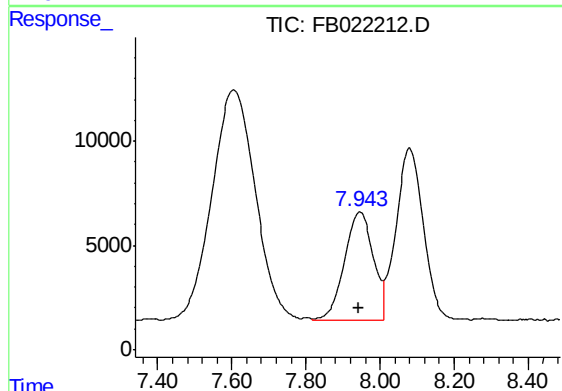


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: 0.004 min
Response: 283651
Conc: 7.43 ng/ml

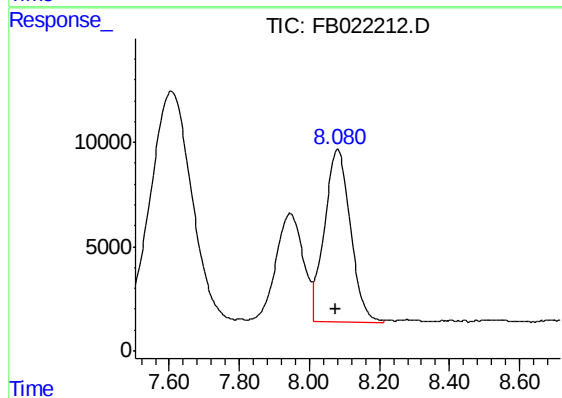

#4 Benzene


R.T.: 8.081 min
Delta R.T.: 0.005 min
Response: 427329
Conc: 9.52 ng/ml

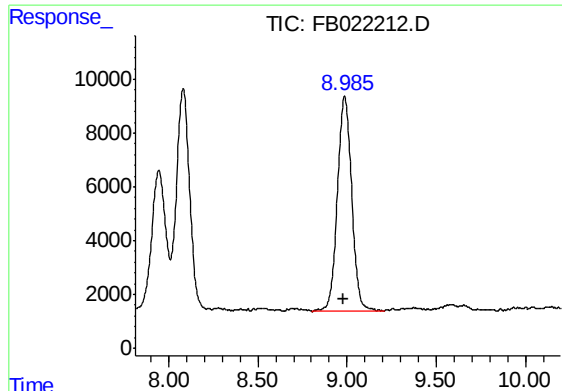

#5 AAA-TFT


R.T.: 8.987 min
Delta R.T.: 0.004 min
Response: 449273
Conc: 21.15 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MSD

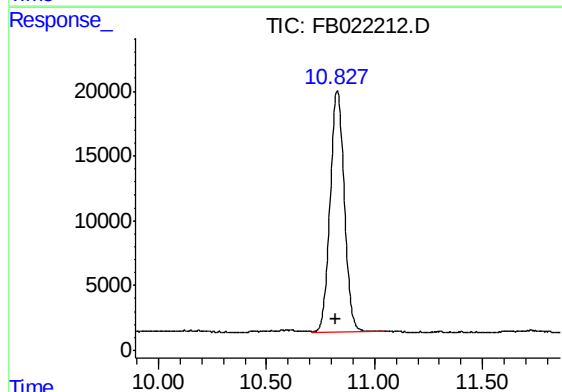


#6 Toluene

R.T.: 10.828 min
Delta R.T.: 0.005 min
Response: 852111
Conc: 27.72 ng/ml

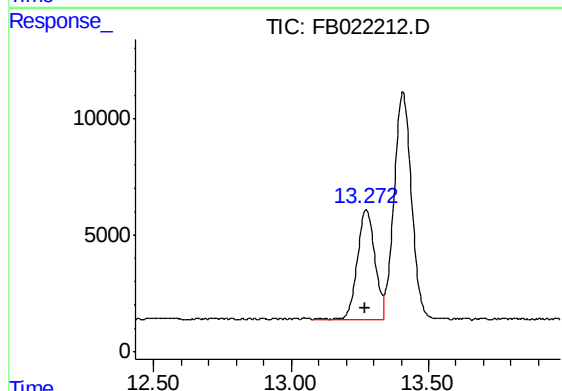


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: 0.004 min
Response: 210530
Conc: 10.32 ng/ml

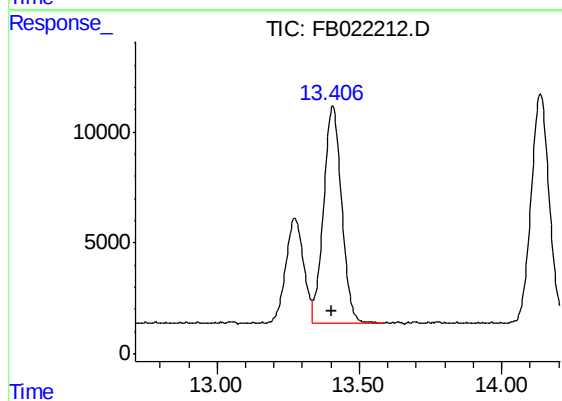

#8 m-Xylene


R.T.: 13.407 min
Delta R.T.: 0.005 min
Response: 433571
Conc: 20.59 ng/ml

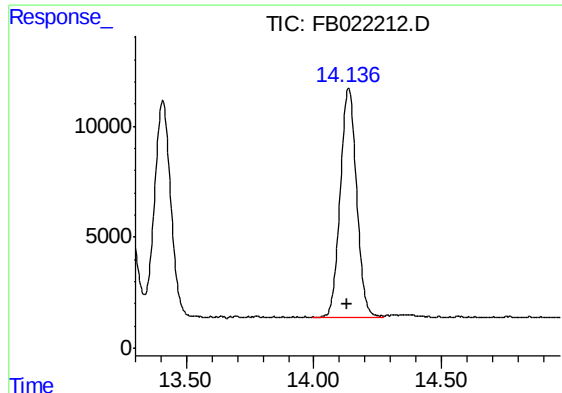

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.005 min
Response: 457682
Conc: 20.46 ng/ml

Instrument :
FID_B
ClientSampleId :
S402-K1-1.0-1.5-082619MSD

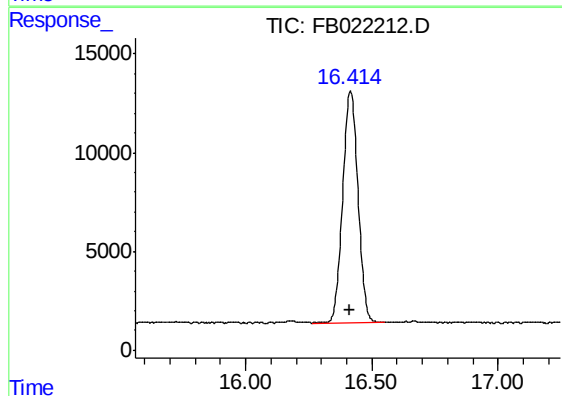

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: 0.004 min
Response: 489511
Conc: 19.09 ng/ml