

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082724\
 Data File : FB030896.D
 Signal(s) : FID2B.CH
 Acq On : 27 Aug 2024 20:14
 Operator : YP/AJ
 Sample : P3751-01MSD
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-CMC-ESLAG-1MSD

Integration File: Calibration.e
 Quant Time: Aug 28 04:10:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	237601	19.638 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	411717	23.041 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	429794	23.441 ng/ml
3) t n-Heptane	7.746	147042	7.951 ng/ml
4) t Benzene	7.883	205207	9.083 ng/ml
6) t Toluene	10.618	578505	26.487 ng/ml
7) t Ethylbenzene	13.054	181185	8.655 ng/ml
8) t m-Xylene	13.187	356515	17.182 ng/ml
9) t O-Xylene	13.914	341290	16.934 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	298988	14.984 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082724\
Data File : FB030896.D
Signal(s) : FID2B.CH
Acq On : 27 Aug 2024 20:14
Operator : YP/AJ
Sample : P3751-01MSD
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-CMC-ESLAG-1MSD

Integration File: Calibration.e
Quant Time: Aug 28 04:10:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

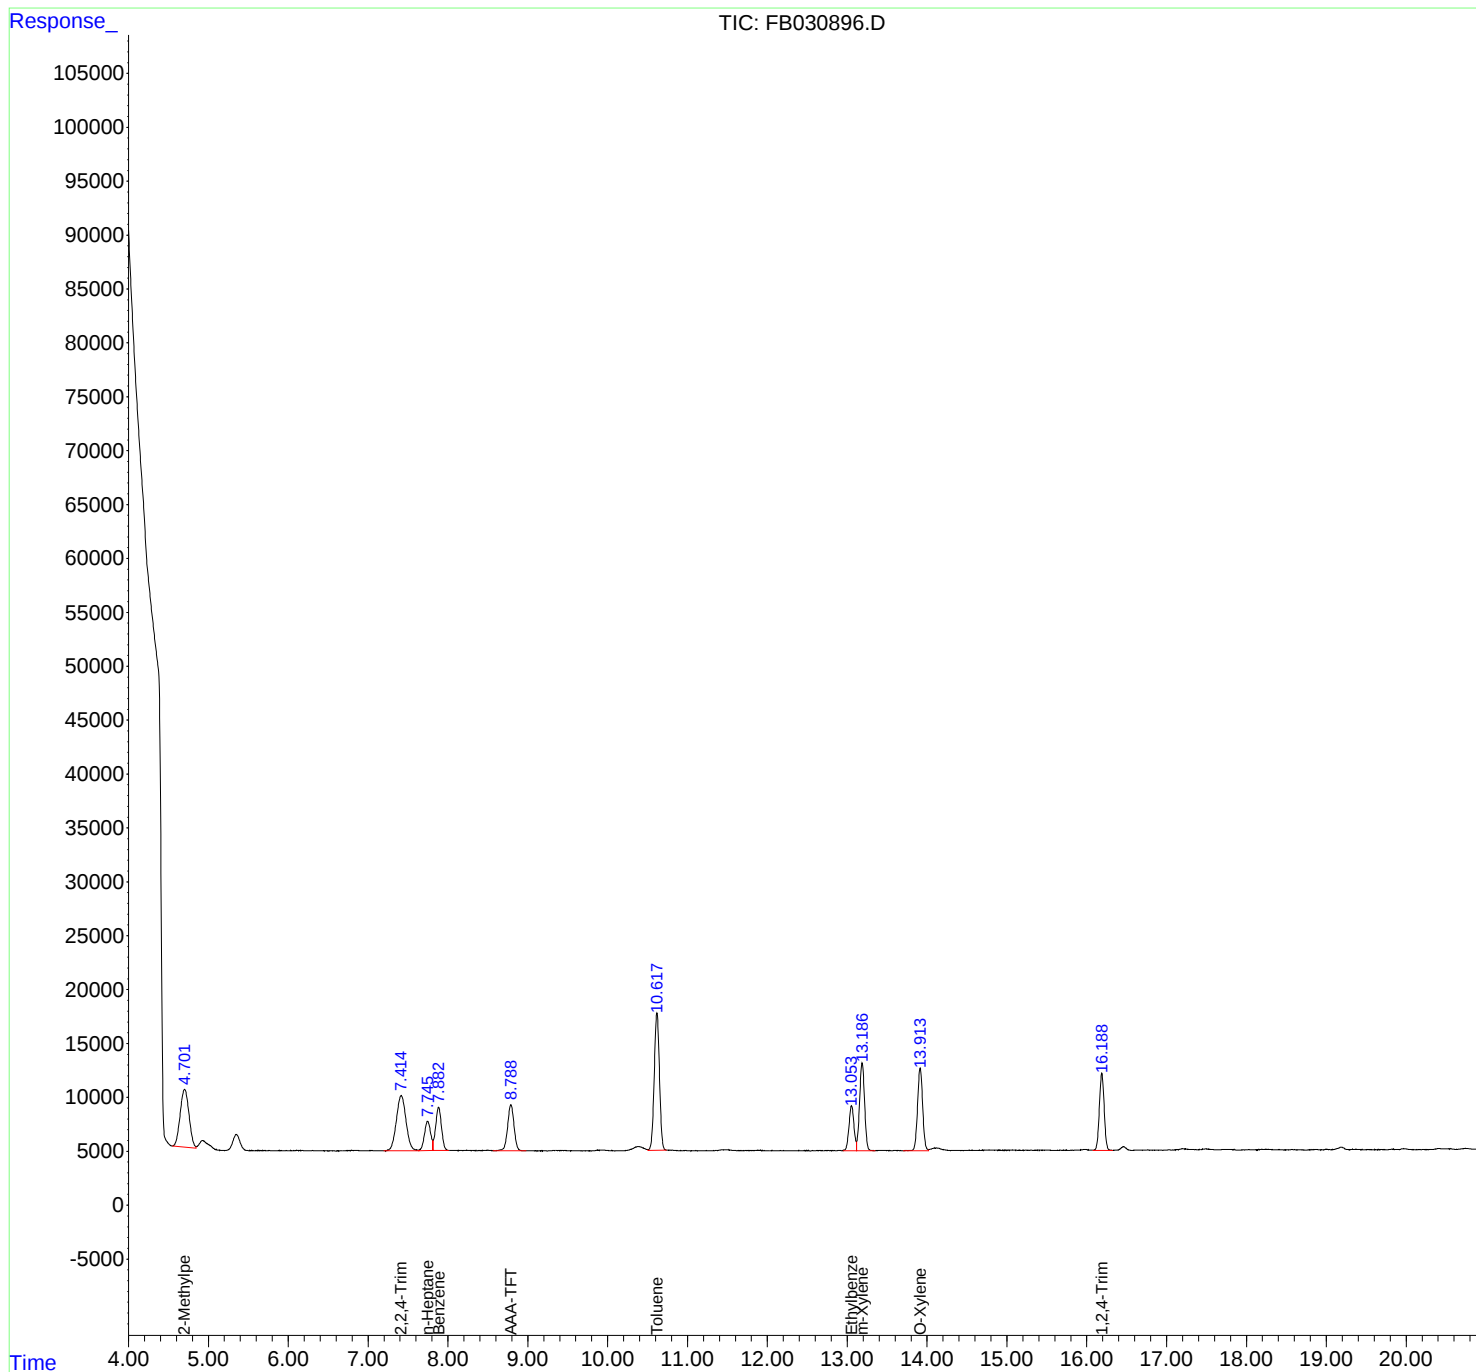


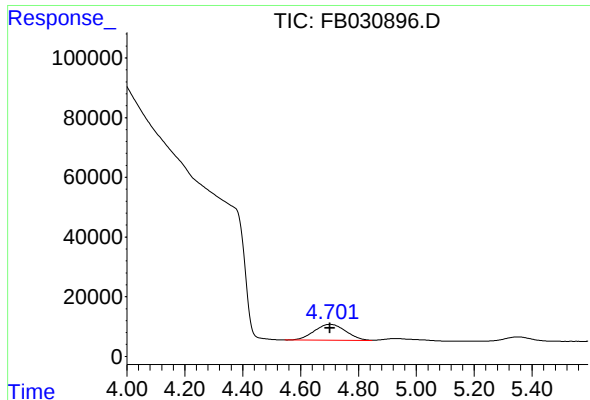

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 411717
Conc: 23.04 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-CMC-ESLAG-1MSD

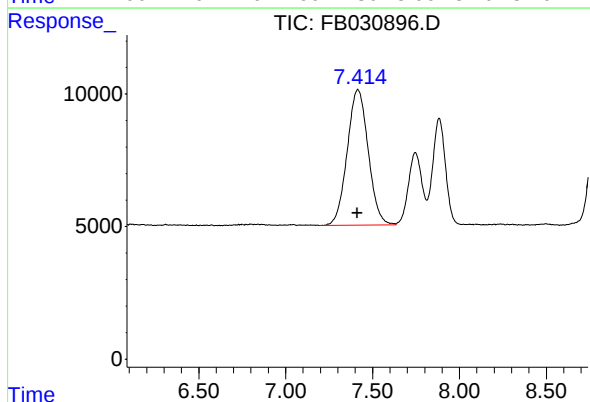


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.004 min
Response: 429794
Conc: 23.44 ng/ml

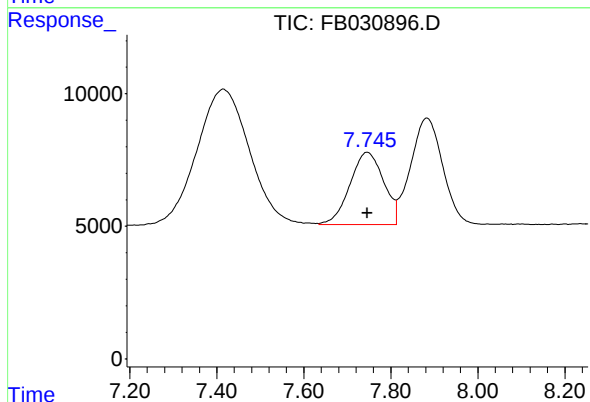


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 147042
Conc: 7.95 ng/ml

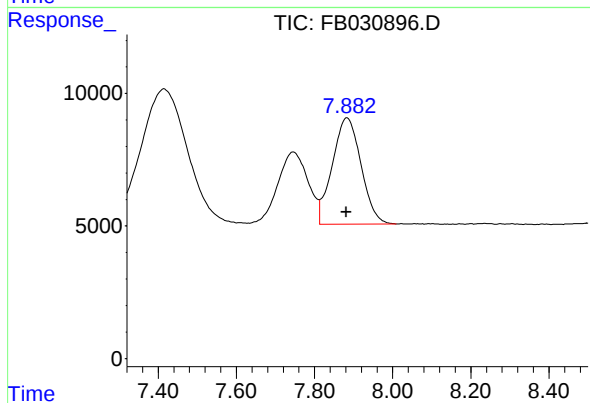

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.002 min
Response: 205207
Conc: 9.08 ng/ml

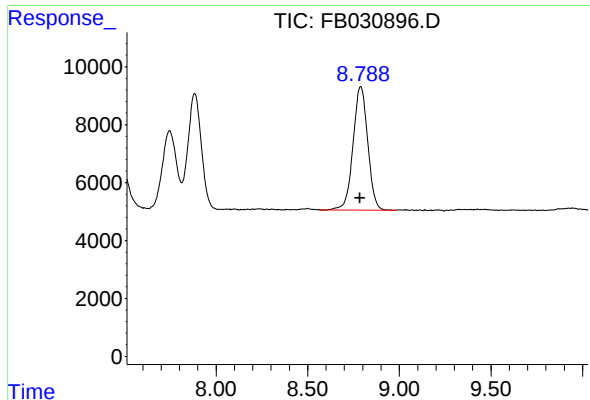

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.003 min
Response: 237601
Conc: 19.64 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-CMC-ESLAG-1MSD

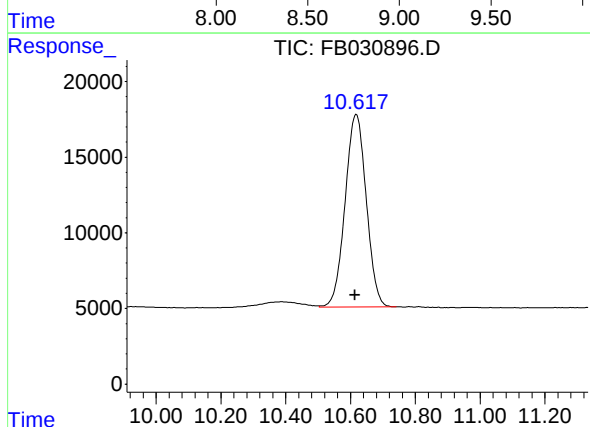


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.004 min
Response: 578505
Conc: 26.49 ng/ml

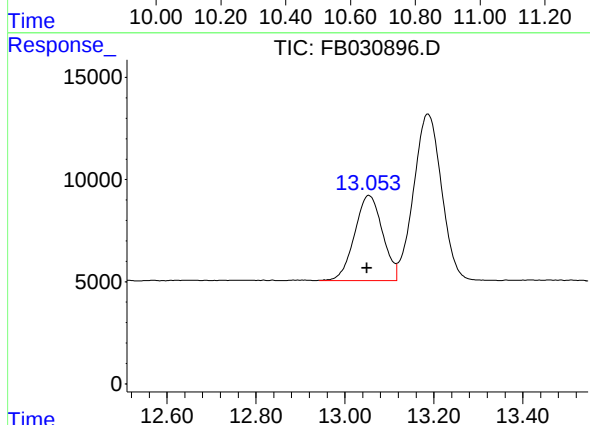


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.004 min
Response: 181185
Conc: 8.66 ng/ml

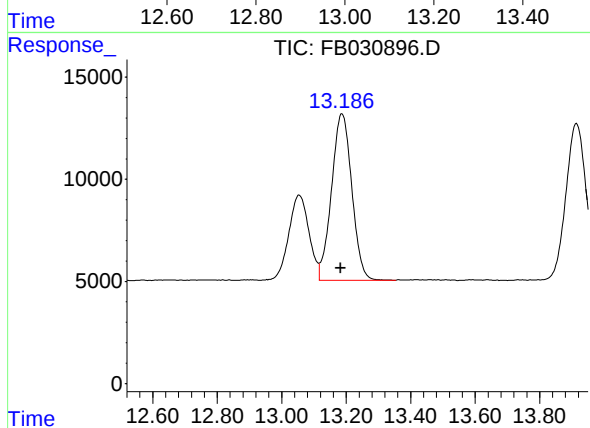

#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: 0.005 min
Response: 356515
Conc: 17.18 ng/ml

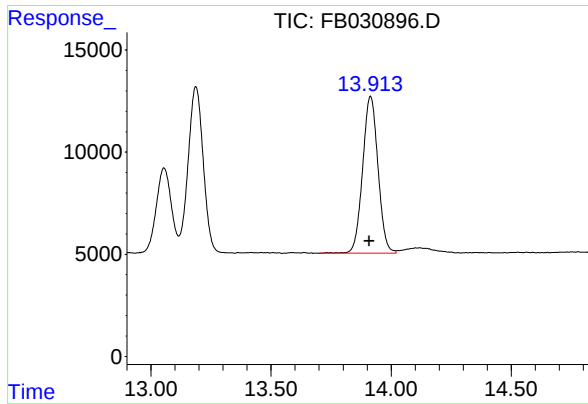

#9 O-Xylene


R.T.: 13.914 min
Delta R.T.: 0.005 min
Response: 341290
Conc: 16.93 ng/ml

Instrument :

FID_B

ClientSampleId :

WC-CMC-ESLAG-1MSD

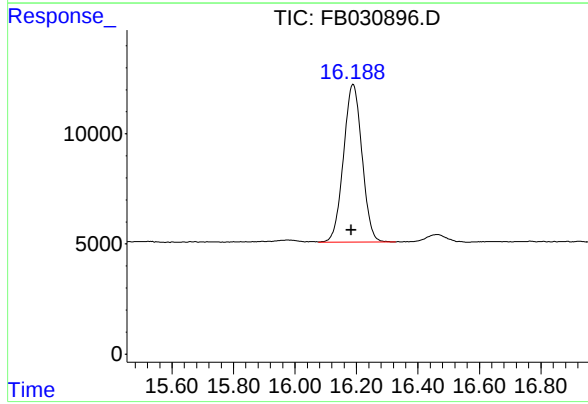

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.005 min
Response: 298988
Conc: 14.98 ng/ml