

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022223.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 9:30
Operator : DD/AJ
Sample : K4571-02
Misc : 5.02/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT-3425

Integration File: Calibration.e
Quant Time: Aug 28 23:19:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	305189	14.368 ng/ml
Target Compounds			
6) t Toluene	10.847	5023	0.163 ng/ml
9) t O-Xylene	14.147	2152	0.096 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	2837	0.111 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022223.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 9:30
Operator : DD/AJ
Sample : K4571-02
Misc : 5.02/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT-3425

Integration File: Calibration.e
Quant Time: Aug 28 23:19:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

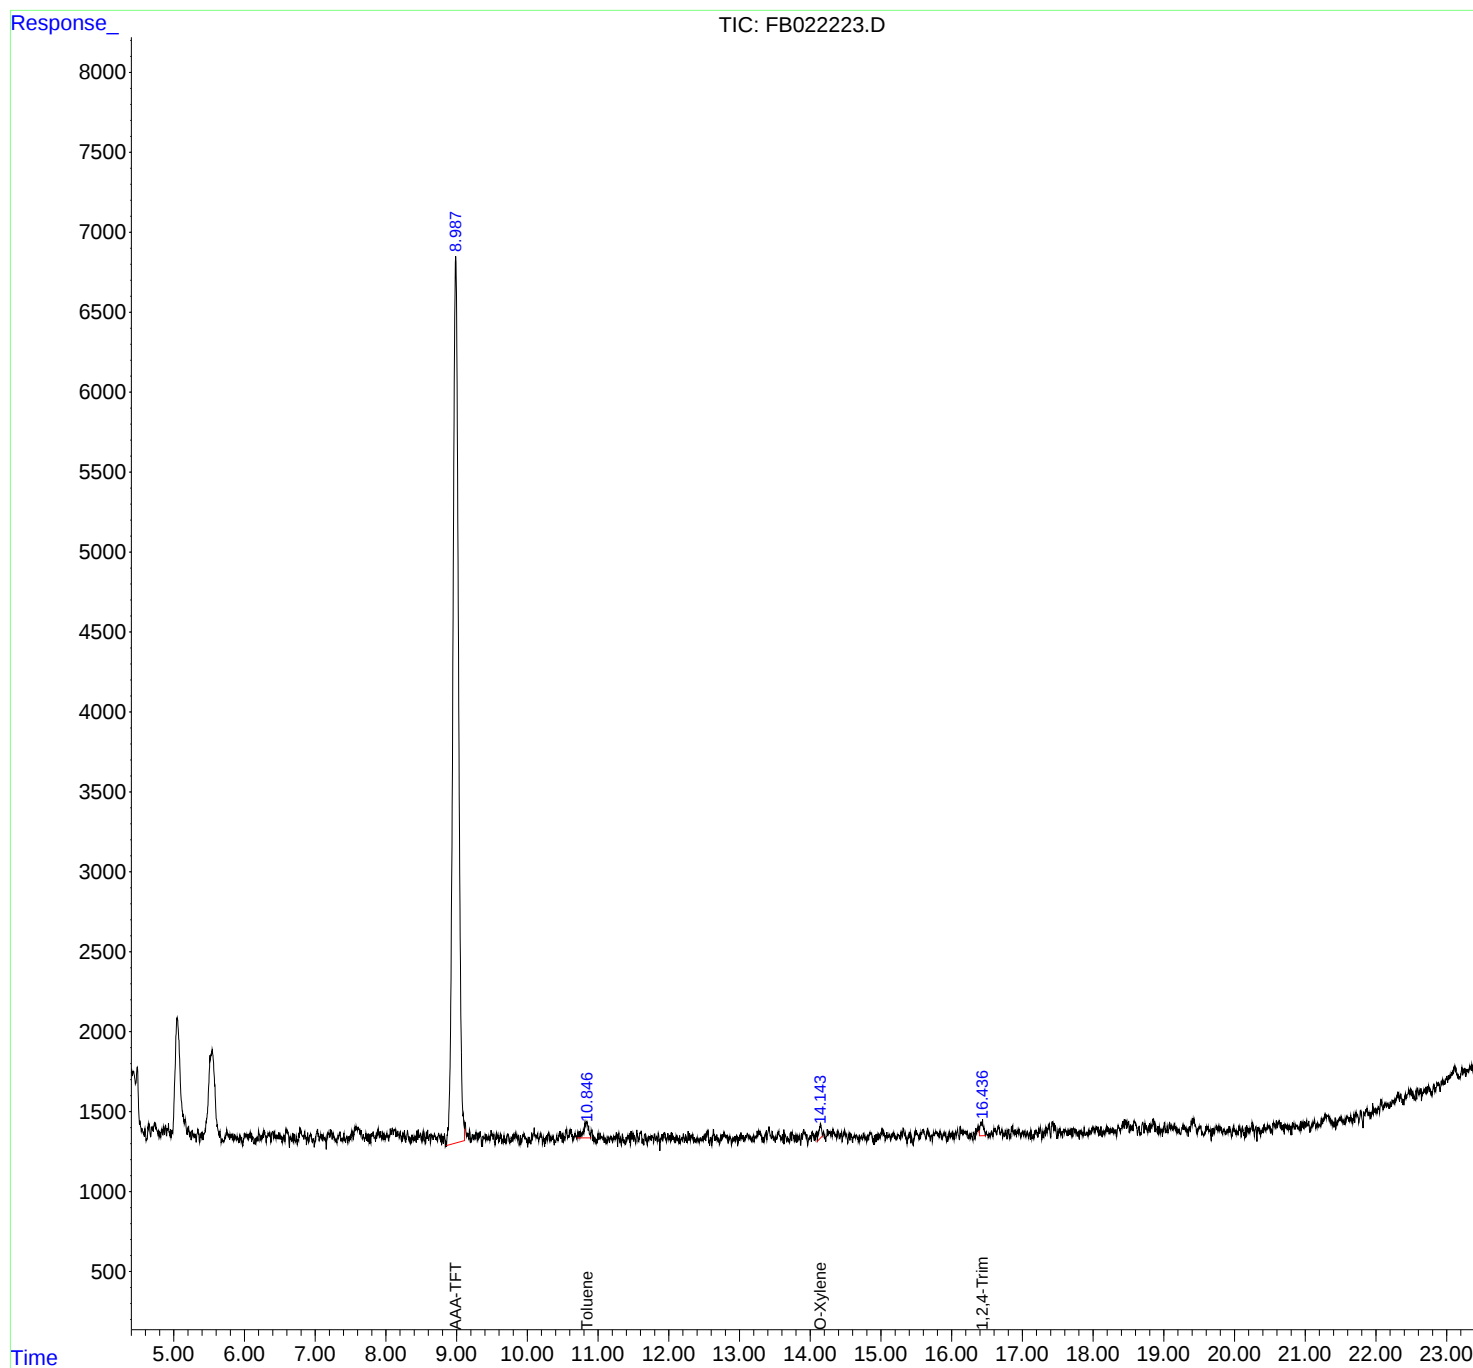


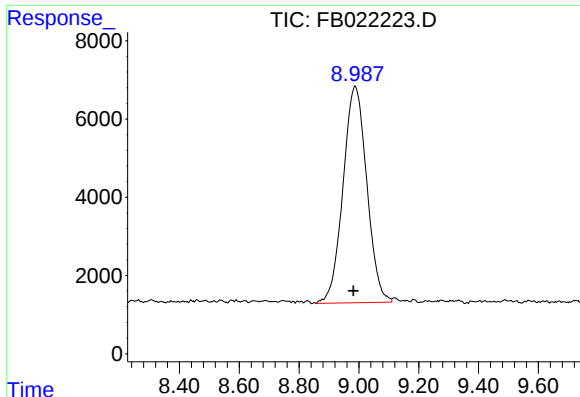

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 305189
Conc: 14.37 ng/ml

Instrument :
FID_B
ClientSampleId :
RT-3425

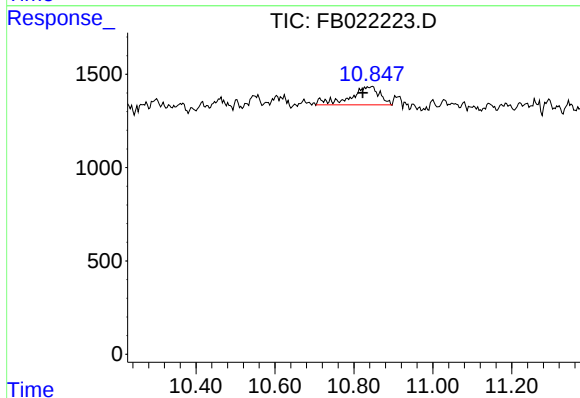


#6 Toluene

R.T.: 10.847 min
Delta R.T.: 0.025 min
Response: 5023
Conc: 0.16 ng/ml

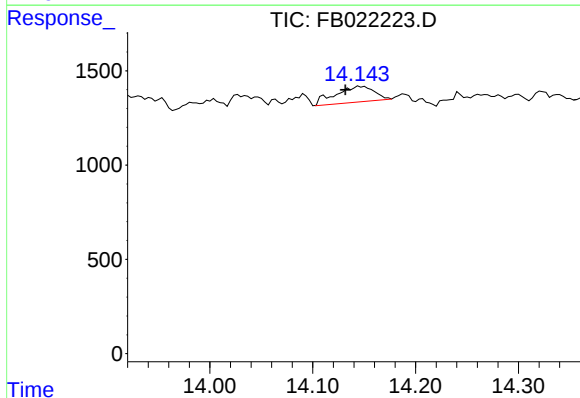

#9 O-Xylene

R.T.: 14.147 min
Delta R.T.: 0.015 min
Response: 2152
Conc: 0.10 ng/ml

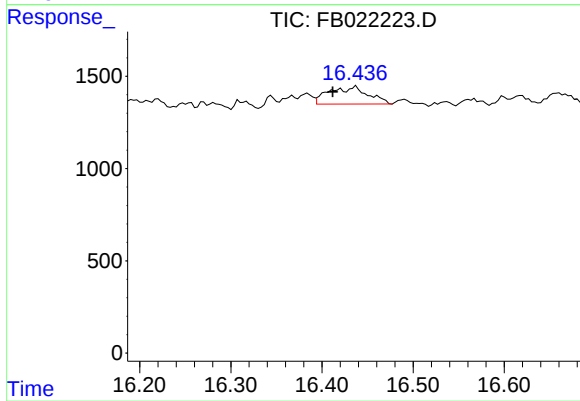

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: 0.025 min
Response: 2837
Conc: 0.11 ng/ml