

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022232.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 14:06
Operator : DD/AJ
Sample : K4568-12
Misc : 5.06/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-19-COMP

Integration File: Calibration.e
Quant Time: Aug 28 23:21:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	96674	4.551 ng/ml
Target Compounds			
9) t O-Xylene	14.090	3894	0.174 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022232.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 14:06
Operator : DD/AJ
Sample : K4568-12
Misc : 5.06/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-19-COMP

Integration File: Calibration.e
Quant Time: Aug 28 23:21:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

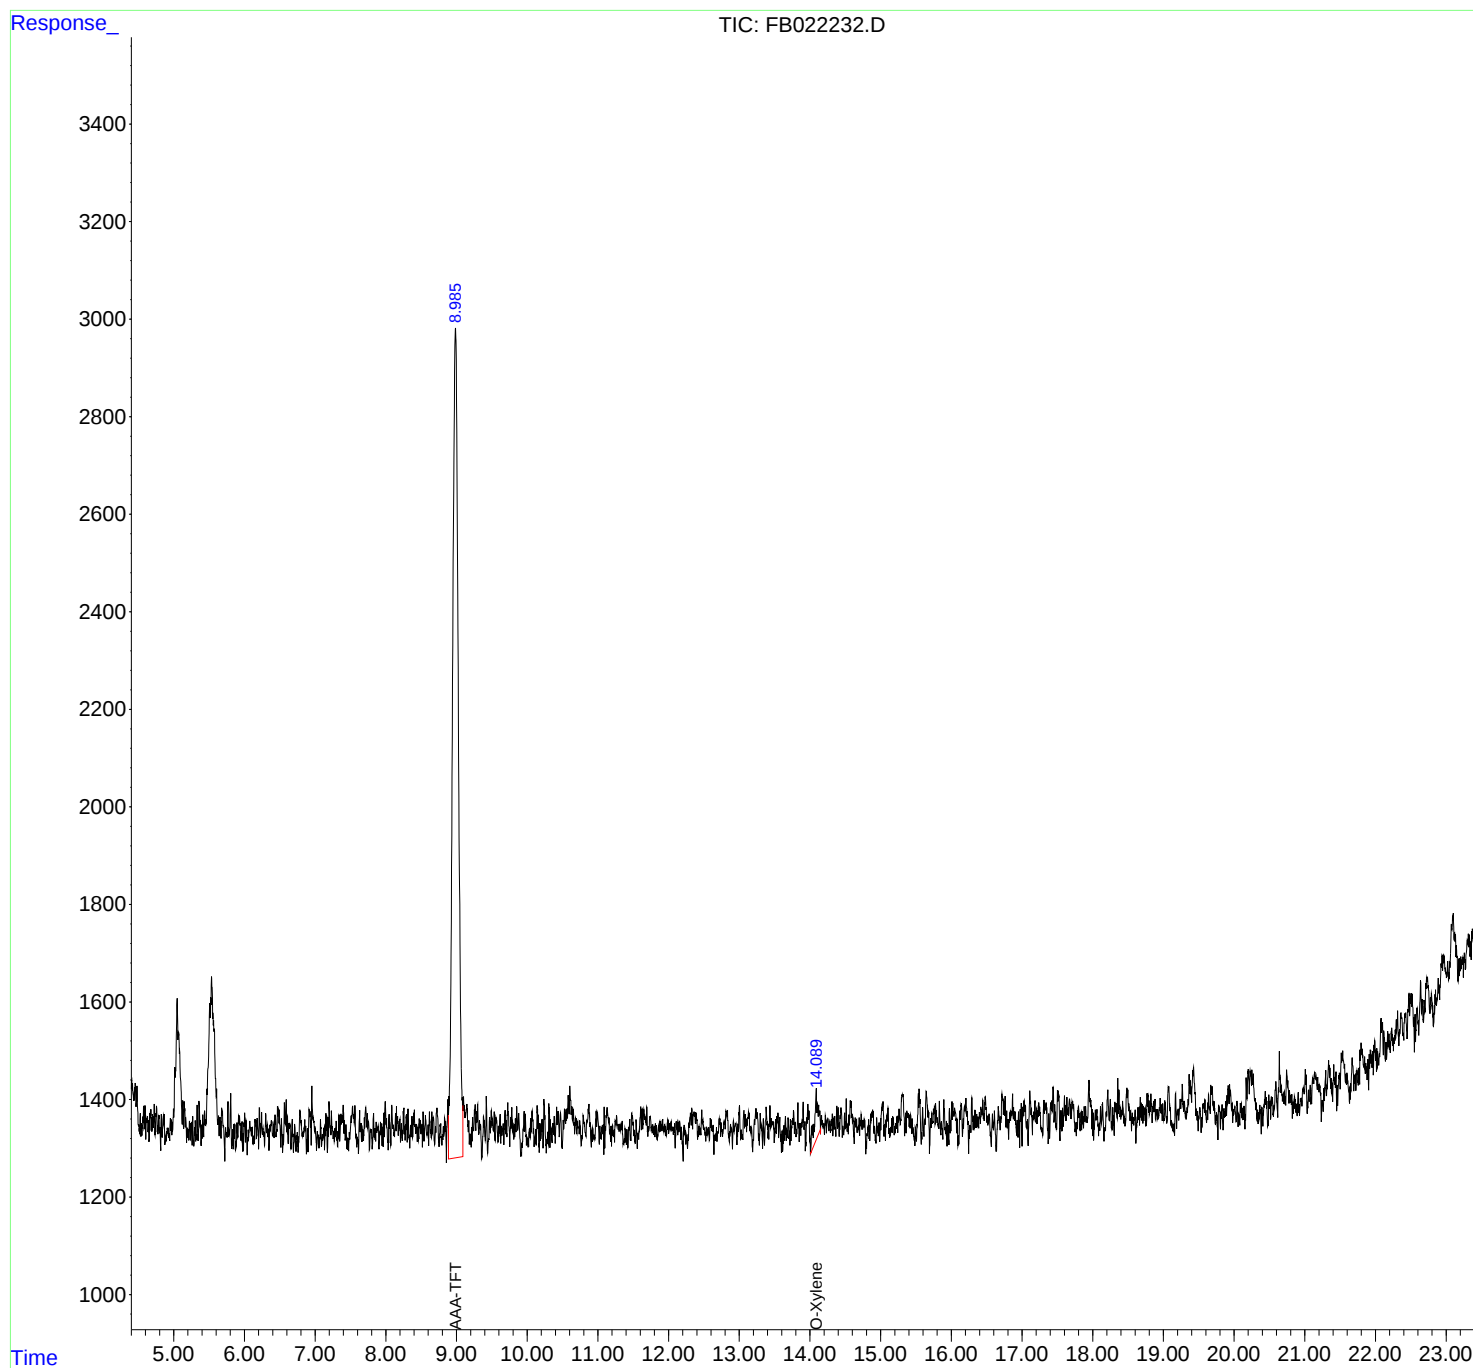


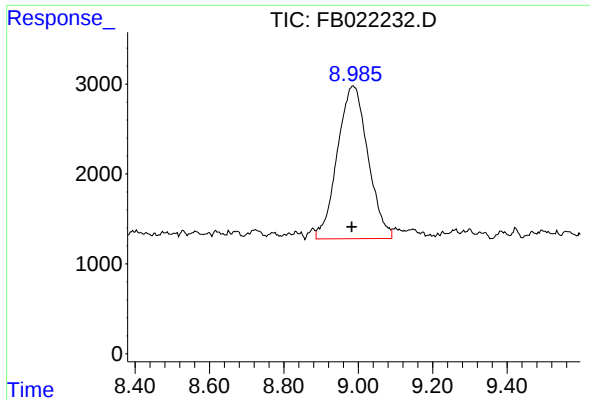

#5 AAA-TFT

R.T.: 8.987 min
Delta R.T.: 0.005 min
Response: 96674
Conc: 4.55 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-19-COMP

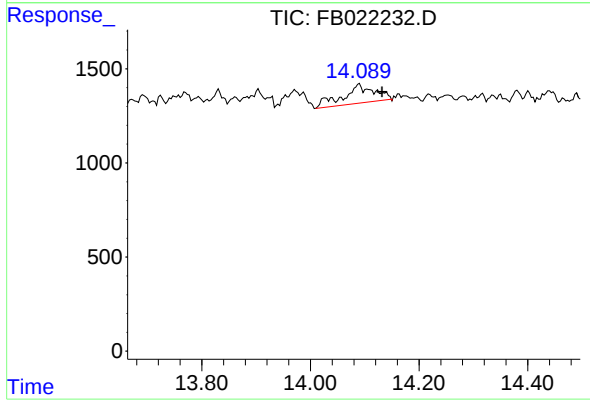

#9 O-Xylene

R.T.: 14.090 min
Delta R.T.: -0.042 min
Response: 3894
Conc: 0.17 ng/ml