

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022234.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 15:07
Operator : DD/AJ
Sample : K4568-16
Misc : 5.01/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-36-COMP

Integration File: Calibration.e
Quant Time: Aug 28 23:21:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.985	416295	19.599 ng/ml
Target Compounds			
9) t O-Xylene	14.083	2150	0.096 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022234.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 15:07
Operator : DD/AJ
Sample : K4568-16
Misc : 5.01/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-36-COMP

Integration File: Calibration.e
Quant Time: Aug 28 23:21:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

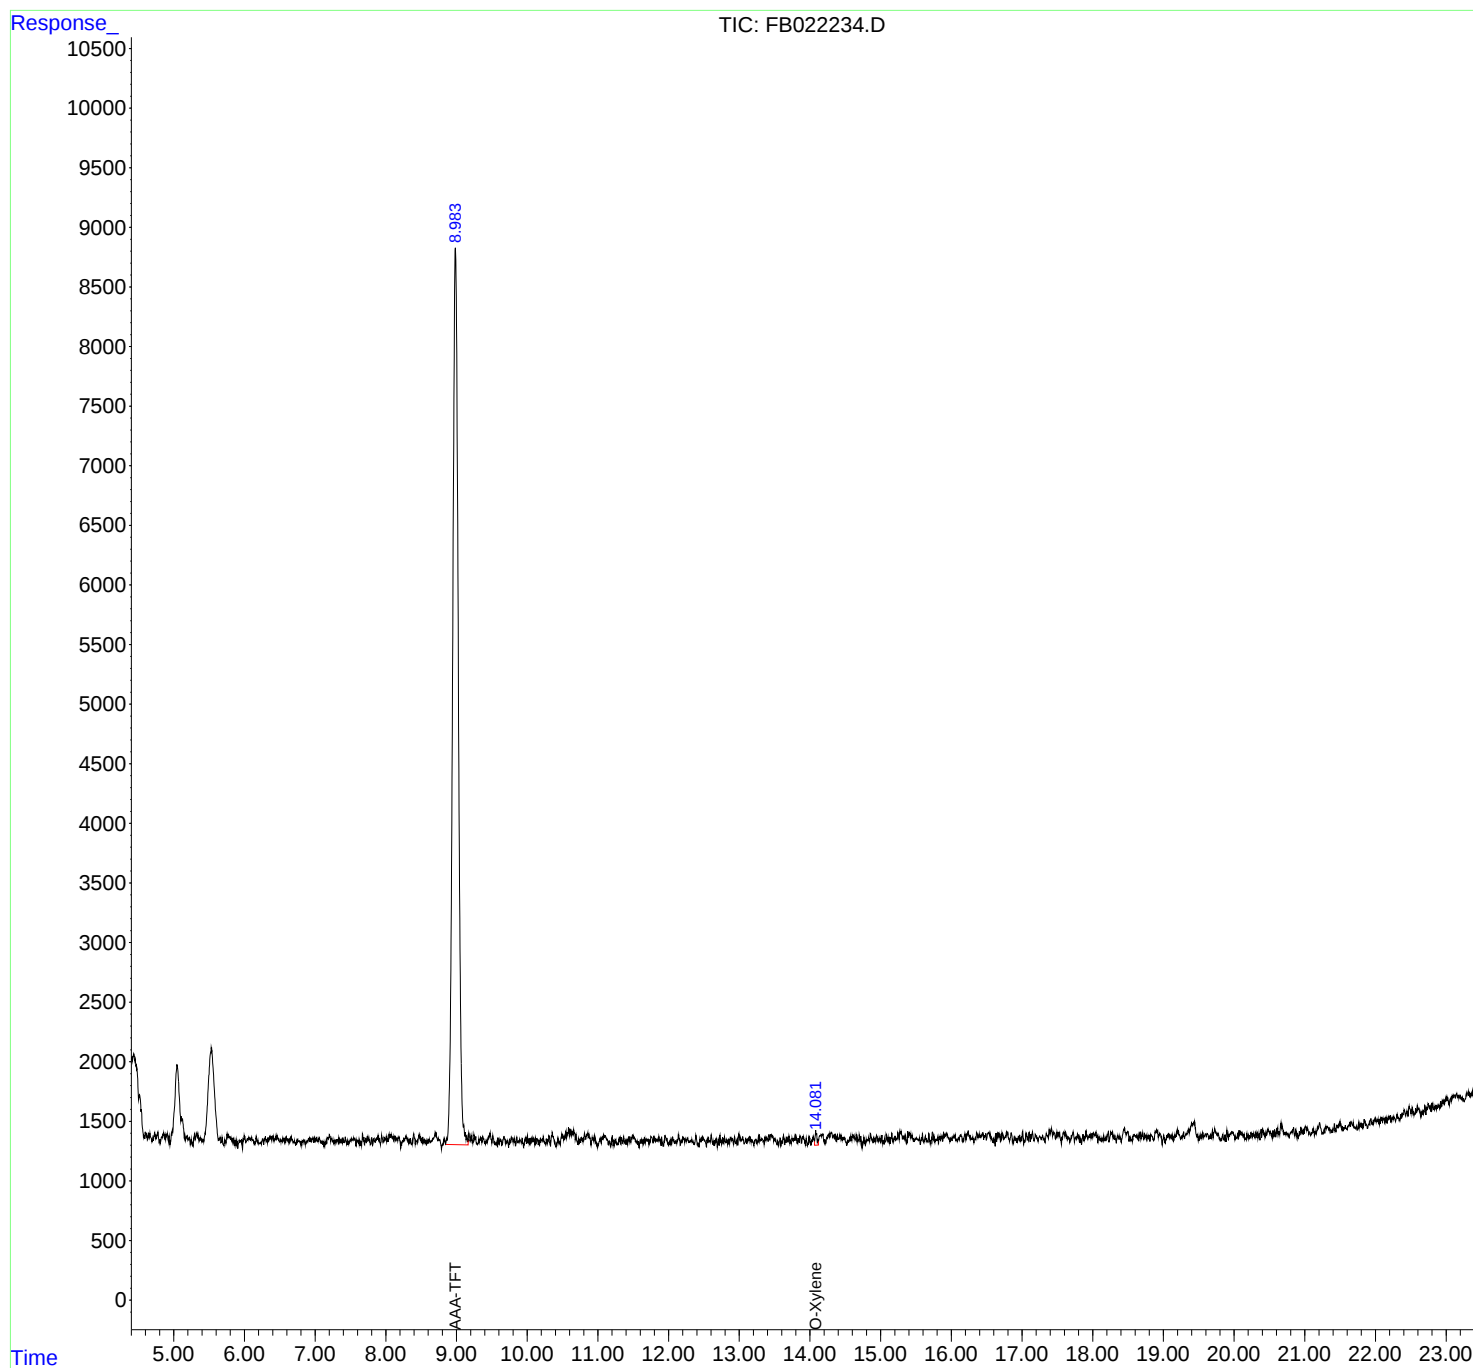


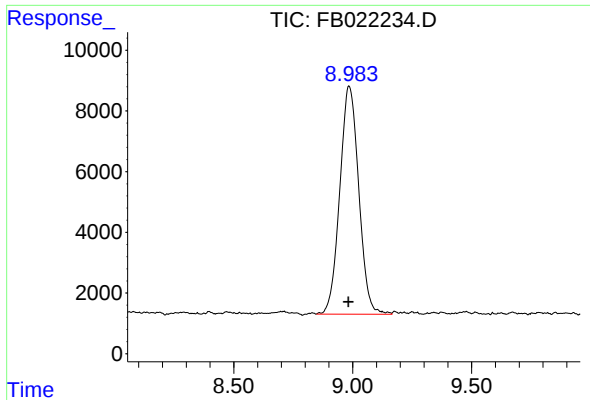

#5 AAA-TFT

R.T.: 8.985 min
Delta R.T.: 0.003 min
Response: 416295
Conc: 19.60 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-36-COMP

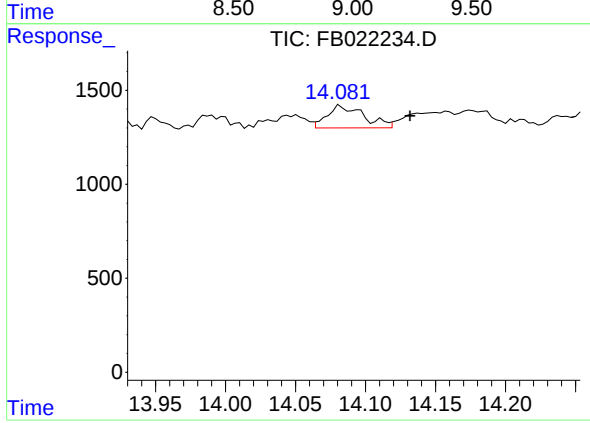

#9 O-Xylene

R.T.: 14.083 min
Delta R.T.: -0.049 min
Response: 2150
Conc: 0.10 ng/ml