

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
 Data File : FB022237.D
 Signal(s) : FID2B.CH
 Acq On : 28 Aug 2019 16:39
 Operator : DD/AJ
 Sample : K4568-18MS
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-35-COMPMS

Integration File: Calibration.e
 Quant Time: Aug 28 23:22:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	426365	20.073 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	1143086	28.561 ng/ml
2) t 2,2,4-Trimethylpentane	7.605	1182140	29.350 ng/ml
3) t n-Heptane	7.944	367442	9.619 ng/ml
4) t Benzene	8.079	426442	9.499 ng/ml
6) t Toluene	10.827	863906	28.102 ng/ml
7) t Ethylbenzene	13.273	219637	10.763 ng/ml
8) t m-Xylene	13.405	446185	21.186 ng/ml
9) t O-Xylene	14.135	468863	20.964 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	521189	20.322 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022237.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 16:39
Operator : DD/AJ
Sample : K4568-18MS
Misc : 5.02/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMS

Integration File: Calibration.e
Quant Time: Aug 28 23:22:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

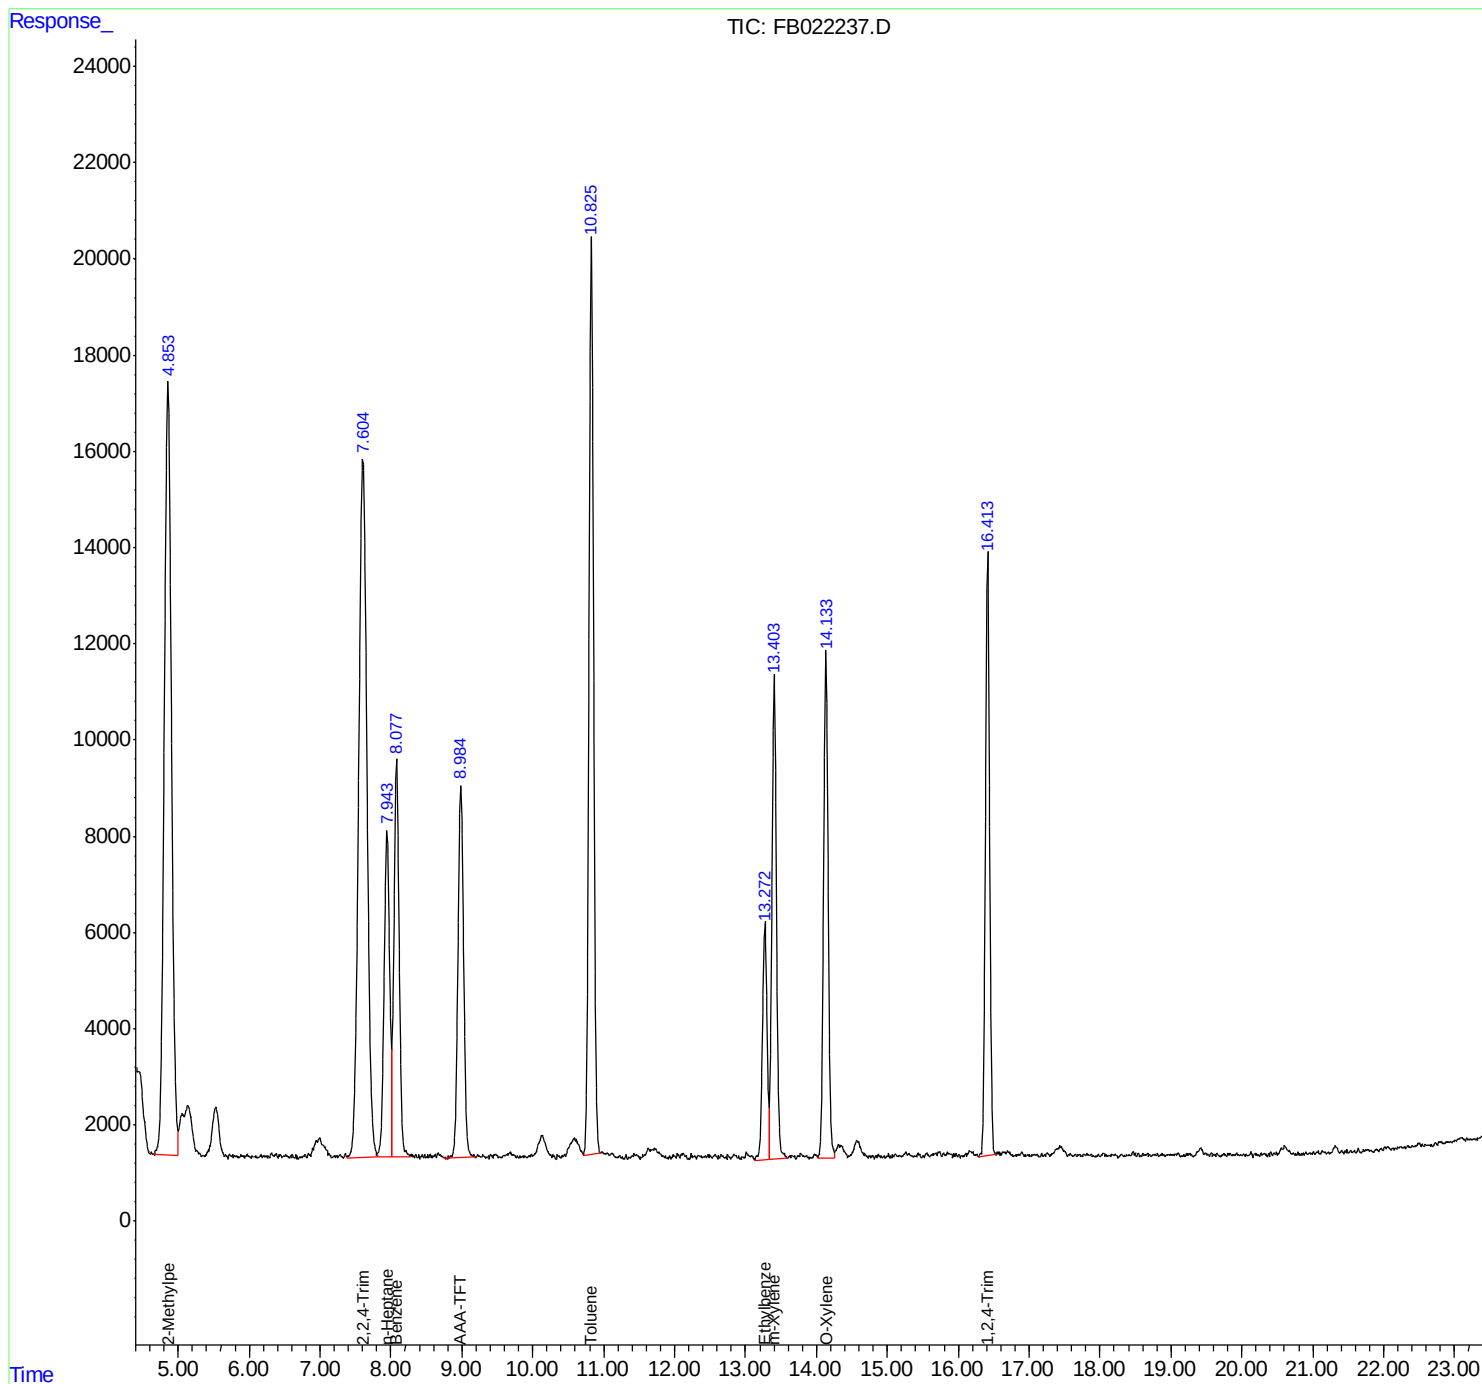


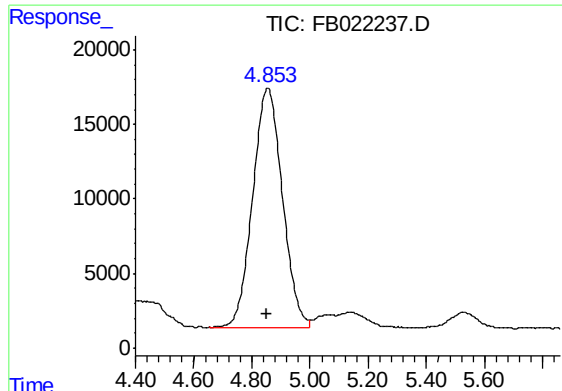

#1 2-Methylpentane


R.T.: 4.855 min
Delta R.T.: 0.003 min
Response: 1143086
Conc: 28.56 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMS

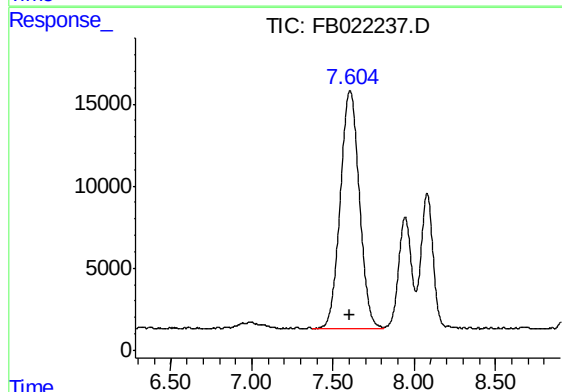


#2 2,2,4-Trimethylpentane

R.T.: 7.605 min
Delta R.T.: 0.005 min
Response: 1182140
Conc: 29.35 ng/ml

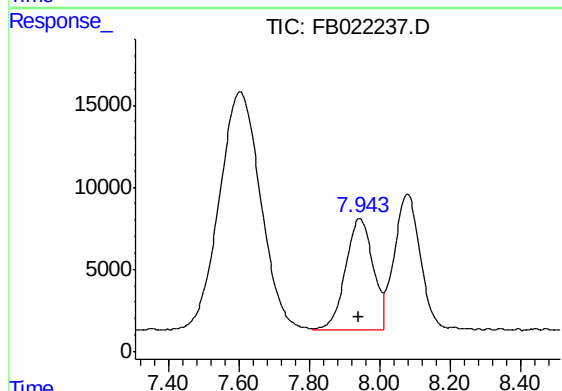


#3 n-Heptane

R.T.: 7.944 min
Delta R.T.: 0.003 min
Response: 367442
Conc: 9.62 ng/ml

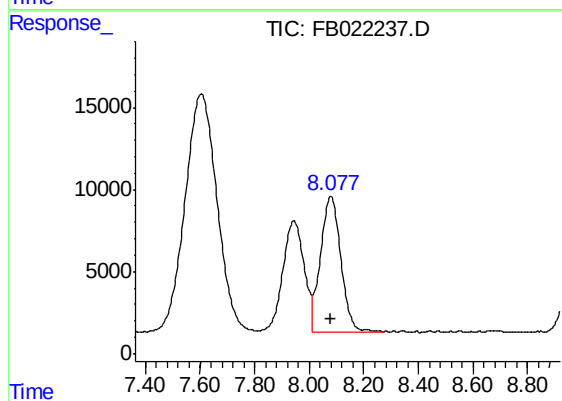

#4 Benzene


R.T.: 8.079 min
Delta R.T.: 0.003 min
Response: 426442
Conc: 9.50 ng/ml

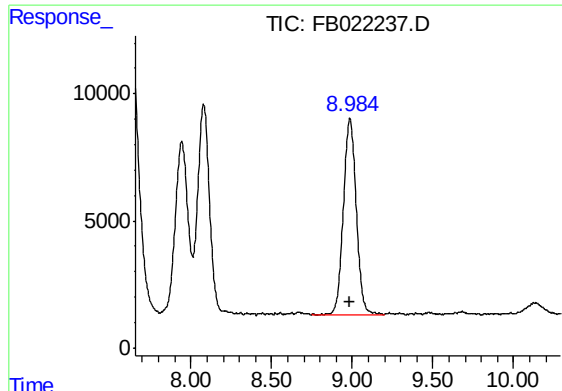

#5 AAA-TFT


R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 426365
Conc: 20.07 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMS

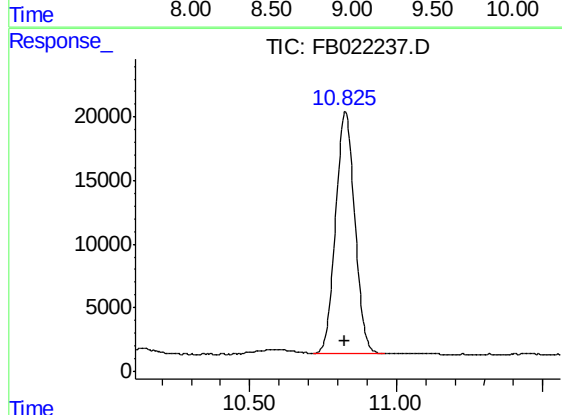


#6 Toluene

R.T.: 10.827 min
Delta R.T.: 0.004 min
Response: 863906
Conc: 28.10 ng/ml

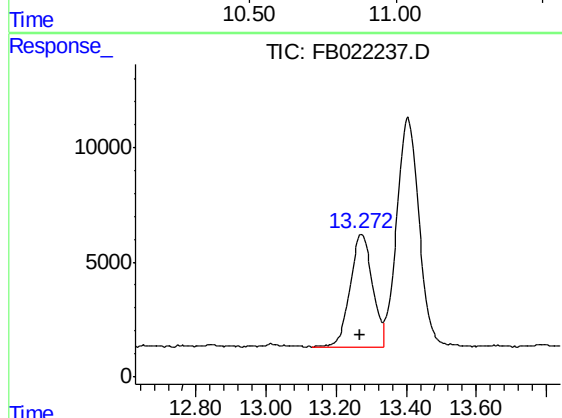


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.003 min
Response: 219637
Conc: 10.76 ng/ml

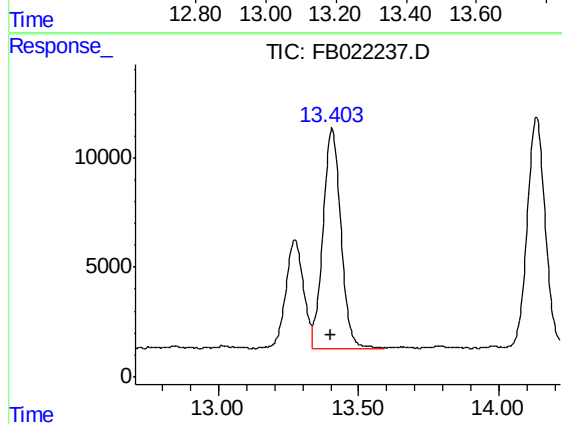

#8 m-Xylene


R.T.: 13.405 min
Delta R.T.: 0.003 min
Response: 446185
Conc: 21.19 ng/ml

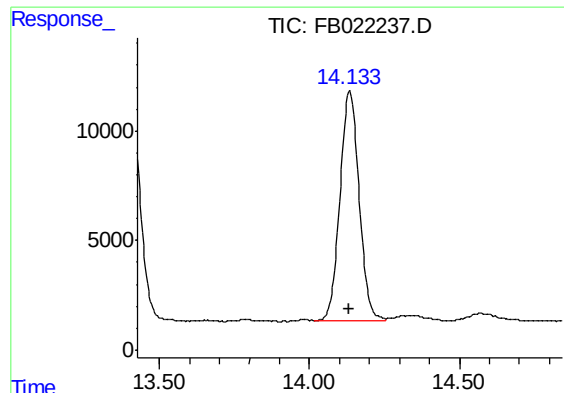

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.003 min
Response: 468863
Conc: 20.96 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMS

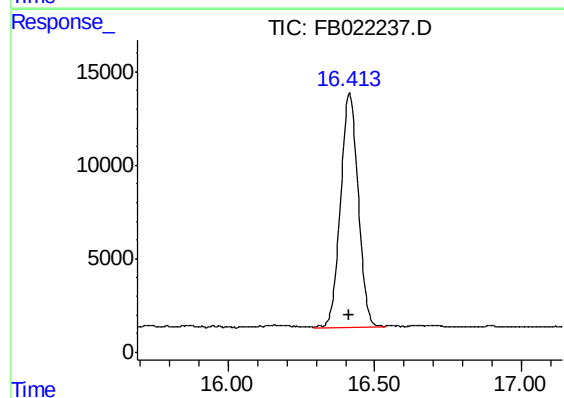

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.002 min
Response: 521189
Conc: 20.32 ng/ml