

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
 Data File : FB022238.D
 Signal(s) : FID2B.CH
 Acq On : 28 Aug 2019 17:10
 Operator : DD/AJ
 Sample : K4568-18MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-35-COMPMSD

Integration File: Calibration.e
 Quant Time: Aug 28 23:22:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	434915	20.476 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	1170549	29.247 ng/ml
2) t 2,2,4-Trimethylpentane	7.604	1204960	29.916 ng/ml
3) t n-Heptane	7.944	375721	9.836 ng/ml
4) t Benzene	8.080	448300	9.986 ng/ml
6) t Toluene	10.827	886284	28.830 ng/ml
7) t Ethylbenzene	13.273	214600	10.516 ng/ml
8) t m-Xylene	13.406	444885	21.124 ng/ml
9) t O-Xylene	14.135	468810	20.962 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	522735	20.383 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082819\
Data File : FB022238.D
Signal(s) : FID2B.CH
Acq On : 28 Aug 2019 17:10
Operator : DD/AJ
Sample : K4568-18MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMSD

Integration File: Calibration.e
Quant Time: Aug 28 23:22:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

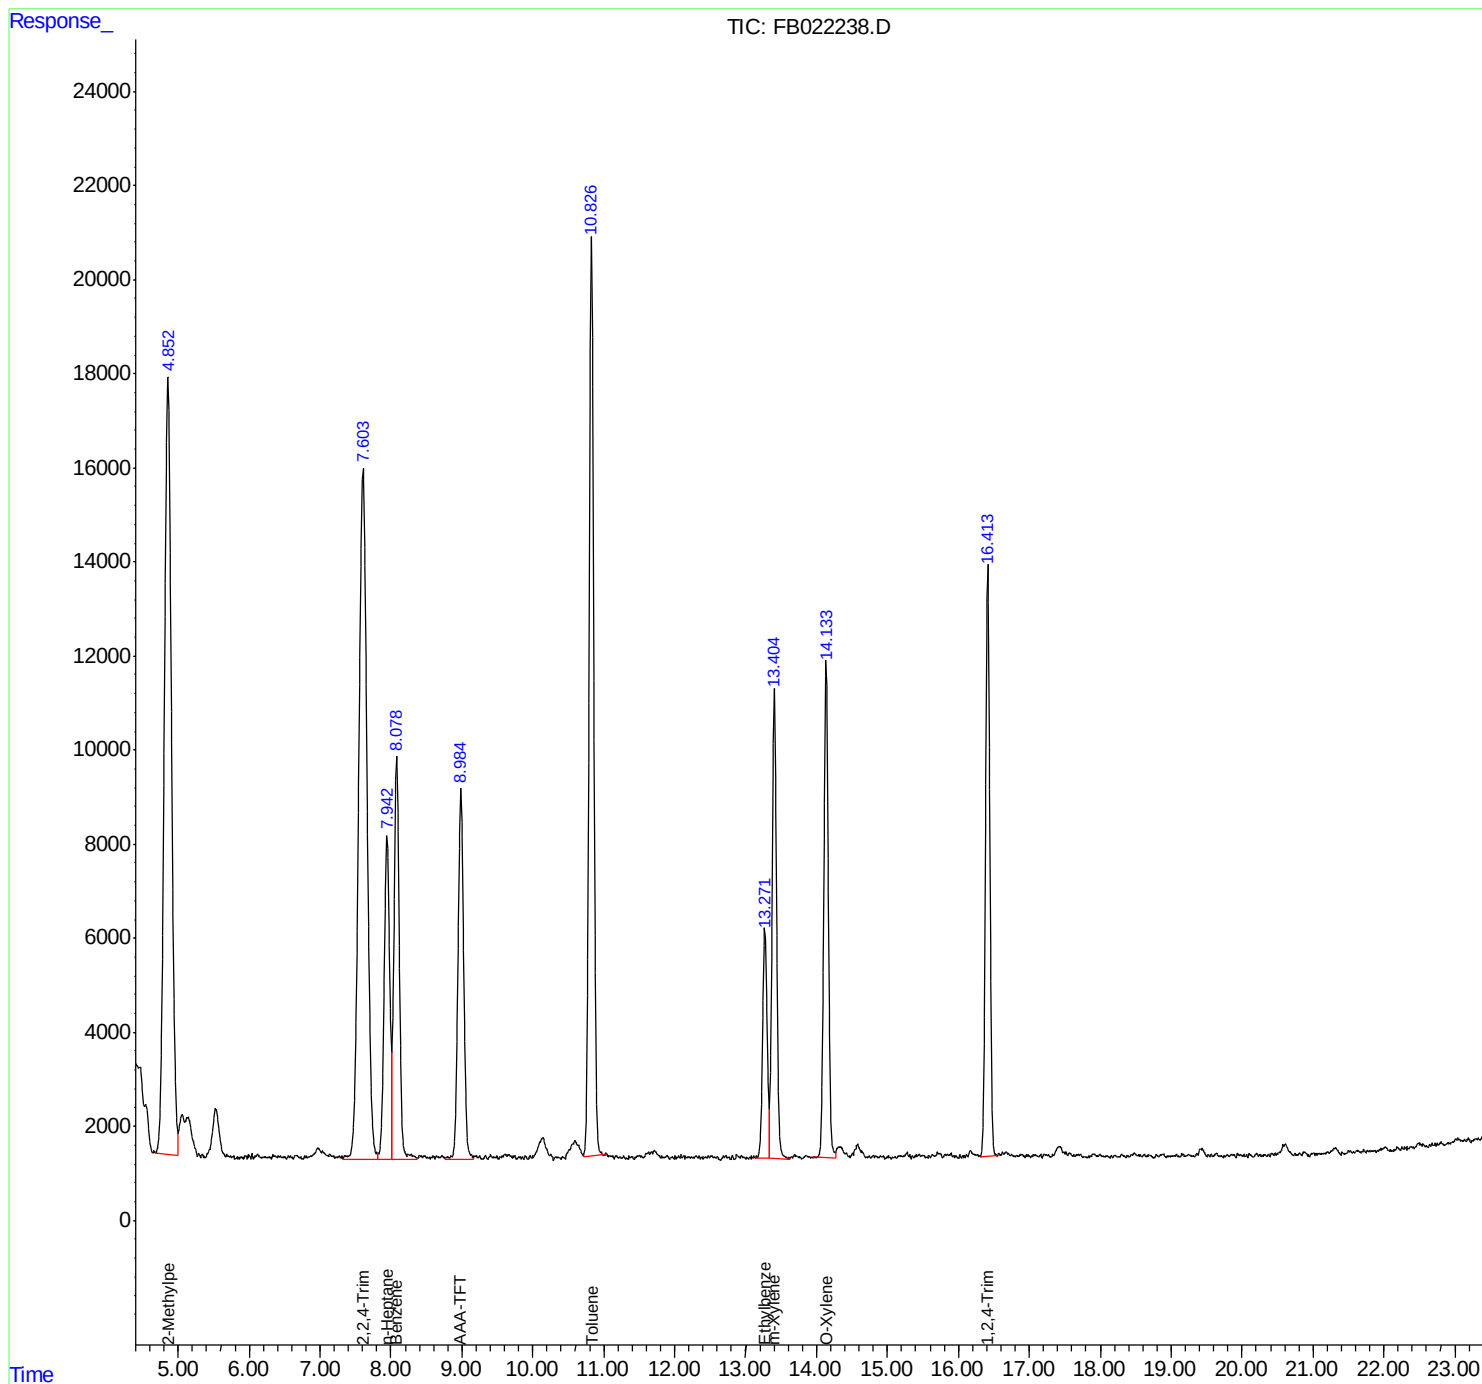


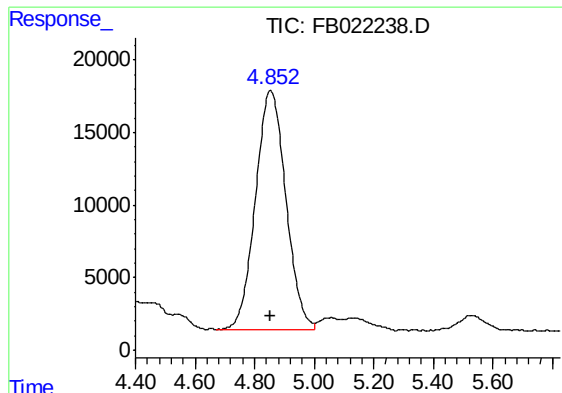

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: 0.002 min
Response: 1170549
Conc: 29.25 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMSD

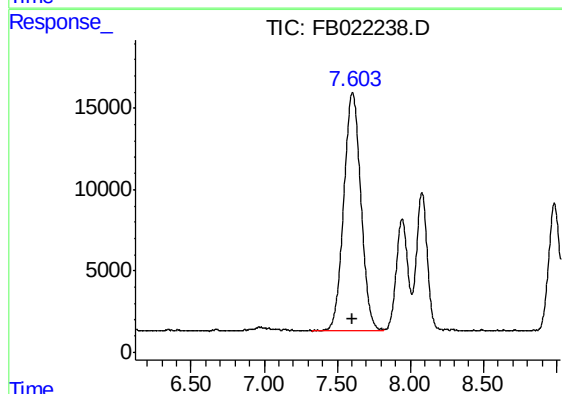


#2 2,2,4-Trimethylpentane

R.T.: 7.604 min
Delta R.T.: 0.004 min
Response: 1204960
Conc: 29.92 ng/ml

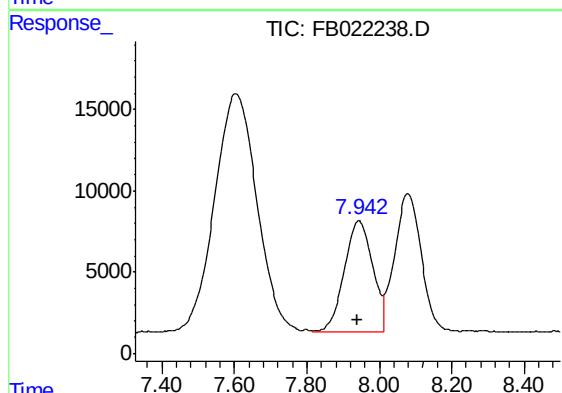


#3 n-Heptane

R.T.: 7.944 min
Delta R.T.: 0.003 min
Response: 375721
Conc: 9.84 ng/ml

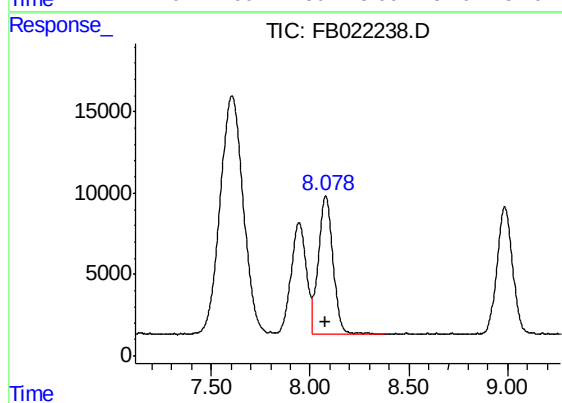

#4 Benzene


R.T.: 8.080 min
Delta R.T.: 0.003 min
Response: 448300
Conc: 9.99 ng/ml

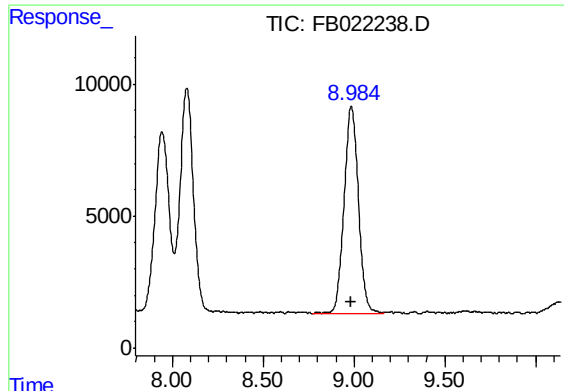

#5 AAA-TFT


R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 434915
Conc: 20.48 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMSD

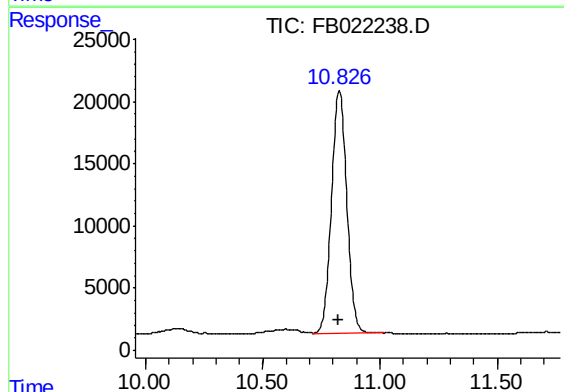


#6 Toluene

R.T.: 10.827 min
Delta R.T.: 0.004 min
Response: 886284
Conc: 28.83 ng/ml

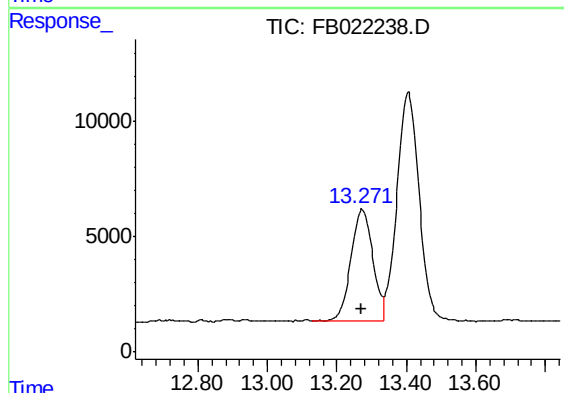


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.003 min
Response: 214600
Conc: 10.52 ng/ml

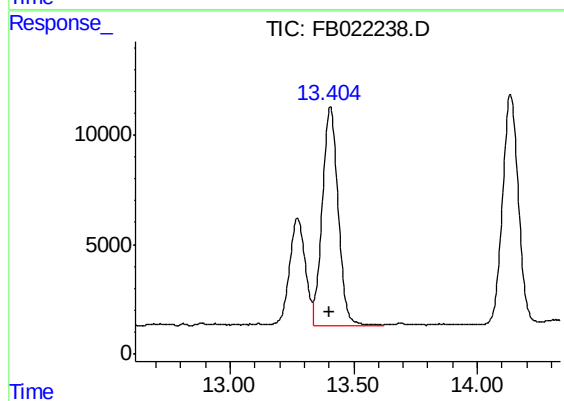

#8 m-Xylene


R.T.: 13.406 min
Delta R.T.: 0.004 min
Response: 444885
Conc: 21.12 ng/ml

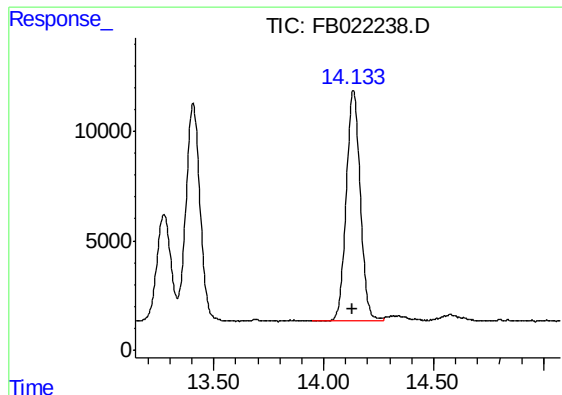

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.004 min
Response: 468810
Conc: 20.96 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-35-COMPMSD

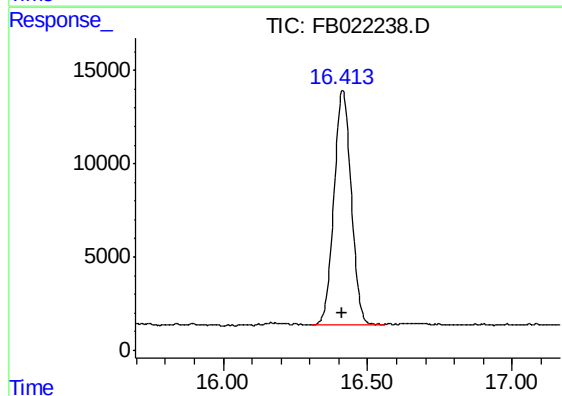

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: 0.003 min
Response: 522735
Conc: 20.38 ng/ml