

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082918\
 Data File : FB017572.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2018 13:15
 Operator : MJ/SJ
 Sample : BSF0829S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 30 08:00:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	170467	20.676 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	404254	28.850 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	415110	29.457 ng/ml
3) t n-Heptane	8.068	122902	8.918 ng/ml
4) t Benzene	8.207	170365	9.663 ng/ml
6) t Toluene	10.961	421839	29.323 ng/ml
7) t Ethylbenzene	13.411	138437	9.387 ng/ml
8) t m-Xylene	13.543	292191	18.796 ng/ml
9) t O-Xylene	14.275	307155	18.711 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	370821	19.039 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082918\
Data File : FB017572.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2018 13:15
Operator : MJ/SJ
Sample : BSF0829S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 30 08:00:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

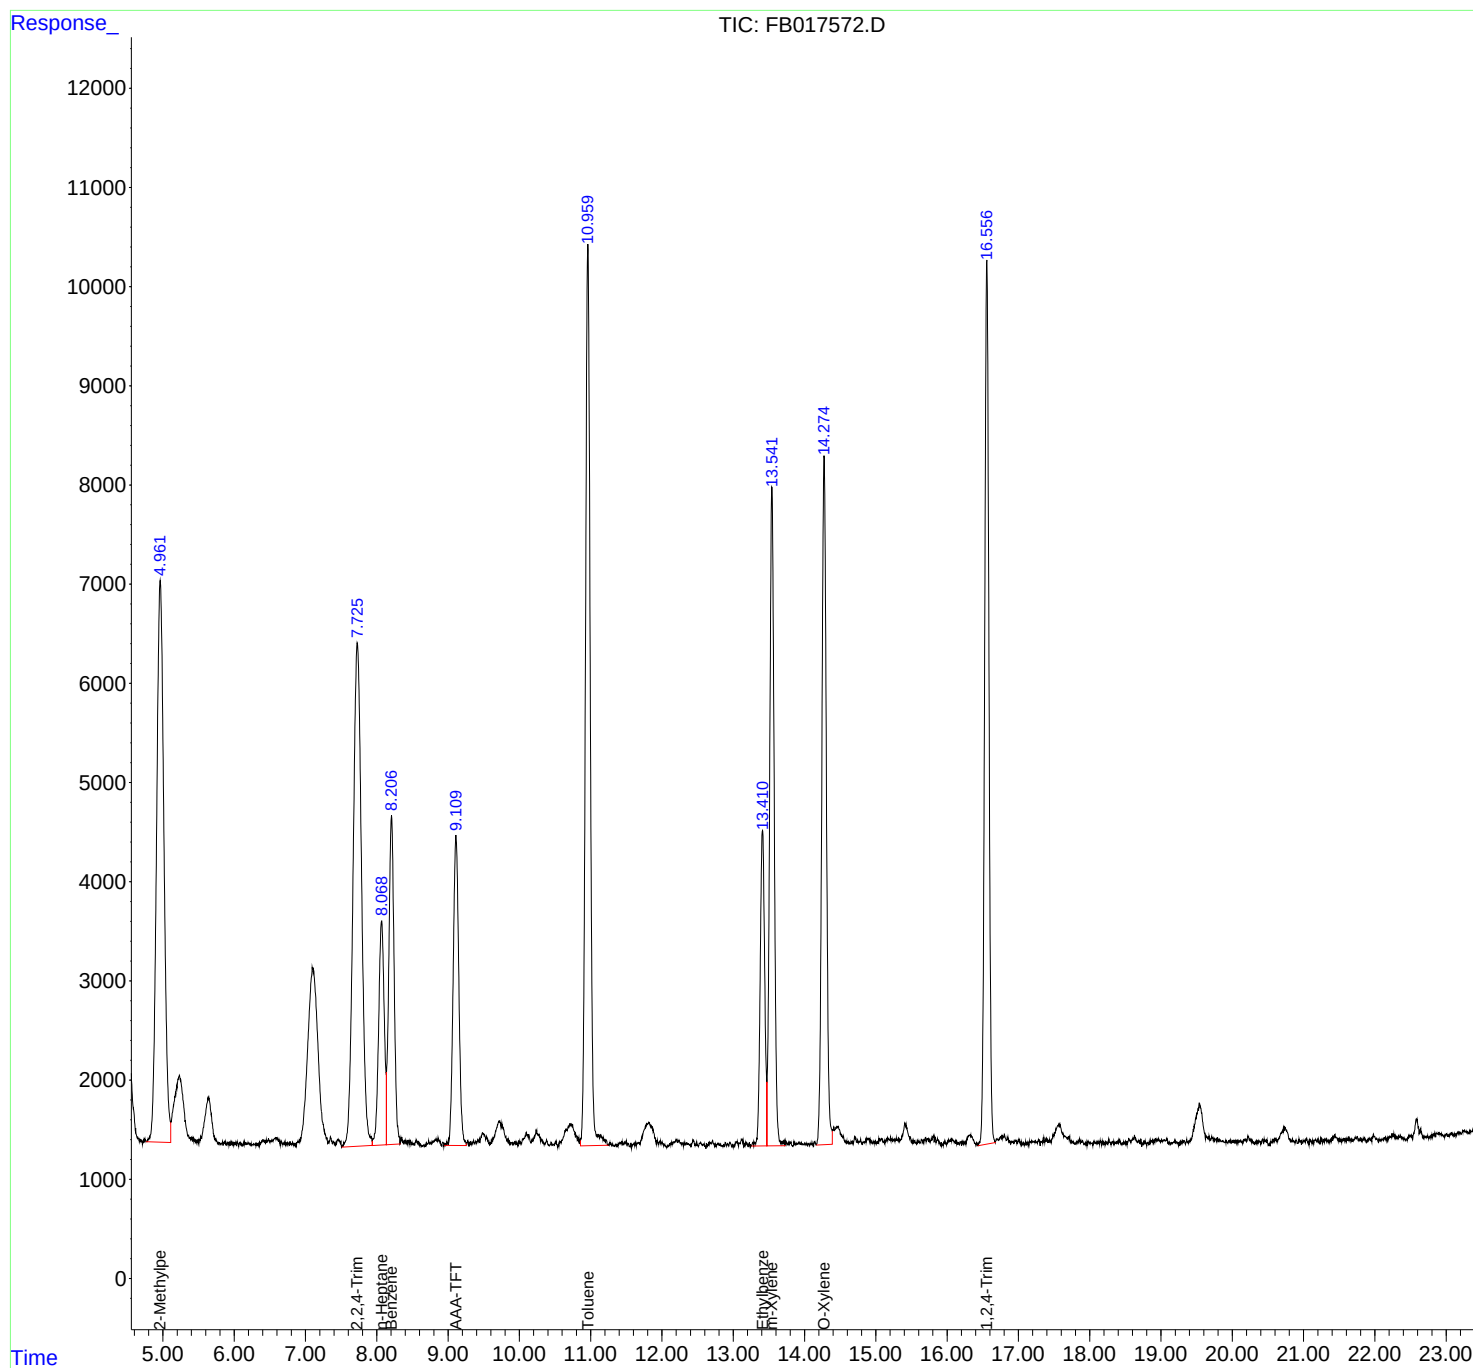

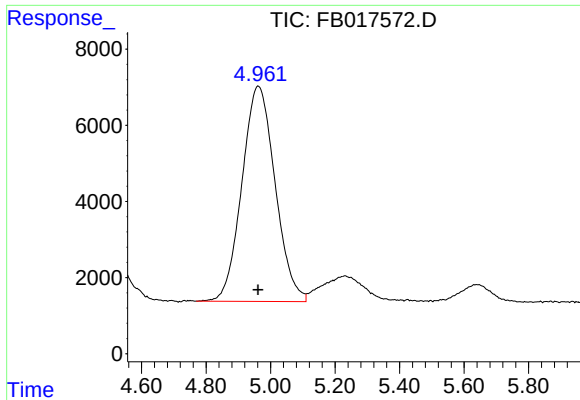


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.001 min
Response: 404254
Conc: 28.85 ng/ml

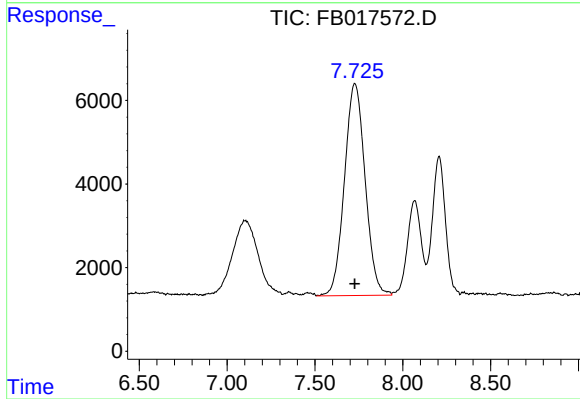


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 415110
Conc: 29.46 ng/ml

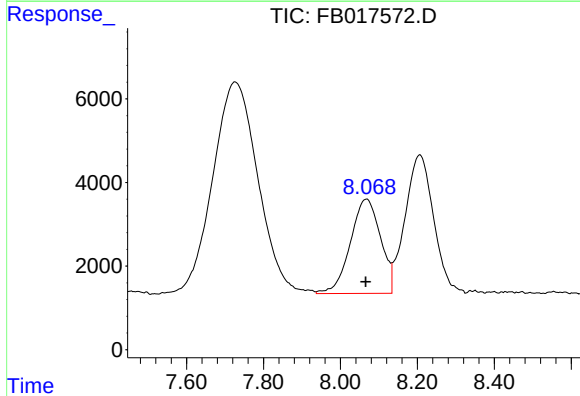


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.002 min
Response: 122902
Conc: 8.92 ng/ml

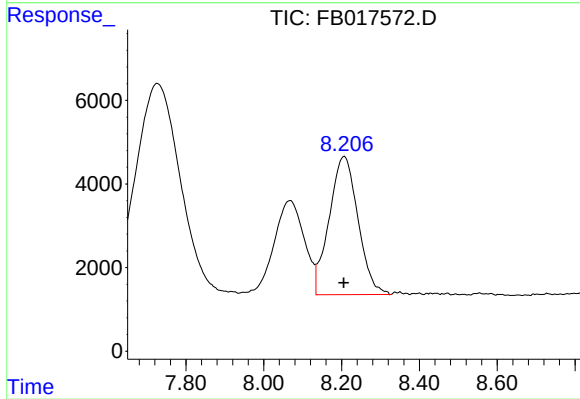


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.002 min
Response: 170365
Conc: 9.66 ng/ml

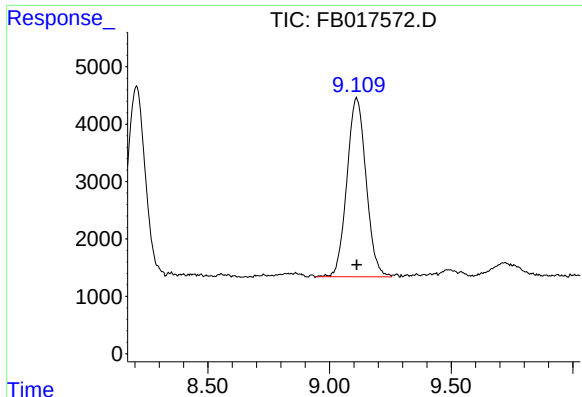


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 170467
Conc: 20.68 ng/ml

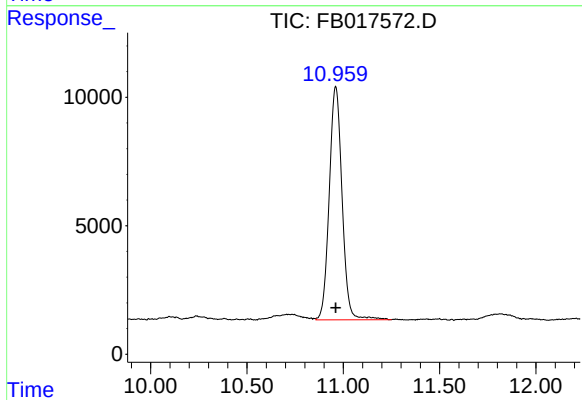


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 421839
Conc: 29.32 ng/ml

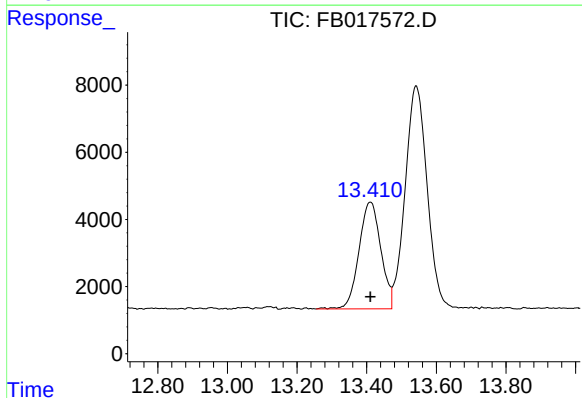


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.000 min
Response: 138437
Conc: 9.39 ng/ml

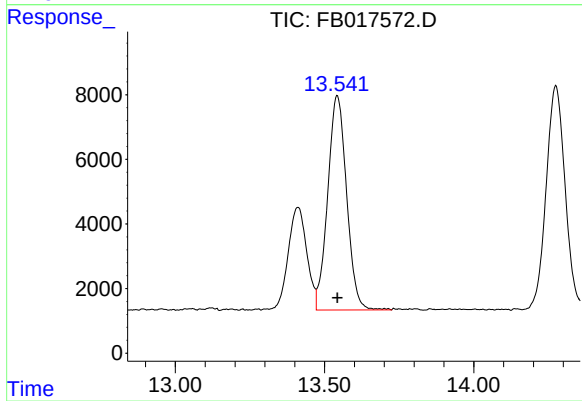


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: 0.000 min
Response: 292191
Conc: 18.80 ng/ml

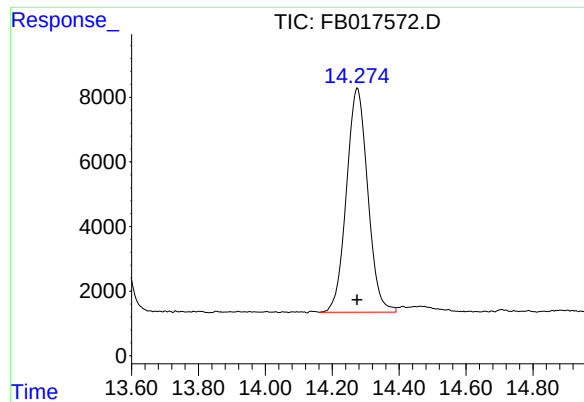

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: 0.001 min
Response: 307155
Conc: 18.71 ng/ml

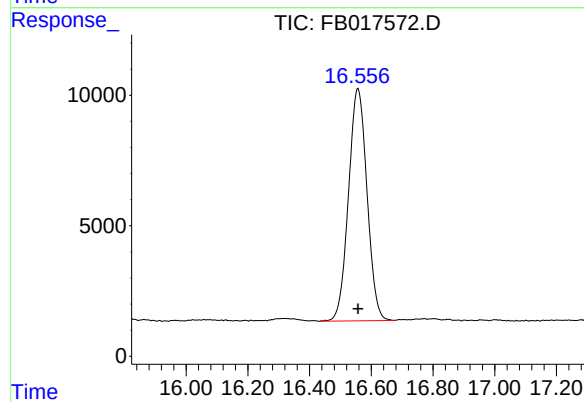

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: 0.000 min
Response: 370821
Conc: 19.04 ng/ml