

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028038.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 13:47
Operator : AJ/MA
Sample : N4421-09
Misc : 5.26G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:42:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.863	29698	2.563 ng/ml
Target Compounds			
7) t Ethylbenzene	13.029	104994	5.095 ng/ml
9) t O-Xylene	13.937	17598	0.888 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028038.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 13:47
Operator : AJ/MA
Sample : N4421-09
Misc : 5.26G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:42:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

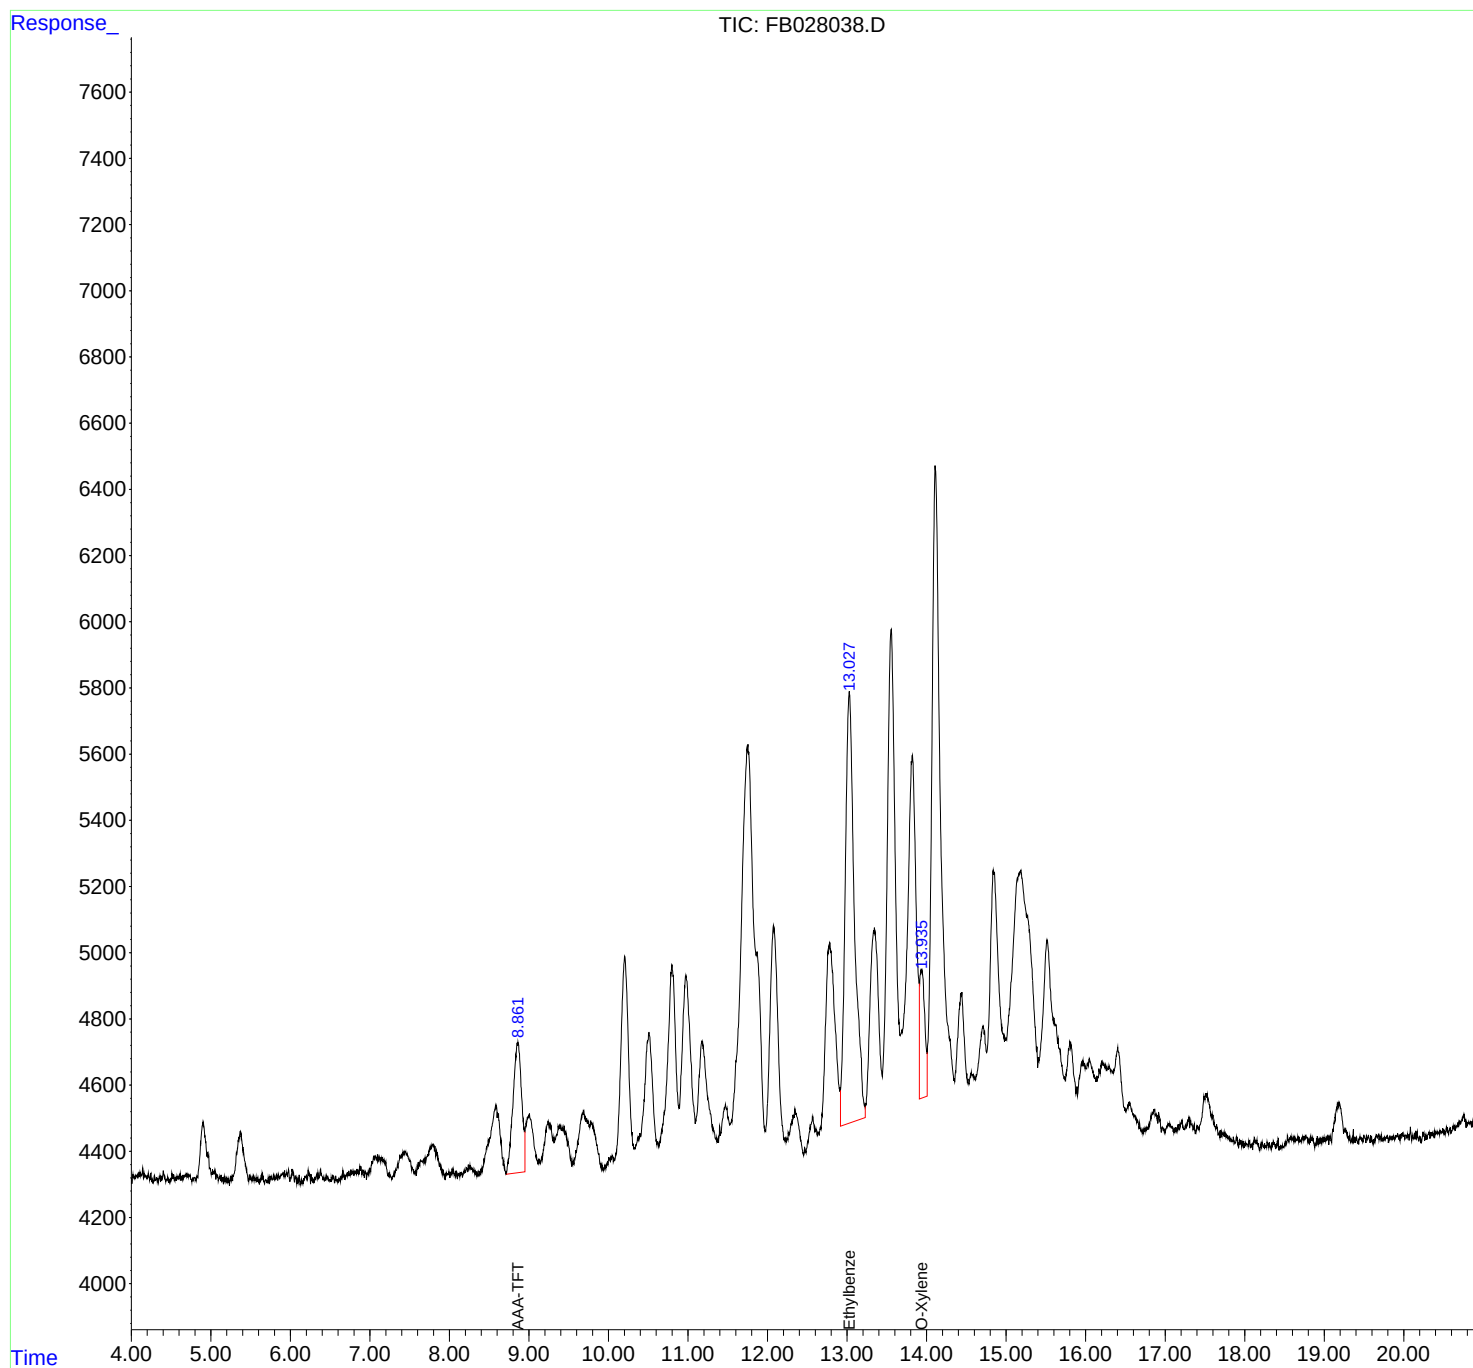


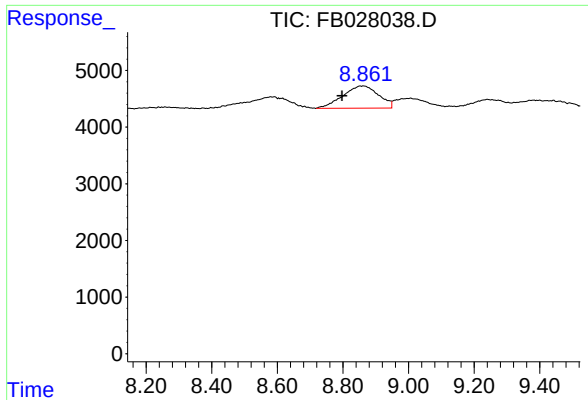

#5 AAA-TFT


R.T.: 8.863 min
Delta R.T.: 0.065 min
Response: 29698
Conc: 2.56 ng/ml

Instrument :
FID_B
ClientSampleId :

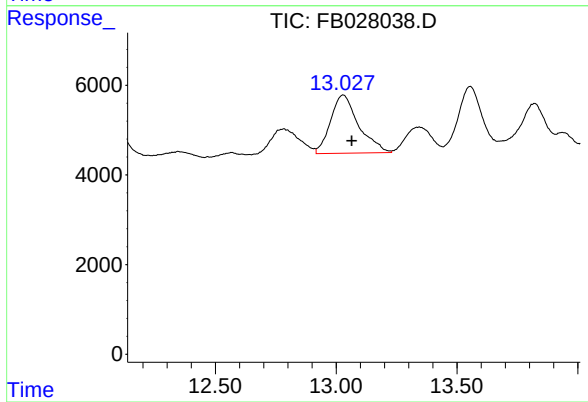

#7 Ethylbenzene

R.T.: 13.029 min
Delta R.T.: -0.036 min
Response: 104994
Conc: 5.10 ng/ml

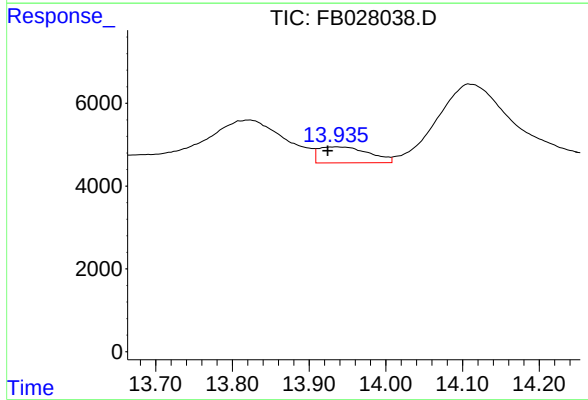

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.013 min
Response: 17598
Conc: 0.89 ng/ml