

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
 Data File : FB028042.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2022 17:09
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 30 05:43:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	311677	26.893 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	1929	0.107 ng/ml
6) t Toluene	10.615	344	0.016 ng/ml
9) t O-Xylene	13.900	16197	0.818 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028042.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 17:09
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:43:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

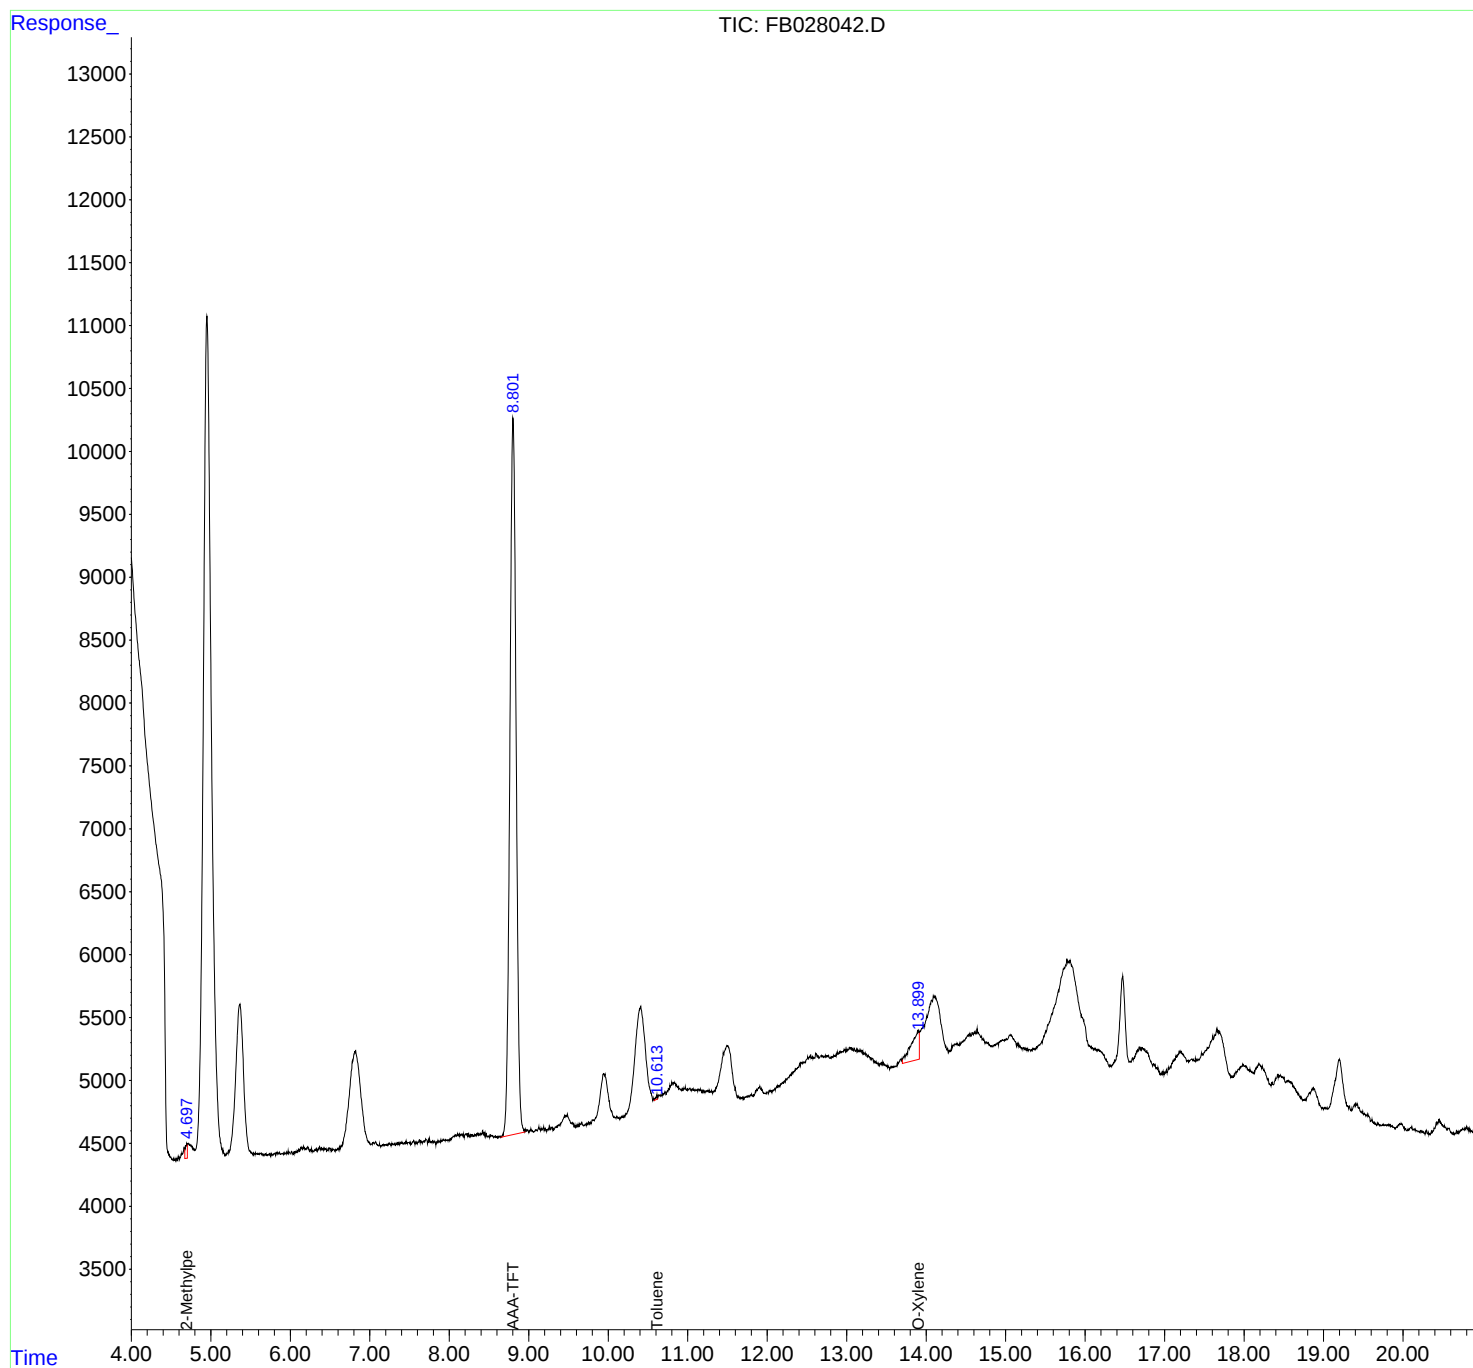


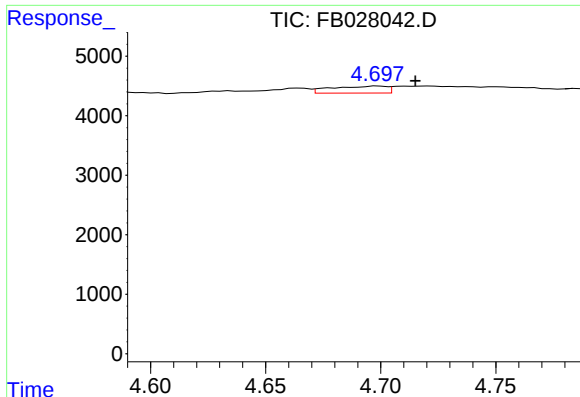

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.016 min
Response: 1929
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :

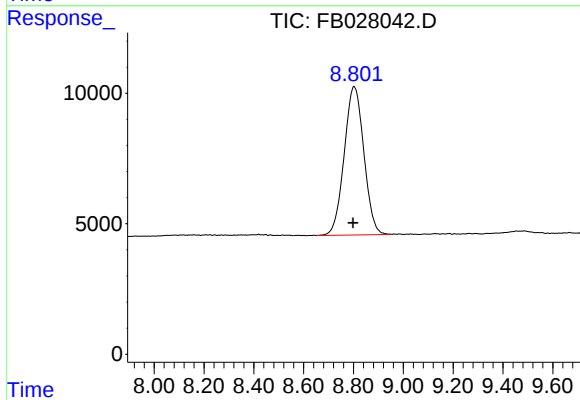


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.005 min
Response: 311677
Conc: 26.89 ng/ml

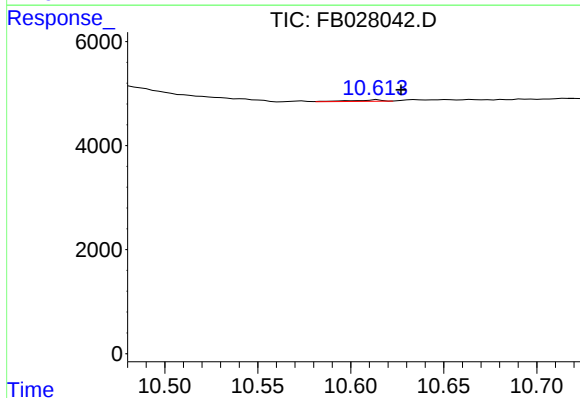

#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.012 min
Response: 344
Conc: 0.02 ng/ml

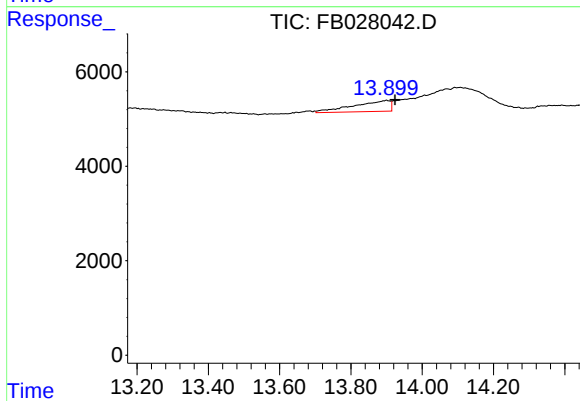

#9 O-Xylene

R.T.: 13.900 min
Delta R.T.: -0.024 min
Response: 16197
Conc: 0.82 ng/ml