

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028046.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 20:16
Operator : AJ/MA
Sample : N4421-14
Misc : 5.16G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:43:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.807	89149	7.692 ng/ml
Target Compounds			
7) t Ethylbenzene	13.032	40053	1.944 ng/ml
8) t m-Xylene	13.152	2863	0.140 ng/ml
9) t O-Xylene	13.950	5888	0.297 ng/ml
10) t 1,2,4-Trimethylbenzene	16.221	8752	0.449 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028046.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 20:16
Operator : AJ/MA
Sample : N4421-14
Misc : 5.16G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:43:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

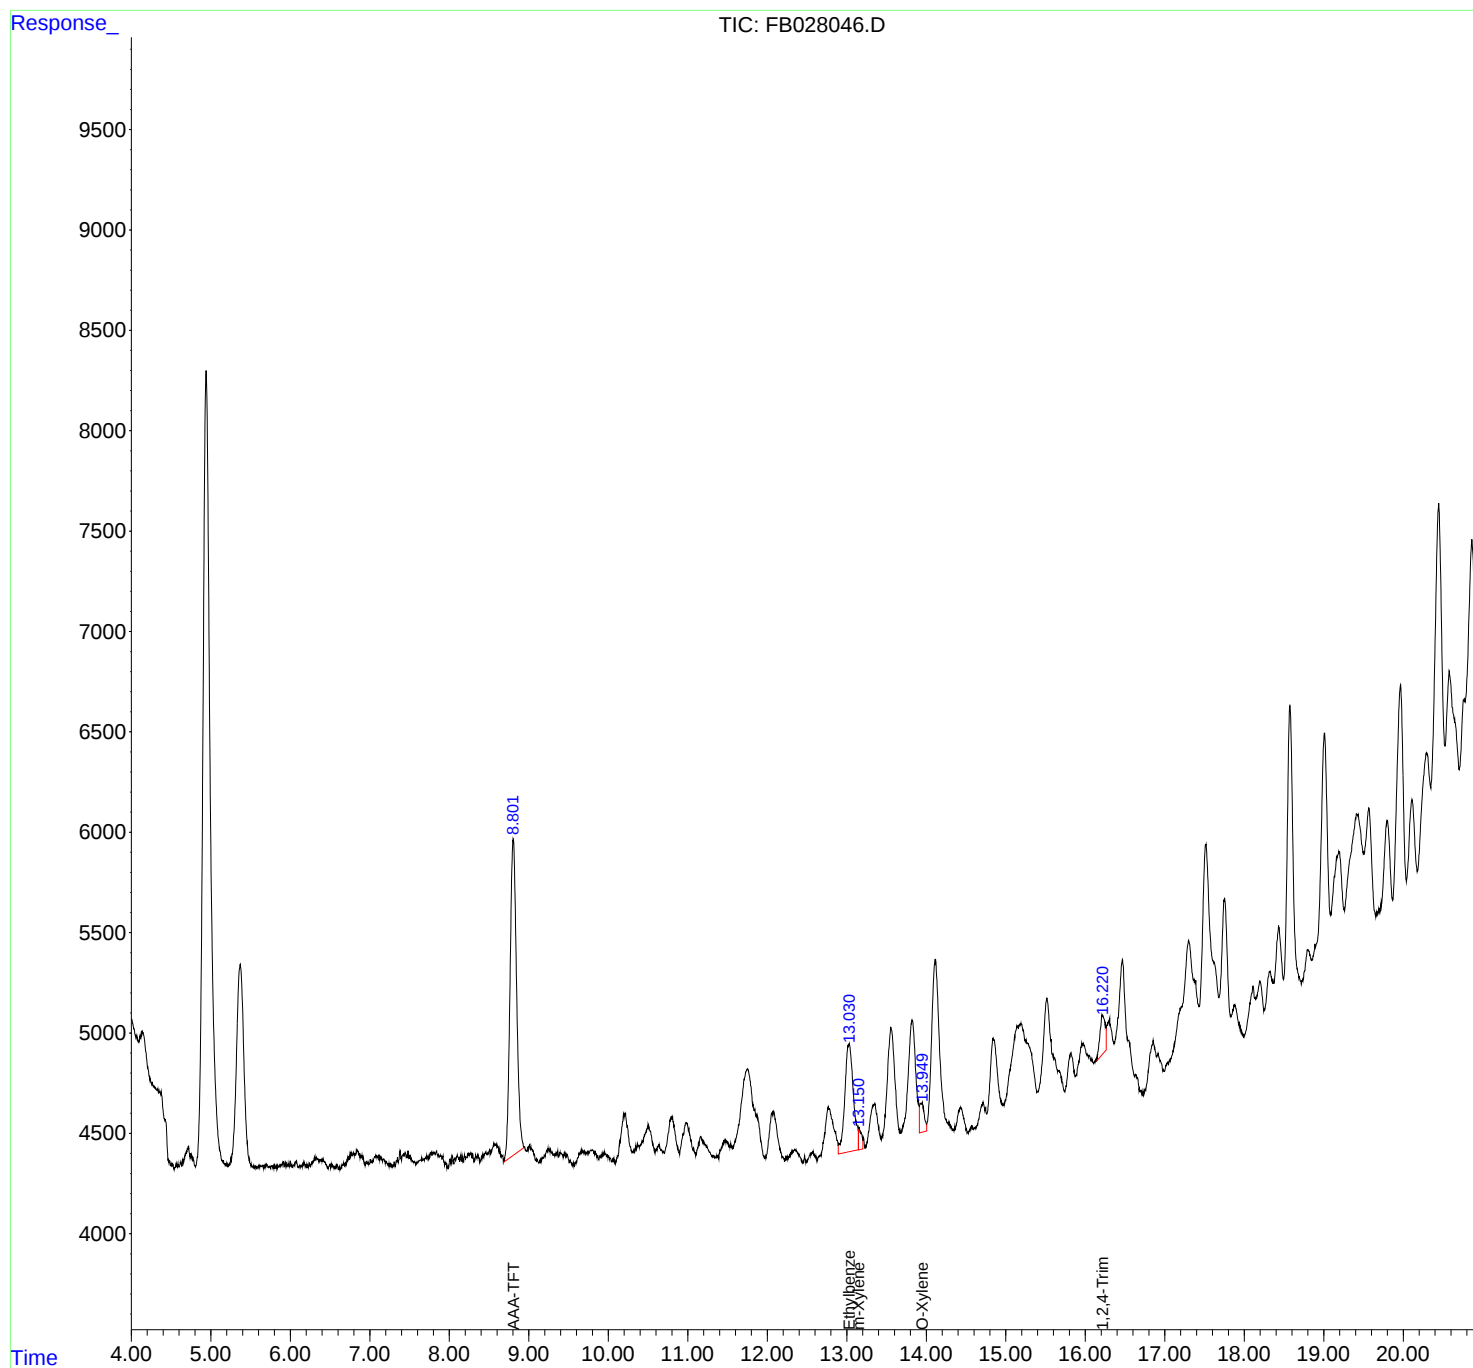


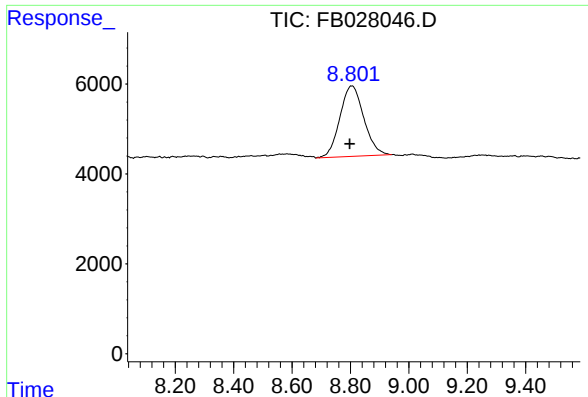

#5 AAA-TFT


R.T.: 8.807 min
Delta R.T.: 0.009 min
Response: 89149
Conc: 7.69 ng/ml

Instrument :
FID_B
ClientSampleId :

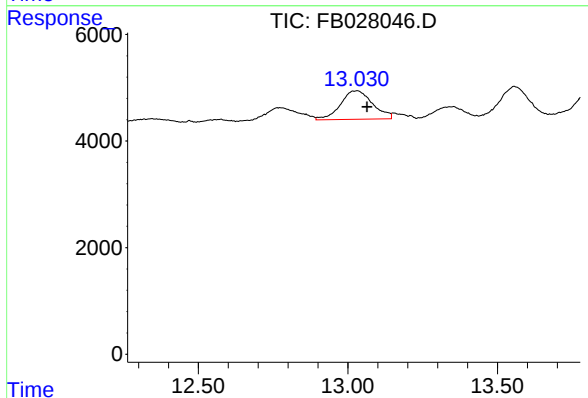


#7 Ethylbenzene

R.T.: 13.032 min
Delta R.T.: -0.032 min
Response: 40053
Conc: 1.94 ng/ml

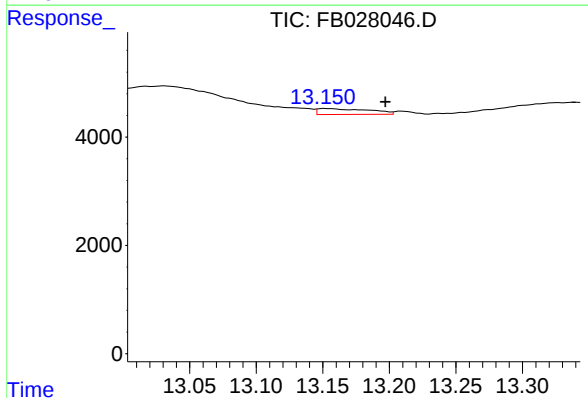


#8 m-Xylene

R.T.: 13.152 min
Delta R.T.: -0.045 min
Response: 2863
Conc: 0.14 ng/ml

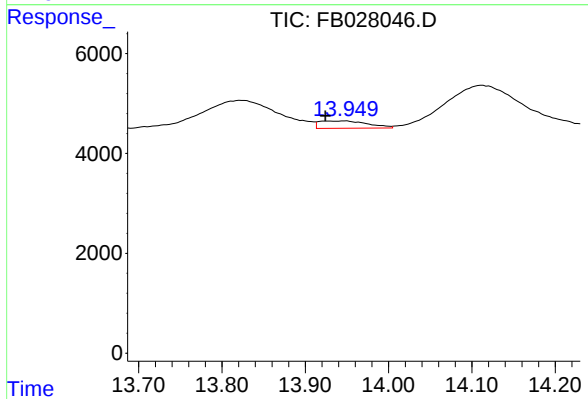

#9 O-Xylene

R.T.: 13.950 min
Delta R.T.: 0.026 min
Response: 5888
Conc: 0.30 ng/ml

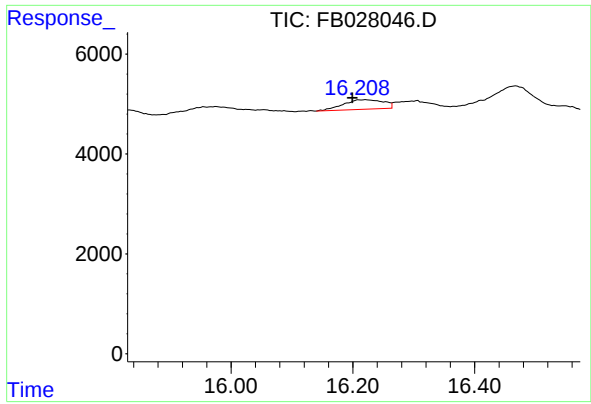

#10 1,2,4-Trimethylbenzene

R.T.: 16.221 min
Delta R.T.: 0.022 min
Response: 8752
Conc: 0.45 ng/ml

Instrument :
FID_B
ClientSampleId :