

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028048.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 21:31
Operator : AJ/MA
Sample : N4421-14RE
Misc : 5.39G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:43:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	87146	7.519 ng/ml
Target Compounds			
7) t Ethylbenzene	13.027	22488	1.091 ng/ml
9) t O-Xylene	13.944	3000	0.151 ng/ml
10) t 1,2,4-Trimethylbenzene	16.217	2149	0.110 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028048.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 21:31
Operator : AJ/MA
Sample : N4421-14RE
Misc : 5.39G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:43:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

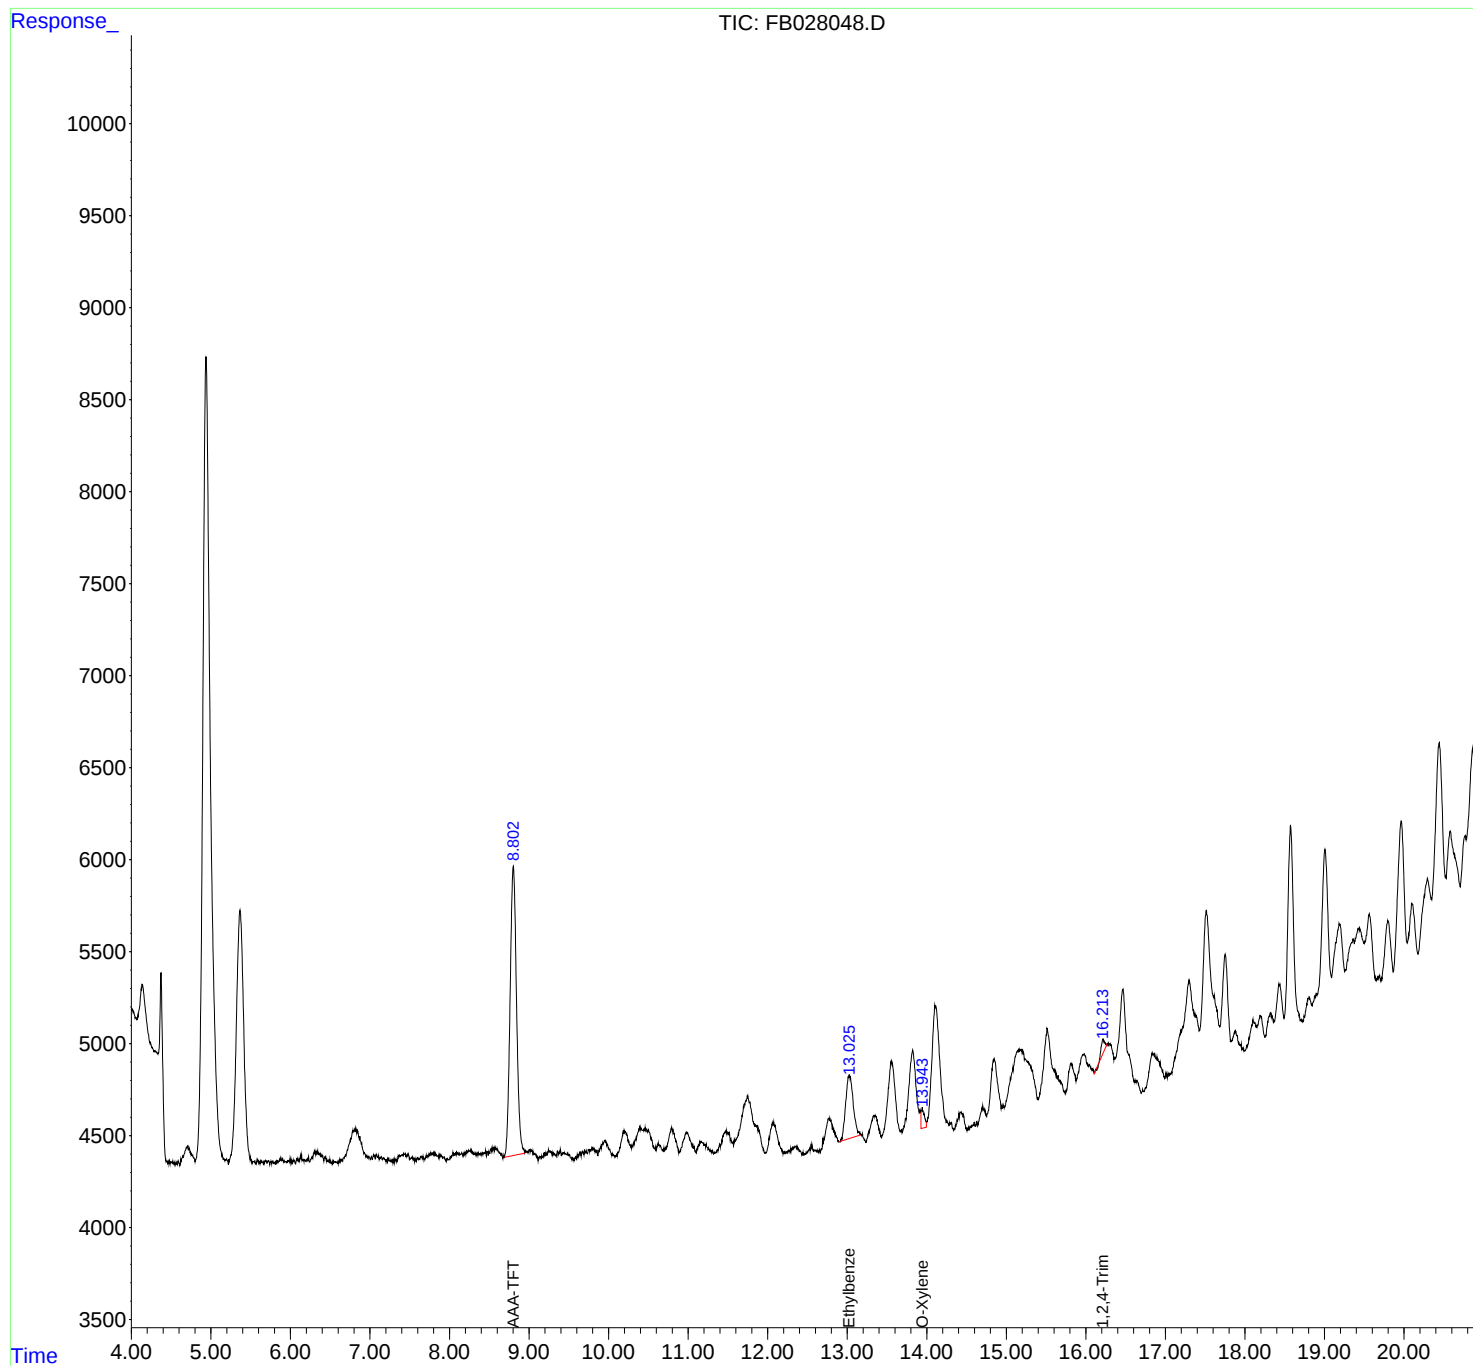


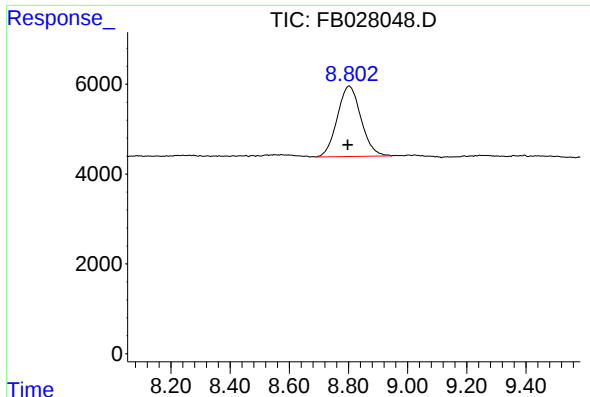

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 87146
Conc: 7.52 ng/ml

Instrument :
FID_B
ClientSampleId :

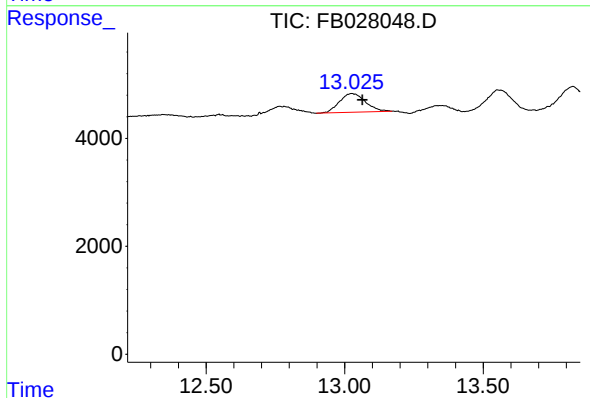


#7 Ethylbenzene

R.T.: 13.027 min
Delta R.T.: -0.038 min
Response: 22488
Conc: 1.09 ng/ml

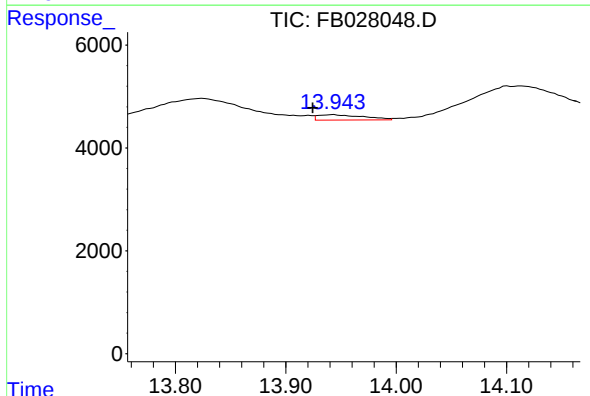

#9 O-Xylene

R.T.: 13.944 min
Delta R.T.: 0.019 min
Response: 3000
Conc: 0.15 ng/ml

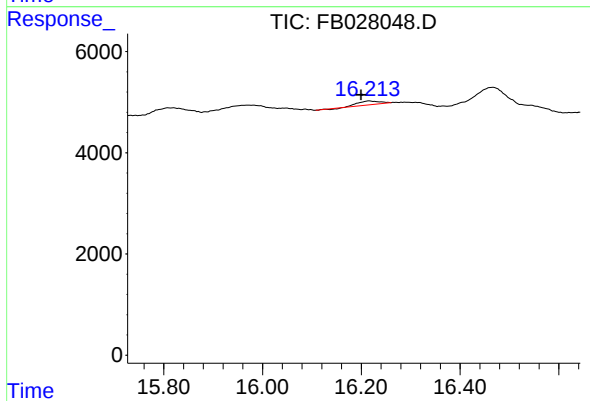

#10 1,2,4-Trimethylbenzene

R.T.: 16.217 min
Delta R.T.: 0.017 min
Response: 2149
Conc: 0.11 ng/ml