

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
 Data File : FB028050.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2022 22:46
 Operator : AJ/MA
 Sample : N4421-09MS
 Misc : 5.17G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 30 05:44:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.852	260803	22.504 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	110245	6.094 ng/ml
2) t 2,2,4-Trimethylpentane	7.445	110543	5.637 ng/ml
3) t n-Heptane	7.768	72332	3.755 ng/ml
4) t Benzene	7.893	111789	4.808 ng/ml
6) t Toluene	10.630	221177	10.087 ng/ml
7) t Ethylbenzene	13.031	1748724	84.861 ng/ml
9) t O-Xylene	13.933	404043	20.397 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	423754	21.730 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028050.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 22:46
Operator : AJ/MA
Sample : N4421-09MS
Misc : 5.17G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 05:44:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

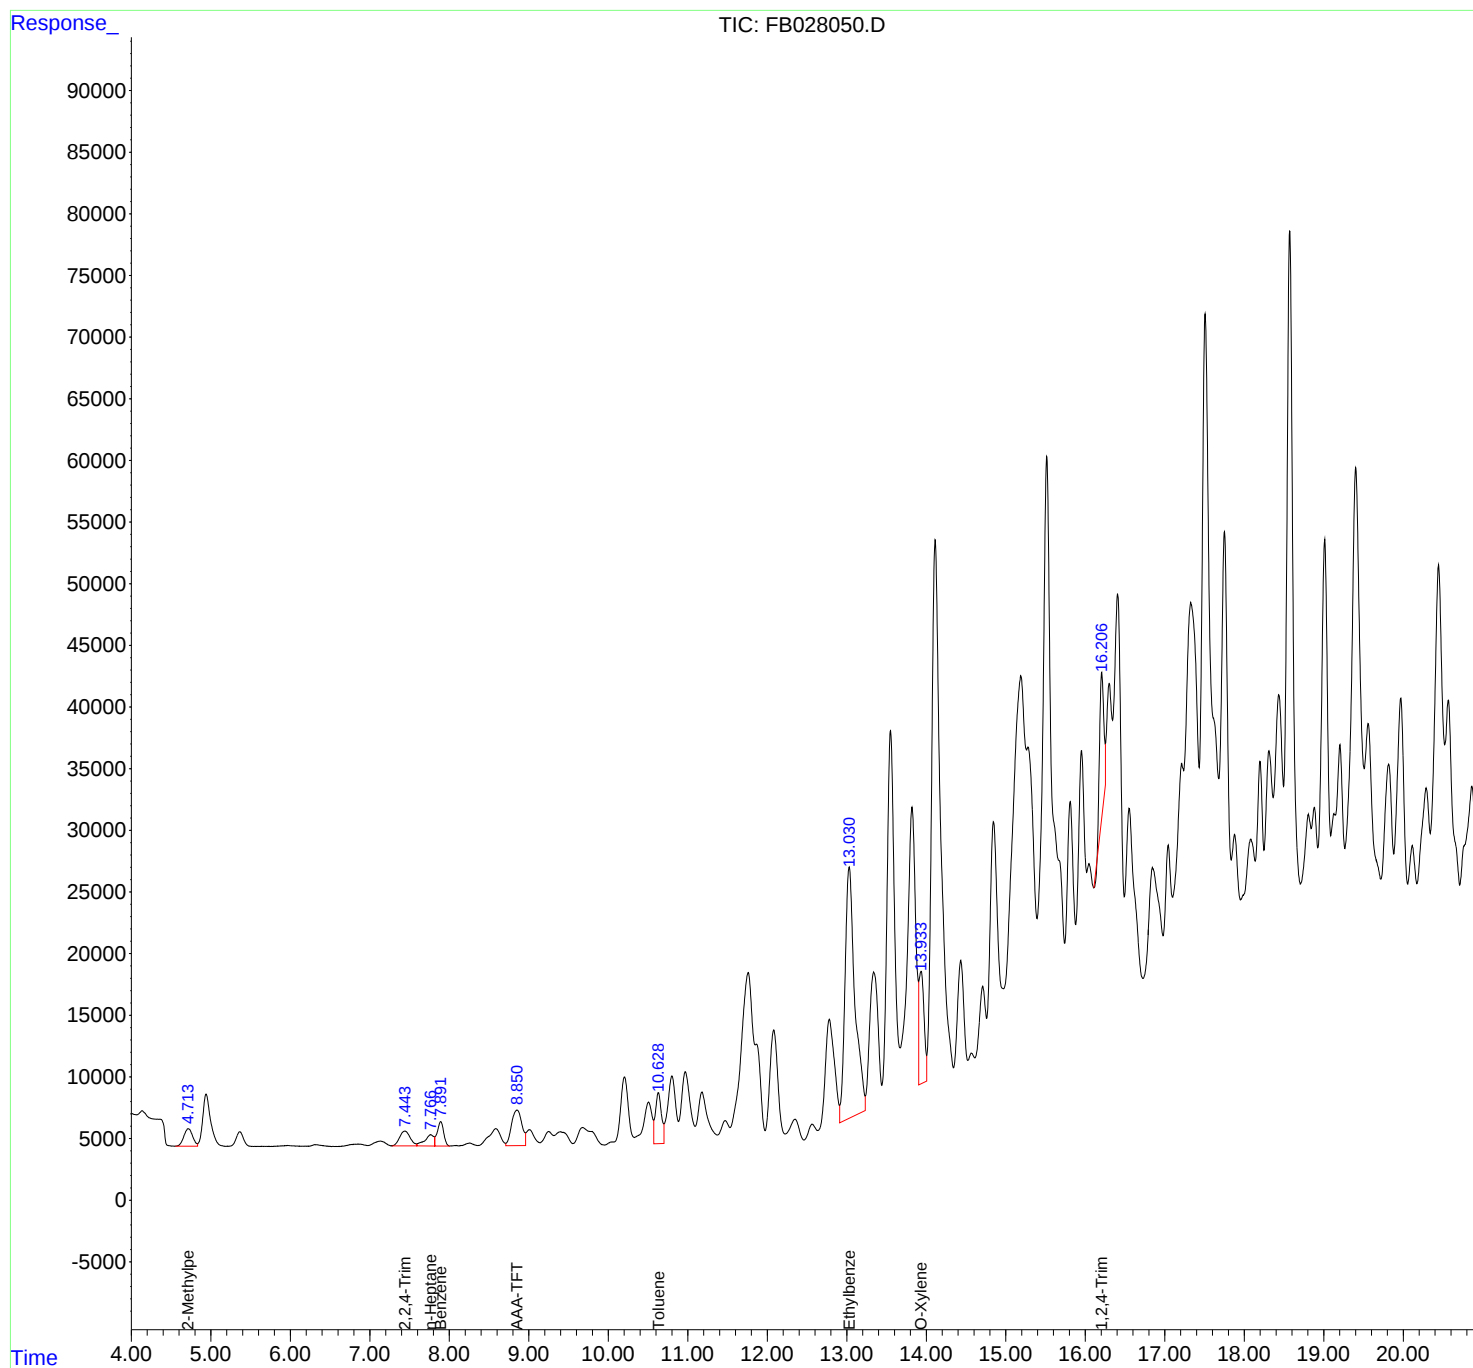


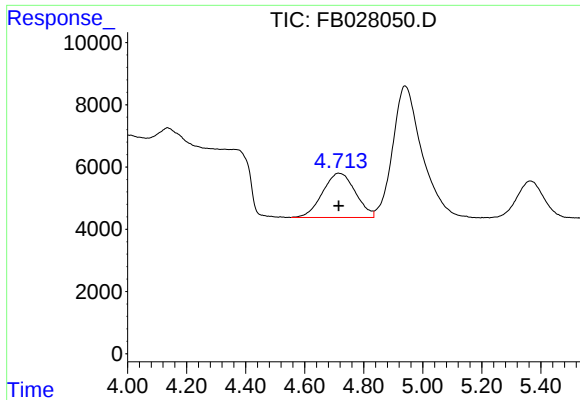

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 110245
Conc: 6.09 ng/ml

Instrument :
FID_B
ClientSampleId :

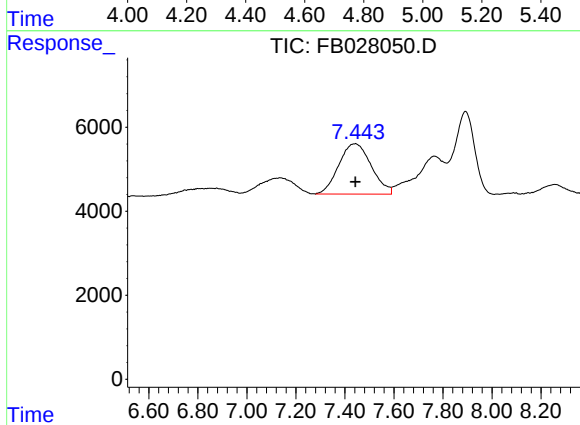


#2 2,2,4-Trimethylpentane

R.T.: 7.445 min
Delta R.T.: 0.002 min
Response: 110543
Conc: 5.64 ng/ml

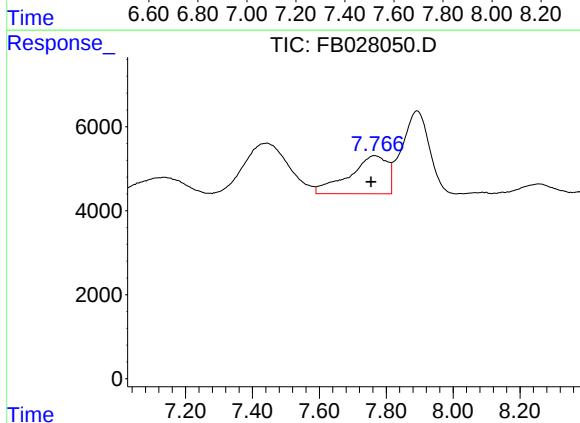


#3 n-Heptane

R.T.: 7.768 min
Delta R.T.: 0.013 min
Response: 72332
Conc: 3.75 ng/ml

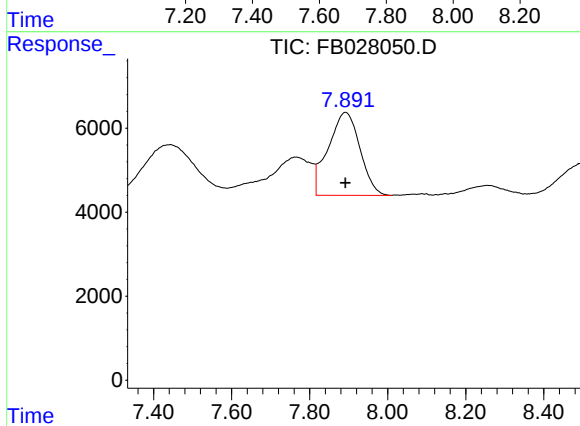

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 111789
Conc: 4.81 ng/ml

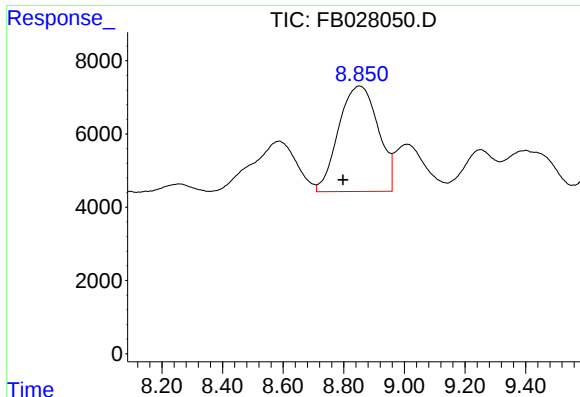

#5 AAA-TFT


R.T.: 8.852 min
Delta R.T.: 0.054 min
Response: 260803
Conc: 22.50 ng/ml

Instrument :
FID_B
ClientSampleId :

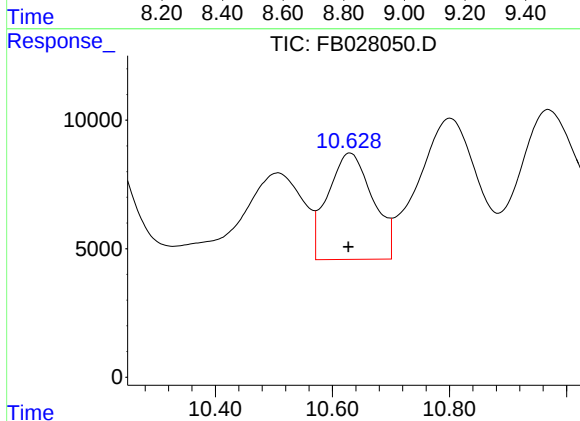


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.003 min
Response: 221177
Conc: 10.09 ng/ml

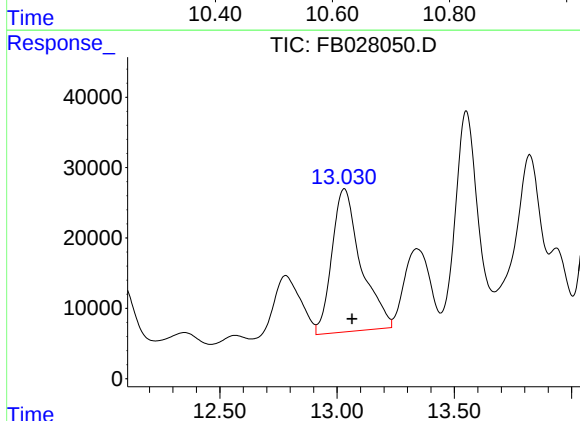


#7 Ethylbenzene

R.T.: 13.031 min
Delta R.T.: -0.034 min
Response: 1748724
Conc: 84.86 ng/ml

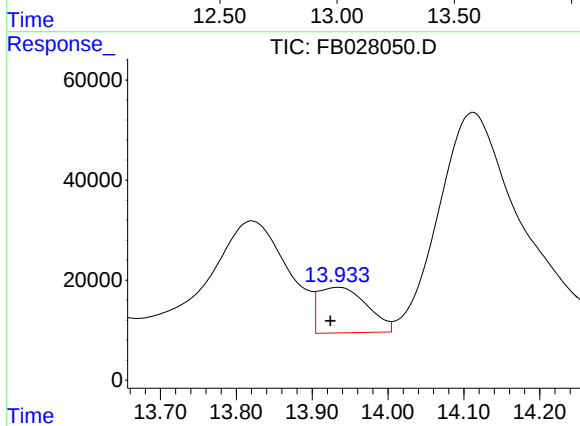

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.009 min
Response: 404043
Conc: 20.40 ng/ml

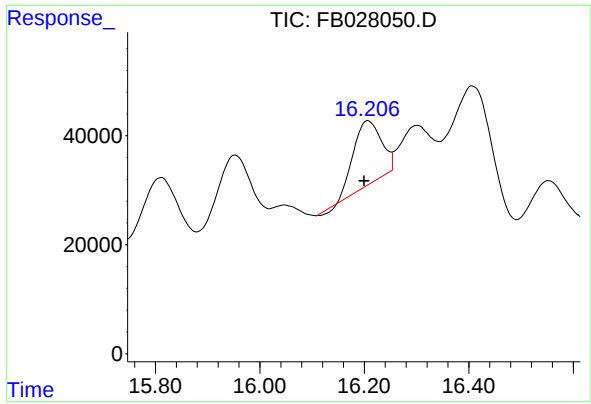

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.009 min
Response: 423754
Conc: 21.73 ng/ml

Instrument :
FID_B
ClientSampleId :