

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082922\  
 Data File : FB028051.D  
 Signal(s) : FID2B.CH  
 Acq On : 29 Aug 2022 23:23  
 Operator : AJ/MA  
 Sample : I.BLK  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Aug 30 05:44:22 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB080922.M  
 Quant Title :  
 QLast Update : Tue Aug 09 12:12:39 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.801  | 279033   | 24.077 ng/ml |
| Target Compounds            |        |          |              |
| 1) t 2-Methylpentane        | 4.724  | 442      | 0.024 ng/ml  |
| 8) t m-Xylene               | 13.208 | 3545     | 0.173 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082922\  
Data File : FB028051.D  
Signal(s) : FID2B.CH  
Acq On : 29 Aug 2022 23:23  
Operator : AJ/MA  
Sample : I.BLK  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Aug 30 05:44:22 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB080922.M  
Quant Title :  
QLast Update : Tue Aug 09 12:12:39 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

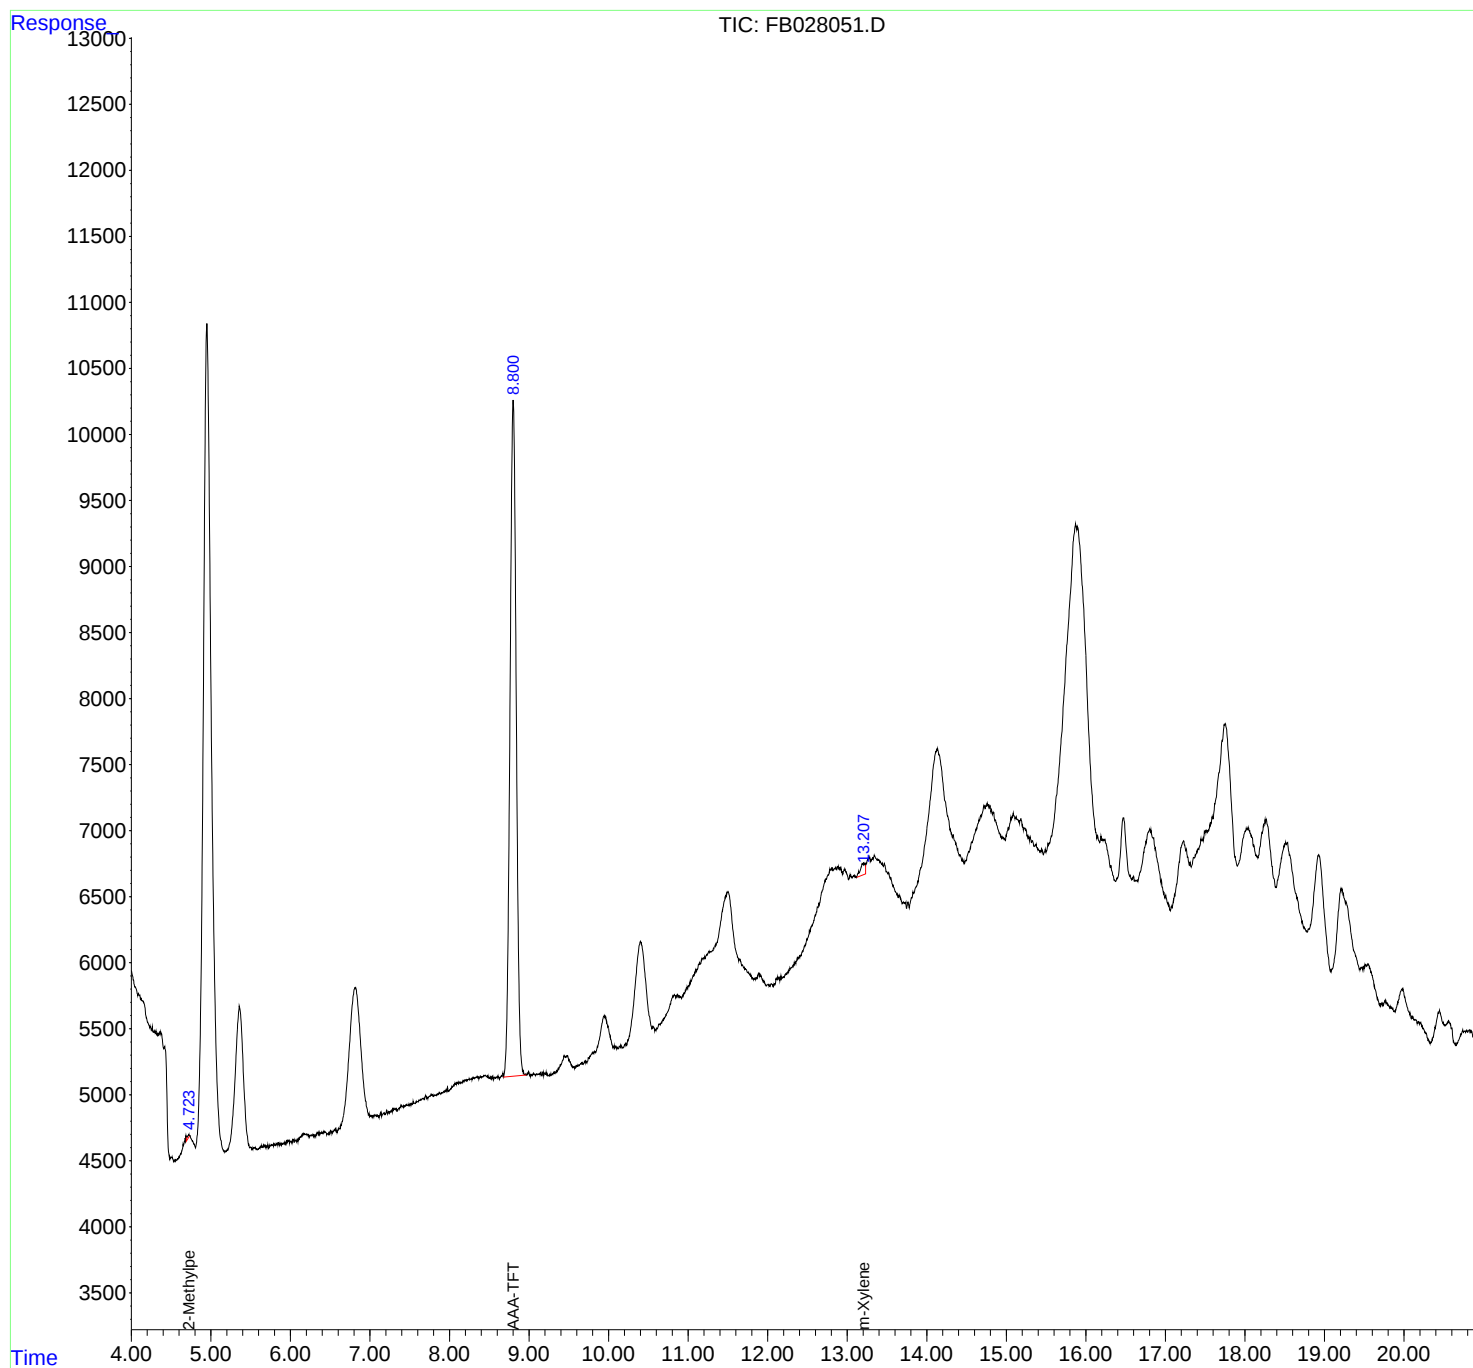


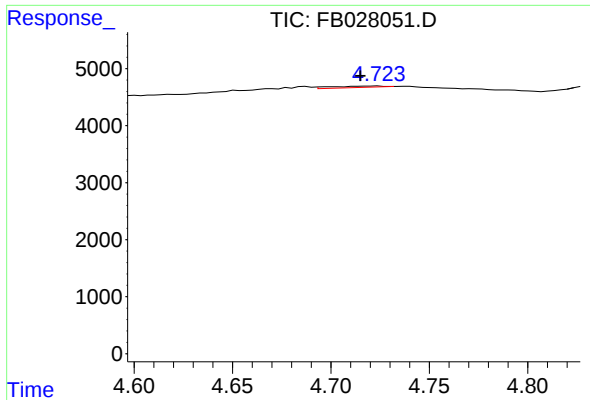

#1 2-Methylpentane


R.T.: 4.724 min  
Delta R.T.: 0.009 min  
Response: 442  
Conc: 0.02 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

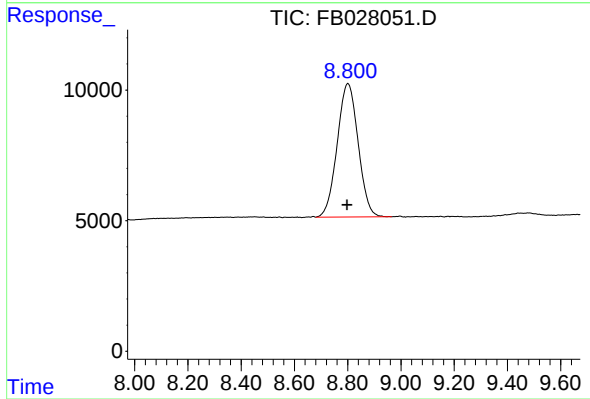

#5 AAA-TFT

R.T.: 8.801 min  
Delta R.T.: 0.003 min  
Response: 279033  
Conc: 24.08 ng/ml

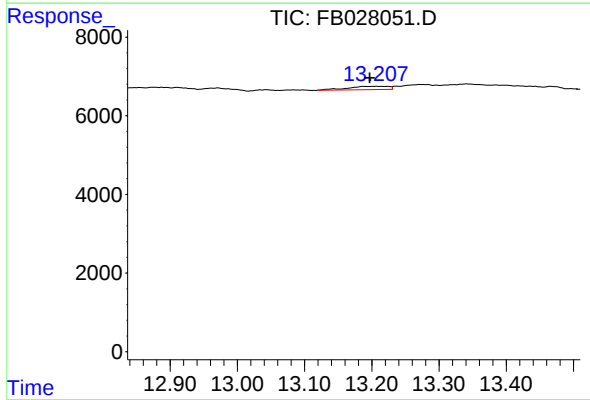

#8 m-Xylene

R.T.: 13.208 min  
Delta R.T.: 0.011 min  
Response: 3545  
Conc: 0.17 ng/ml