

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
 Data File : FB028037.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2022 13:10
 Operator : AJ/MA
 Sample : BSF0829S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0829S1

Integration File: Calibration.e
 Quant Time: Aug 30 05:42:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	229437	19.797 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	492389	27.218 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	587524	29.960 ng/ml
3) t n-Heptane	7.758	173282	8.995 ng/ml
4) t Benzene	7.895	209423	9.007 ng/ml
6) t Toluene	10.629	614244	28.012 ng/ml
7) t Ethylbenzene	13.065	195433	9.484 ng/ml
8) t m-Xylene	13.197	391616	19.138 ng/ml
9) t O-Xylene	13.924	386604	19.516 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	405976	20.818 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028037.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 13:10
Operator : AJ/MA
Sample : BSF0829S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0829S1

Integration File: Calibration.e
Quant Time: Aug 30 05:42:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

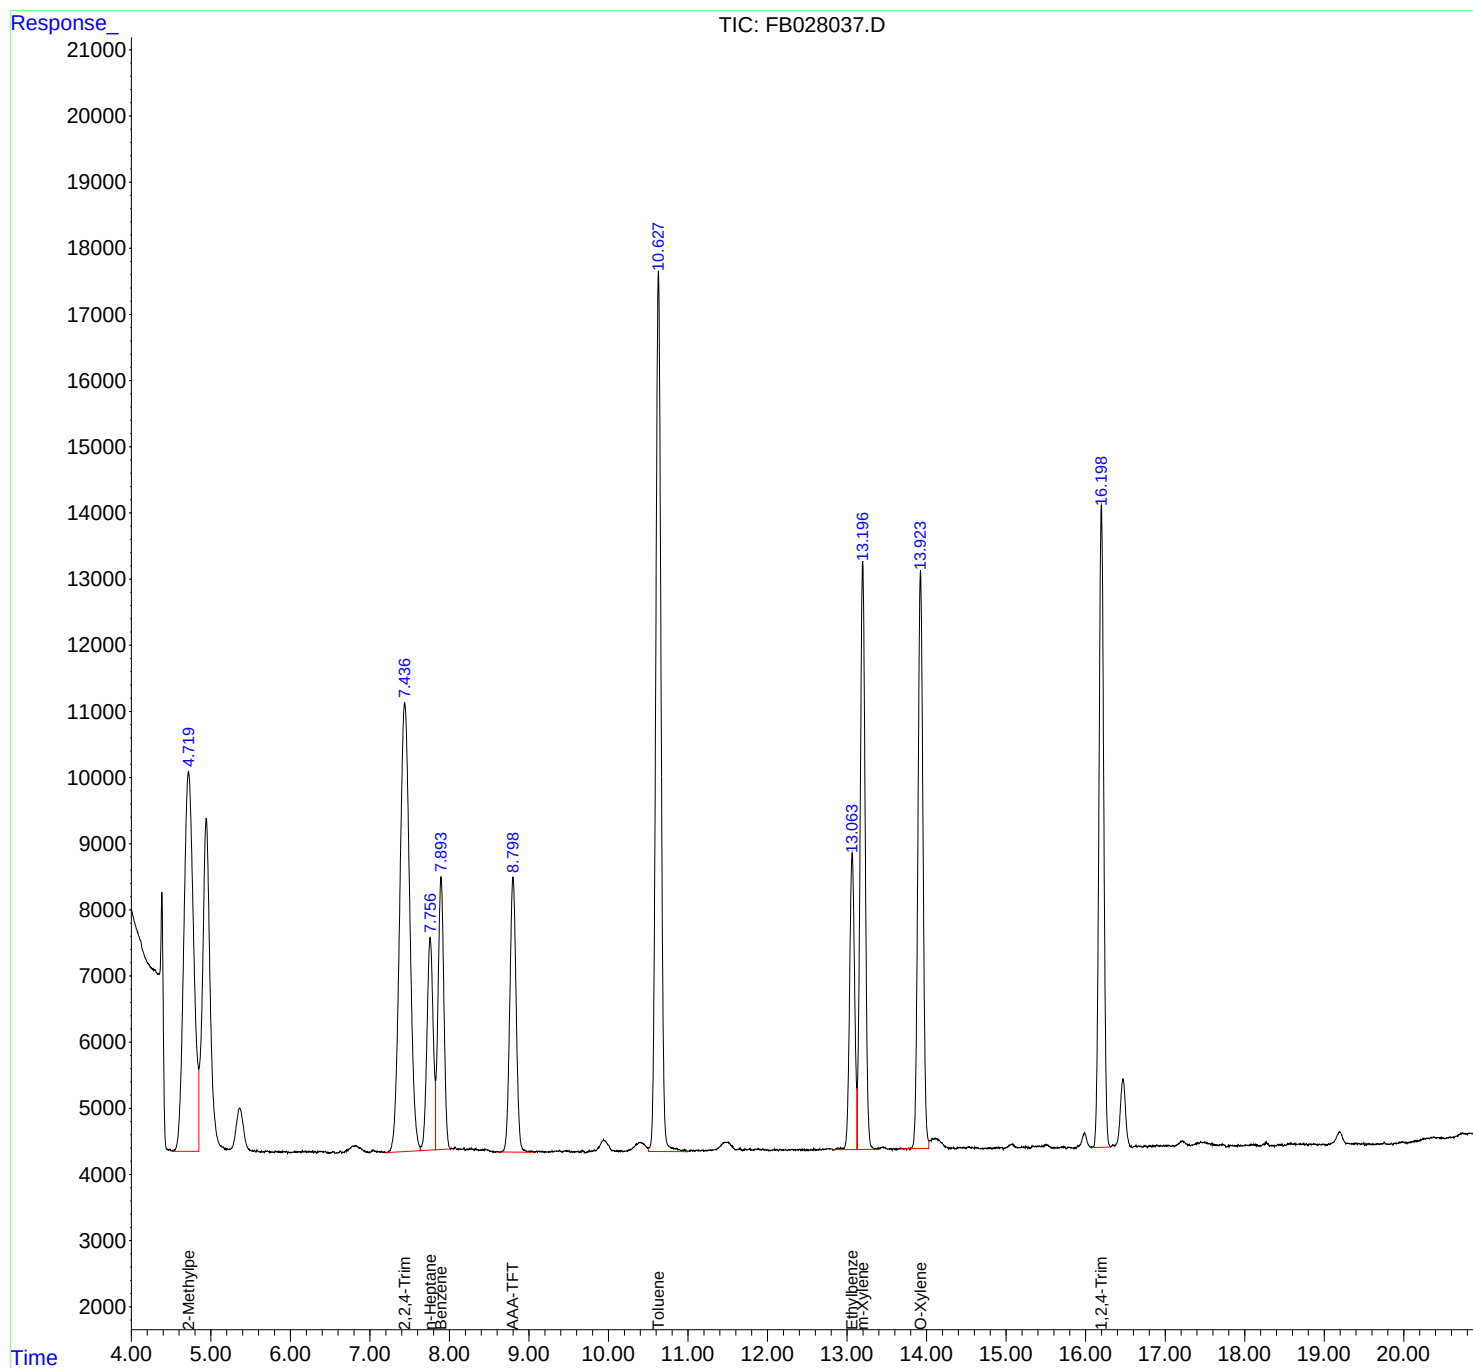


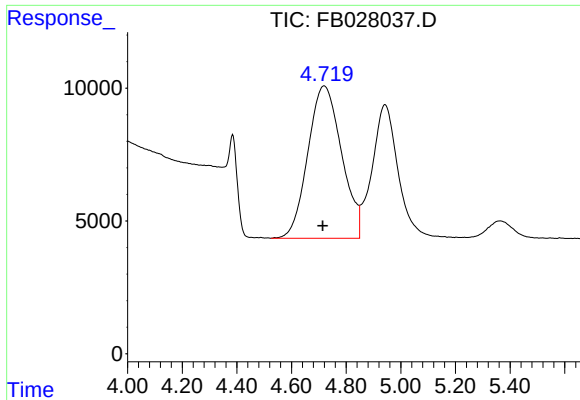

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.005 min
Response: 492389
Conc: 27.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

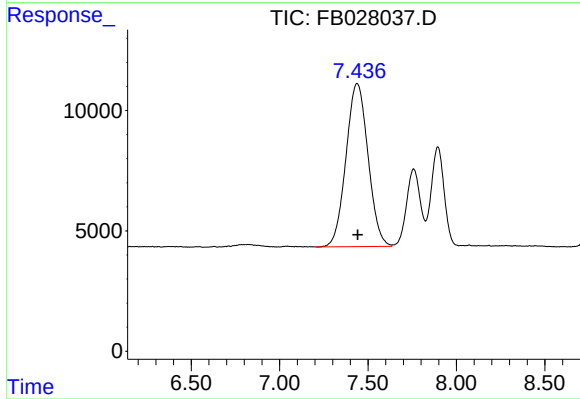


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: -0.005 min
Response: 587524
Conc: 29.96 ng/ml

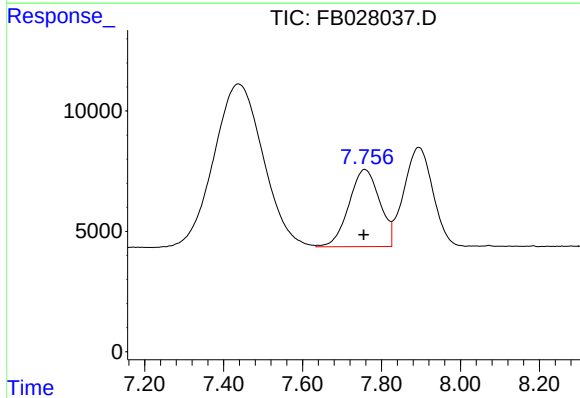


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.003 min
Response: 173282
Conc: 8.99 ng/ml

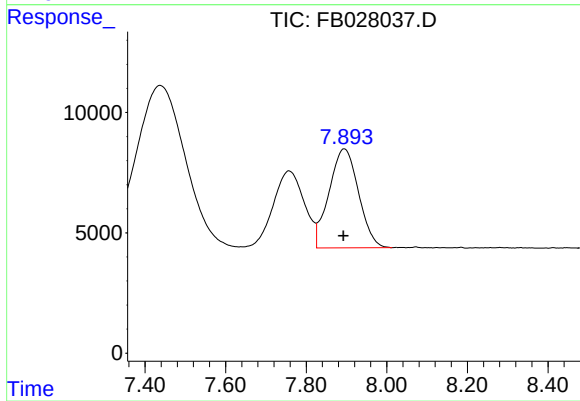

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.003 min
Response: 209423
Conc: 9.01 ng/ml

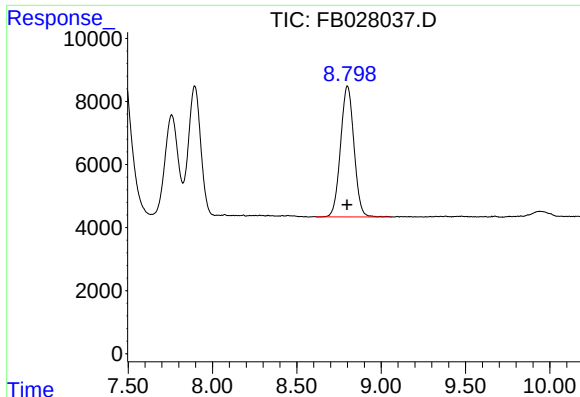

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 229437
Conc: 19.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

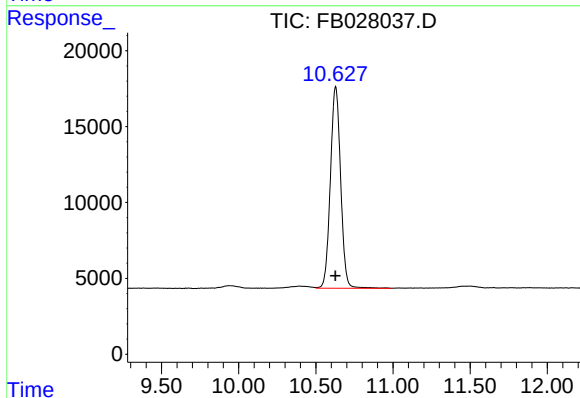


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.001 min
Response: 614244
Conc: 28.01 ng/ml

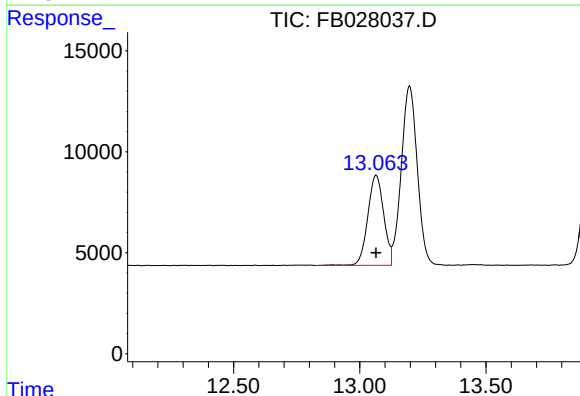


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 195433
Conc: 9.48 ng/ml

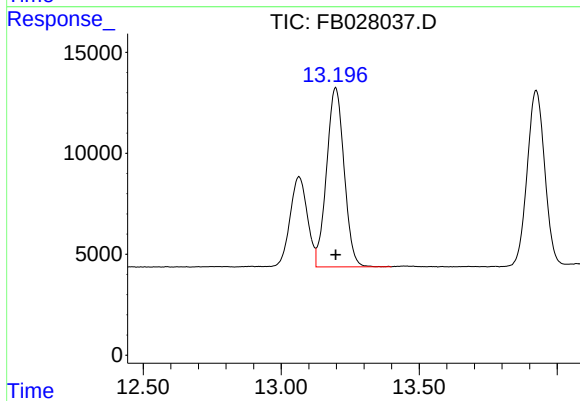

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 391616
Conc: 19.14 ng/ml

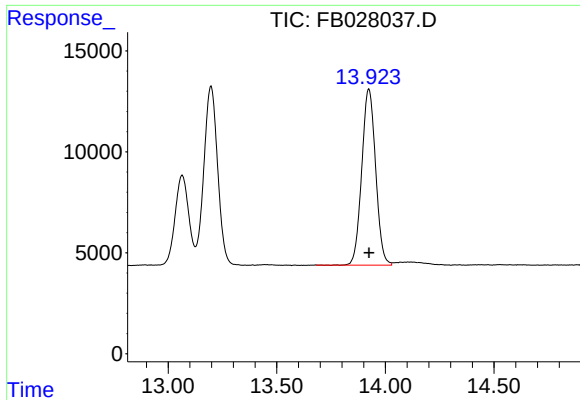

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 386604
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0829S1

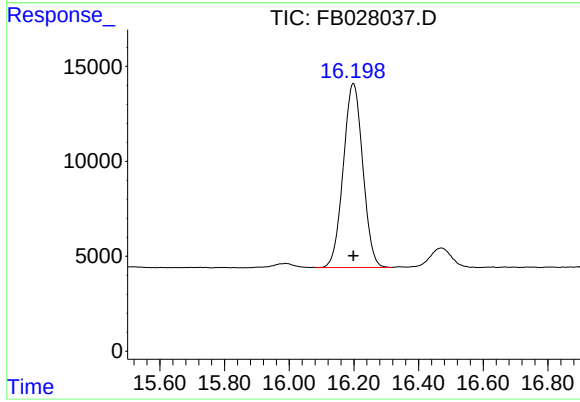

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 405976
Conc: 20.82 ng/ml