

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028049.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 22:08
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
I.BLK

Integration File: Calibration.e
Quant Time: Aug 30 05:44:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	258406	22.297 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082922\
Data File : FB028049.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2022 22:08
Operator : AJ/MA
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
I.BLK

Integration File: Calibration.e
Quant Time: Aug 30 05:44:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

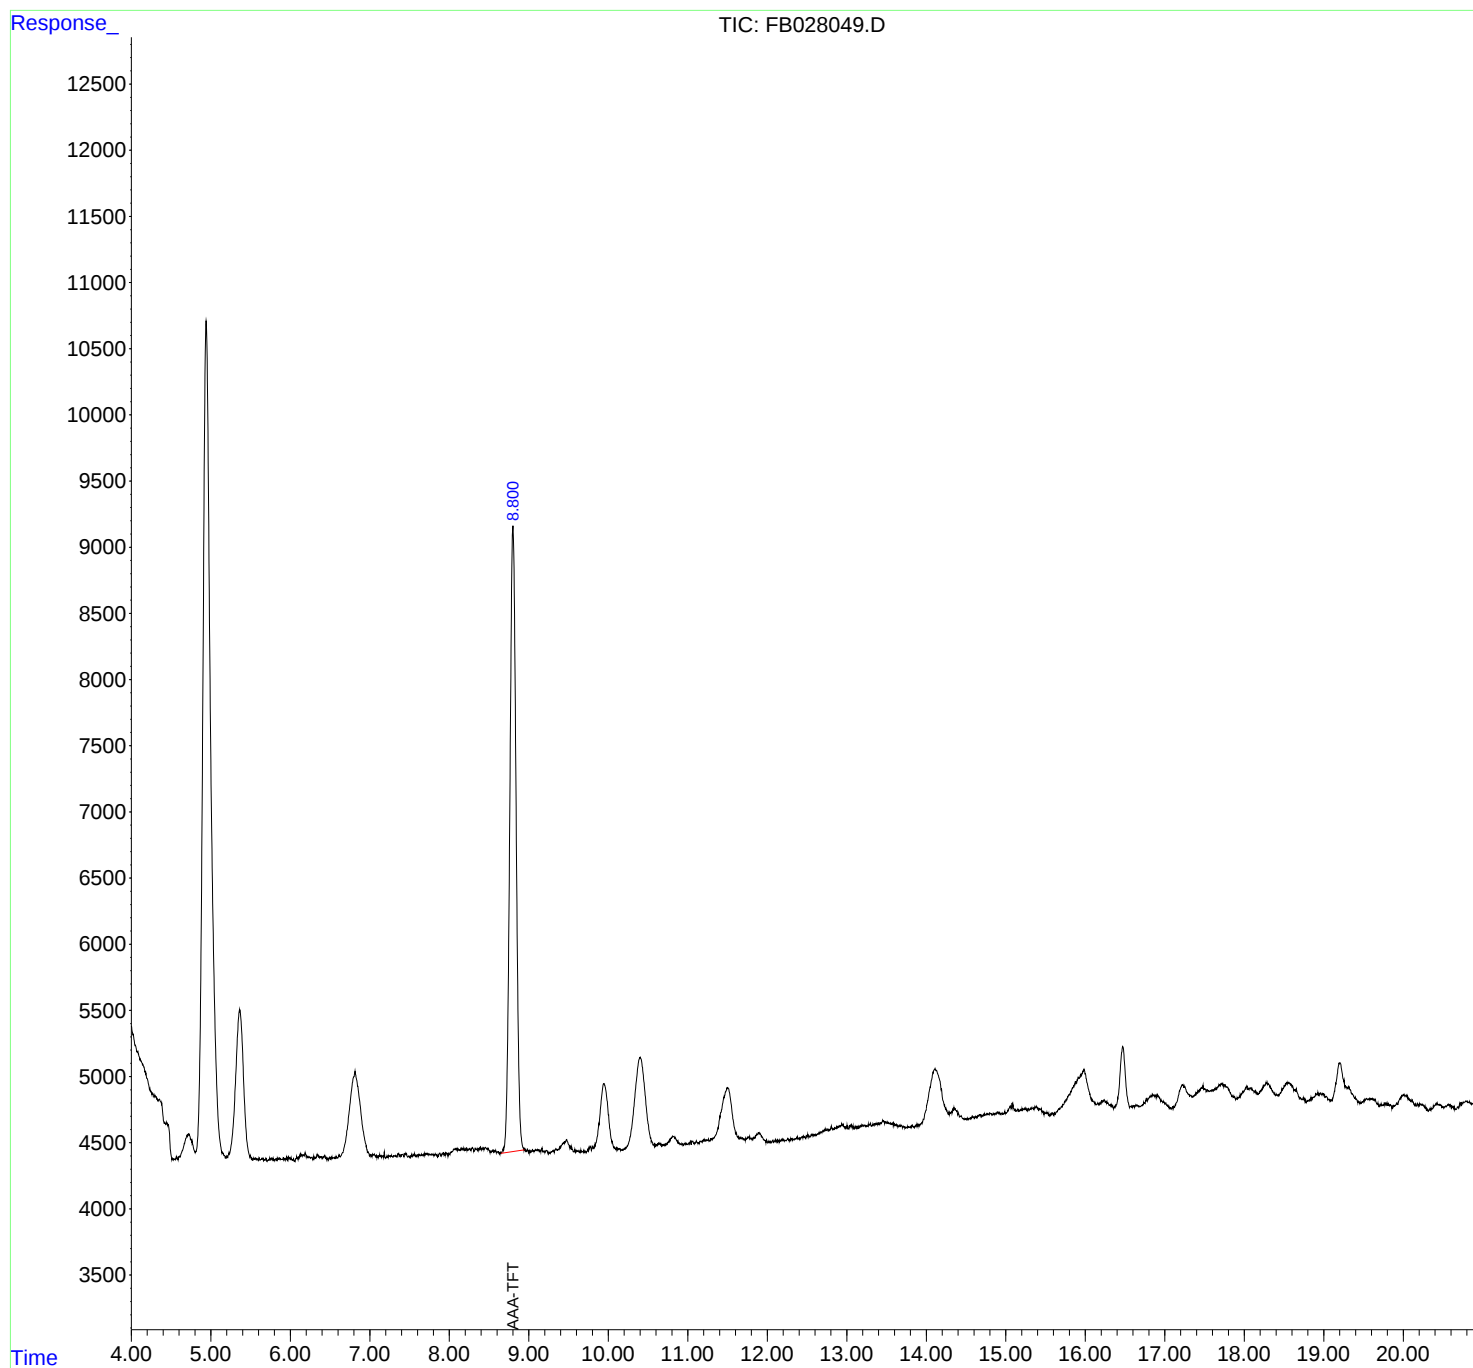

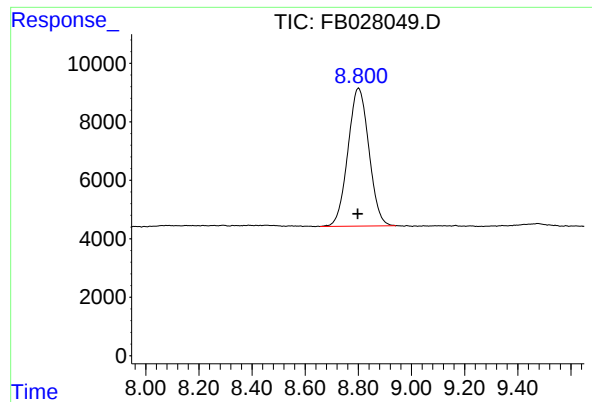

#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 258406
Conc: 22.30 ng/ml

Instrument :

FID_B

ClientSampleId :

I.BLK