

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
 Data File : FB030902.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2024 10:59
 Operator : YP/AJ
 Sample : BSF0829S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 30 06:38:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	261595	21.621 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	572364	32.031 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	587981	32.069 ng/ml
3) t n-Heptane	7.745	198549	10.736 ng/ml
4) t Benzene	7.882	252656	11.183 ng/ml
6) t Toluene	10.615	734387	33.624 ng/ml
7) t Ethylbenzene	13.050	231519	11.059 ng/ml
8) t m-Xylene	13.183	457977	22.072 ng/ml
9) t O-Xylene	13.910	437146	21.690 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	425411	21.320 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
Data File : FB030902.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2024 10:59
Operator : YP/AJ
Sample : BSF0829S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 06:38:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

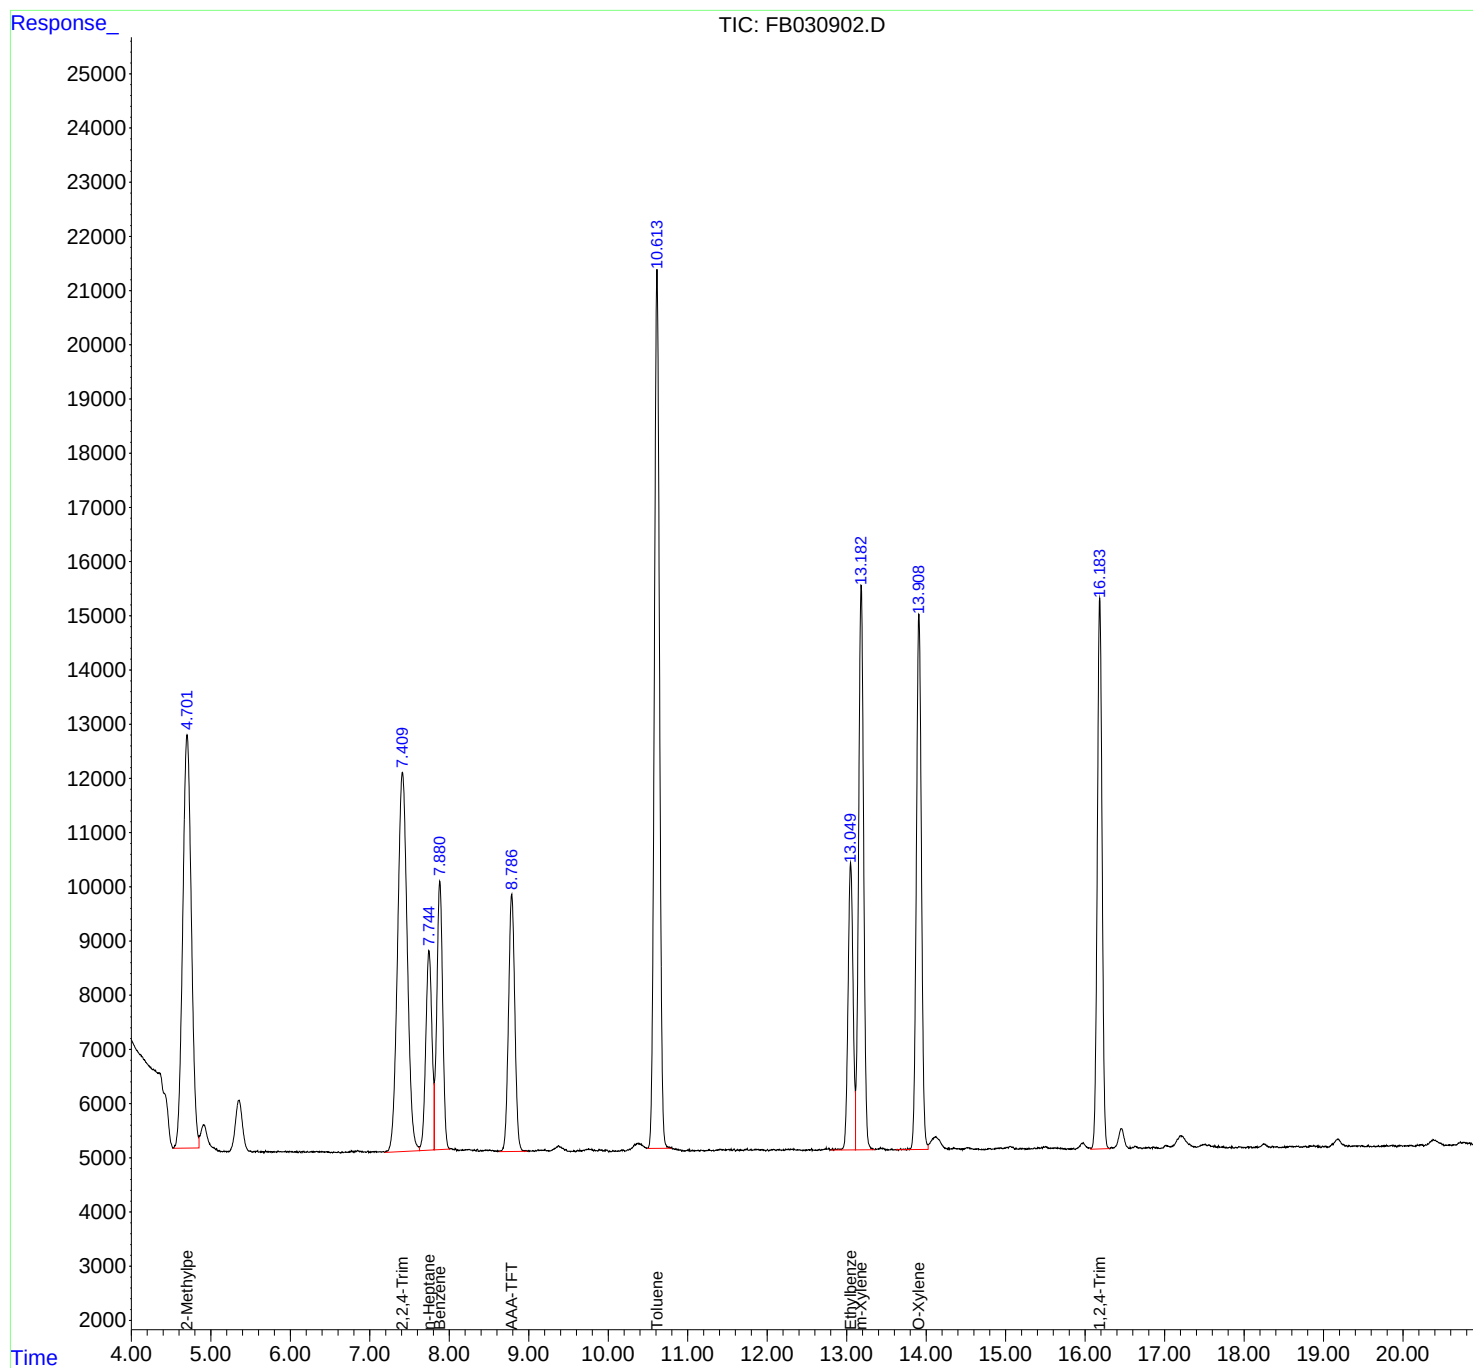


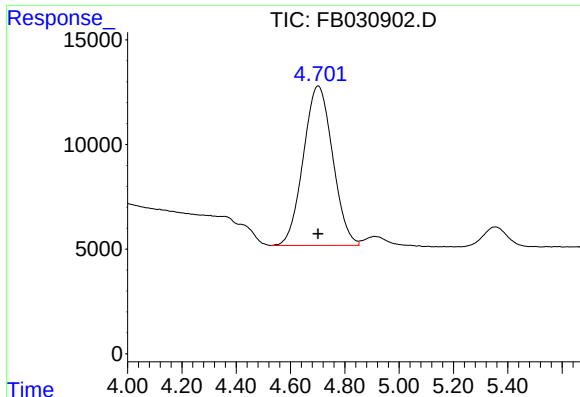

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 572364
Conc: 32.03 ng/ml

Instrument :
FID_B
ClientSampleId :

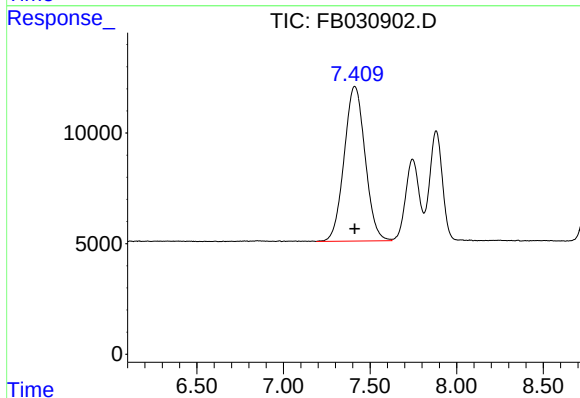


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 587981
Conc: 32.07 ng/ml

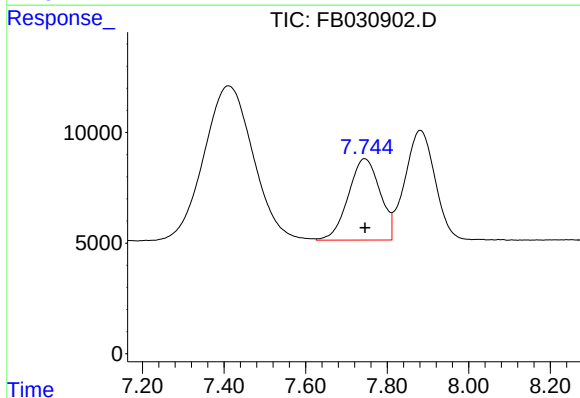


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.001 min
Response: 198549
Conc: 10.74 ng/ml

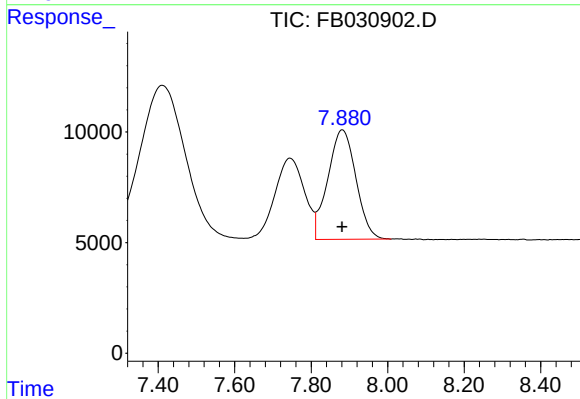

#4 Benzene


R.T.: 7.882 min
Delta R.T.: 0.000 min
Response: 252656
Conc: 11.18 ng/ml

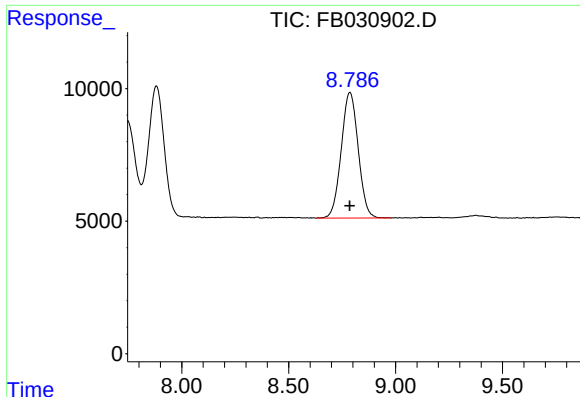

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 261595
Conc: 21.62 ng/ml

Instrument :
FID_B
ClientSampleId :

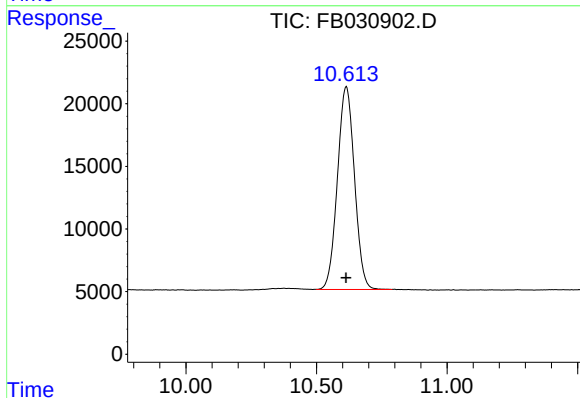


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.000 min
Response: 734387
Conc: 33.62 ng/ml

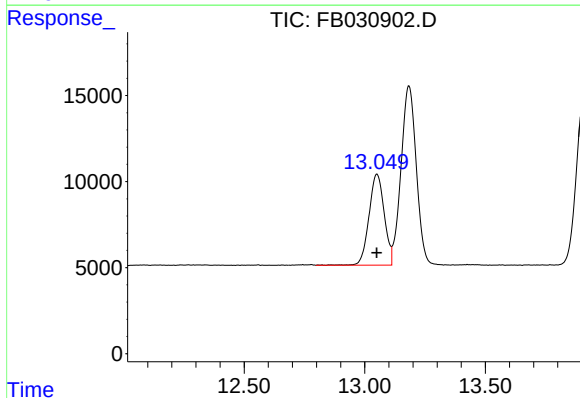


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.000 min
Response: 231519
Conc: 11.06 ng/ml

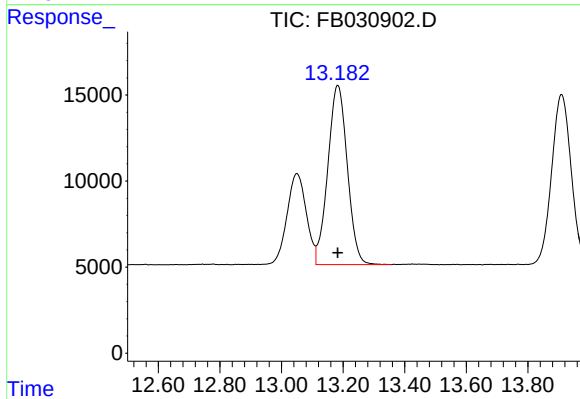

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 457977
Conc: 22.07 ng/ml

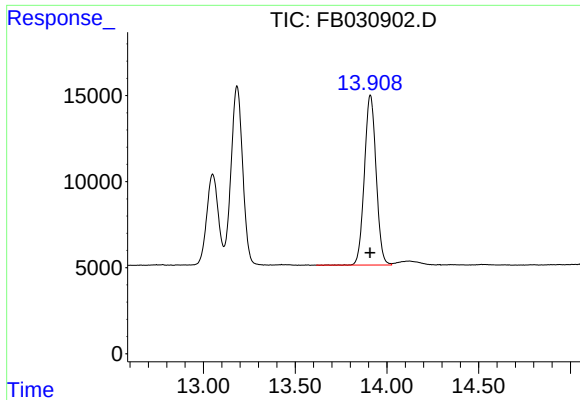

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.000 min
Response: 437146
Conc: 21.69 ng/ml

Instrument :
FID_B
ClientSampleId :

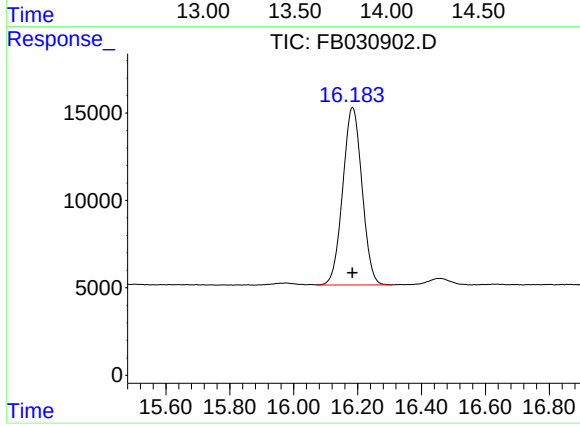

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.000 min
Response: 425411
Conc: 21.32 ng/ml