

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
 Data File : FB030905.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2024 12:56
 Operator : YP/AJ
 Sample : P3773-02MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-082824MS

Integration File: Calibration.e
 Quant Time: Aug 30 06:38:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.785	300506	24.837 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	475038	26.584 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	514608	28.067 ng/ml
3) t n-Heptane	7.743	172356	9.320 ng/ml
4) t Benzene	7.880	241491	10.689 ng/ml
6) t Toluene	10.613	691019	31.639 ng/ml
7) t Ethylbenzene	13.050	214920	10.267 ng/ml
8) t m-Xylene	13.182	426953	20.577 ng/ml
9) t O-Xylene	13.909	410077	20.347 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	379329	19.010 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
Data File : FB030905.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2024 12:56
Operator : YP/AJ
Sample : P3773-02MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-082824MS

Integration File: Calibration.e
Quant Time: Aug 30 06:38:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

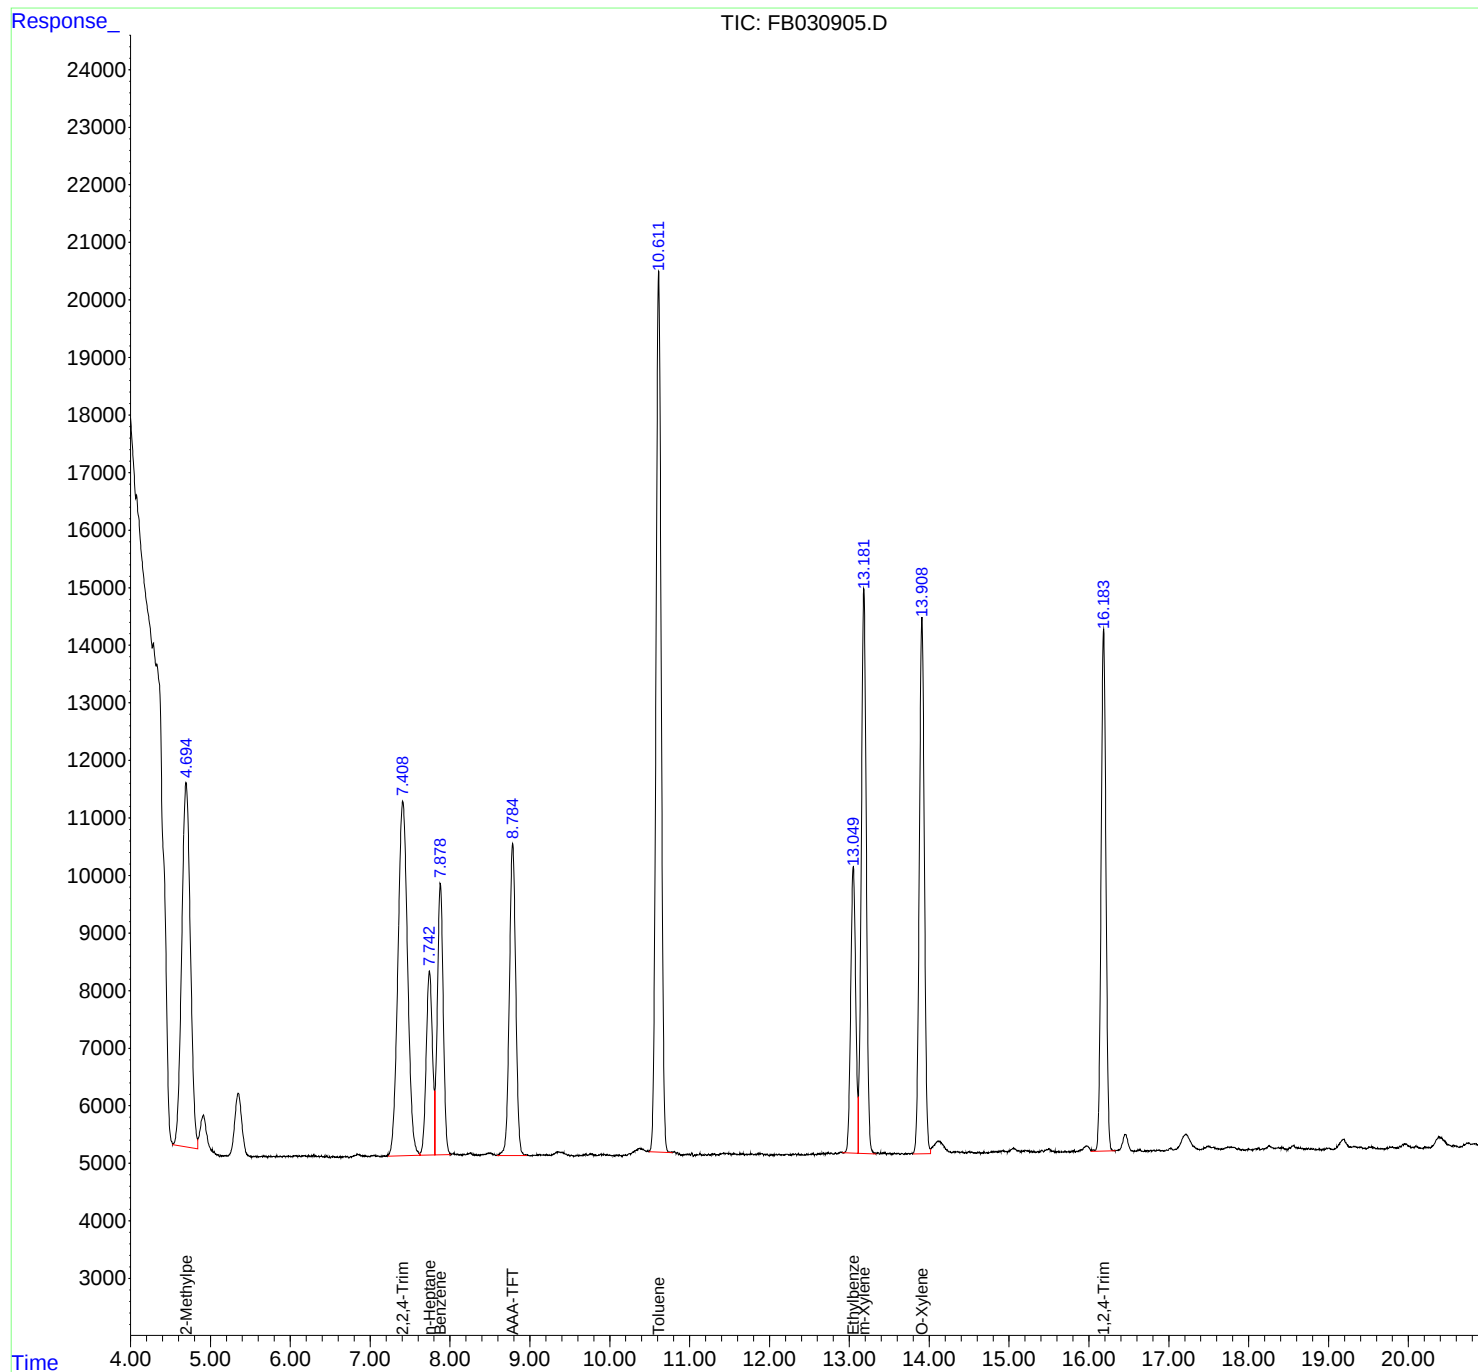


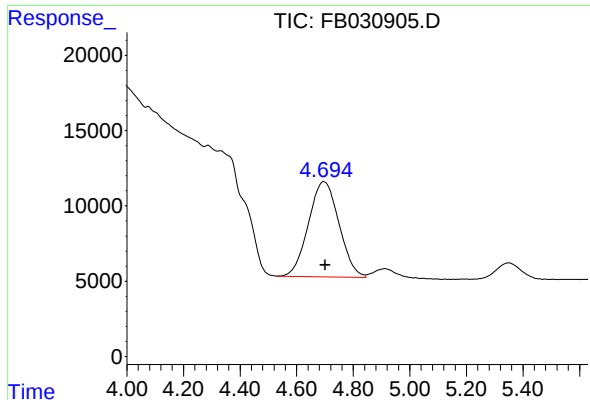

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: -0.006 min
Response: 475038
Conc: 26.58 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MS

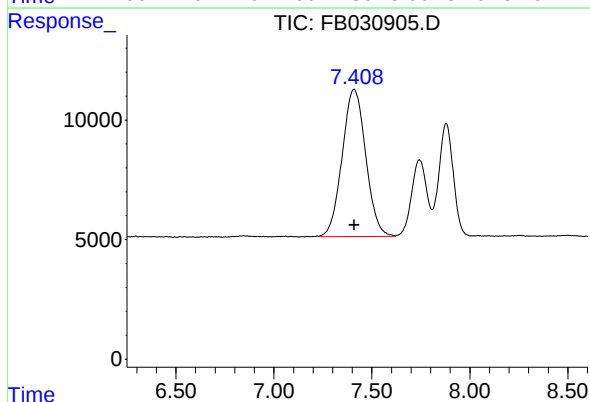


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.001 min
Response: 514608
Conc: 28.07 ng/ml

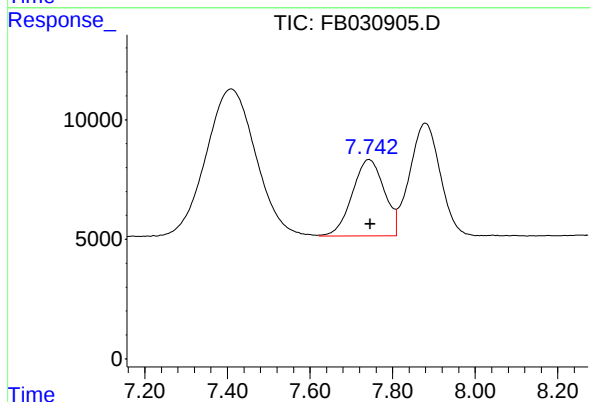


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.003 min
Response: 172356
Conc: 9.32 ng/ml

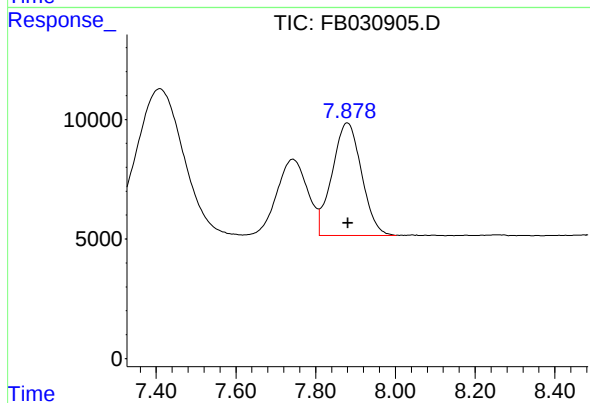

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.002 min
Response: 241491
Conc: 10.69 ng/ml

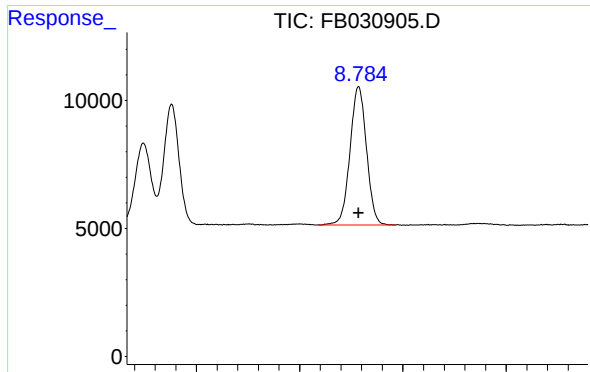

#5 AAA-TFT


R.T.: 8.785 min
Delta R.T.: -0.001 min
Response: 300506
Conc: 24.84 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MS

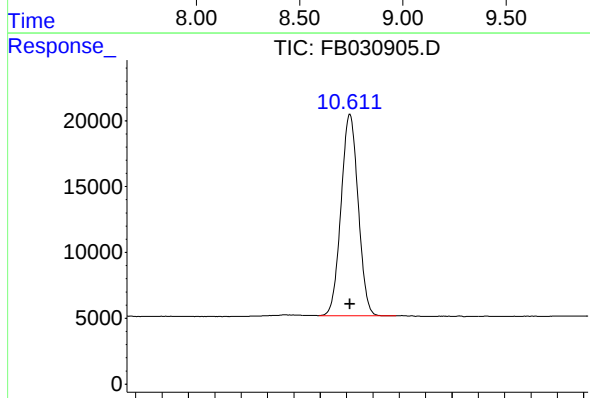


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.001 min
Response: 691019
Conc: 31.64 ng/ml

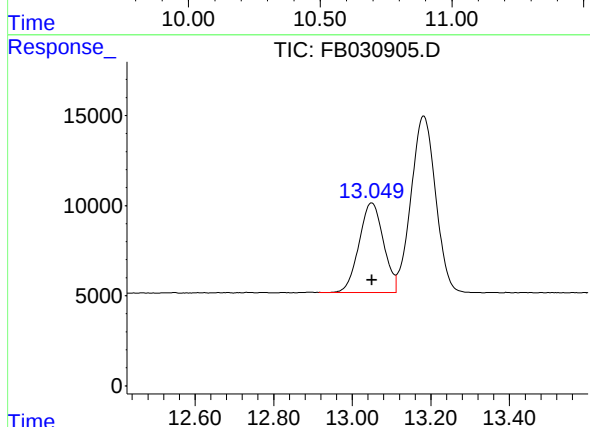


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.000 min
Response: 214920
Conc: 10.27 ng/ml

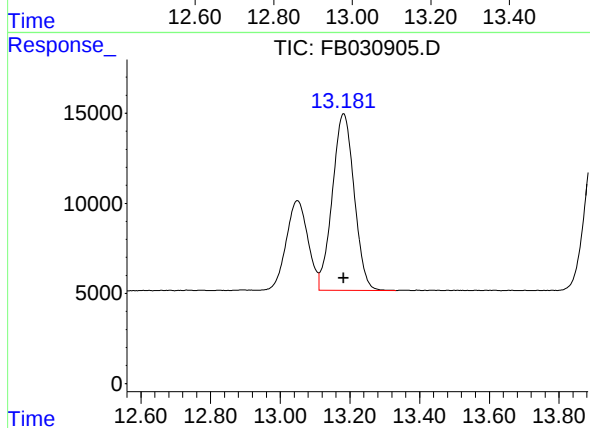

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: 0.000 min
Response: 426953
Conc: 20.58 ng/ml

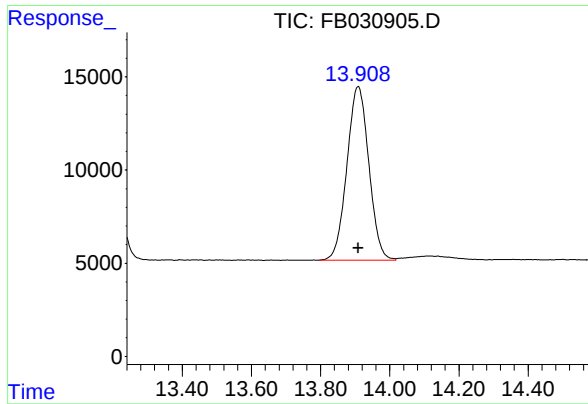

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.000 min
Response: 410077
Conc: 20.35 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MS

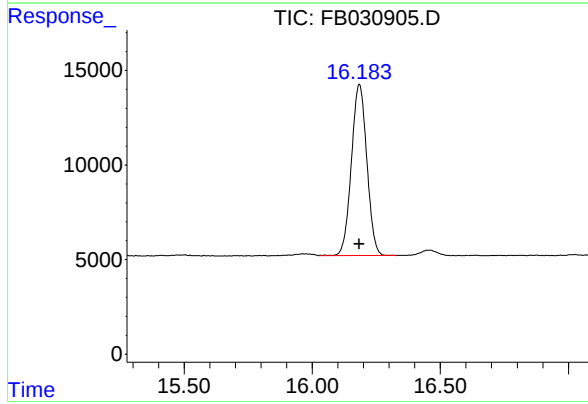

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: 0.000 min
Response: 379329
Conc: 19.01 ng/ml