

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
 Data File : FB030906.D
 Signal(s) : FID2B.CH
 Acq On : 29 Aug 2024 13:35
 Operator : YP/AJ
 Sample : P3773-02MSD
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-082824MSD

Integration File: Calibration.e
 Quant Time: Aug 30 06:38:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
 Quant Title :
 QLast Update : Tue Aug 27 11:54:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	281686	23.282 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	413855	23.160 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	482090	26.293 ng/ml
3) t n-Heptane	7.744	154231	8.339 ng/ml
4) t Benzene	7.880	217974	9.648 ng/ml
6) t Toluene	10.614	619560	28.367 ng/ml
7) t Ethylbenzene	13.051	193452	9.241 ng/ml
8) t m-Xylene	13.184	383508	18.483 ng/ml
9) t O-Xylene	13.910	370609	18.388 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	344272	17.254 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082924\
Data File : FB030906.D
Signal(s) : FID2B.CH
Acq On : 29 Aug 2024 13:35
Operator : YP/AJ
Sample : P3773-02MSD
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-082824MSD

Integration File: Calibration.e
Quant Time: Aug 30 06:38:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082724.M
Quant Title :
QLast Update : Tue Aug 27 11:54:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

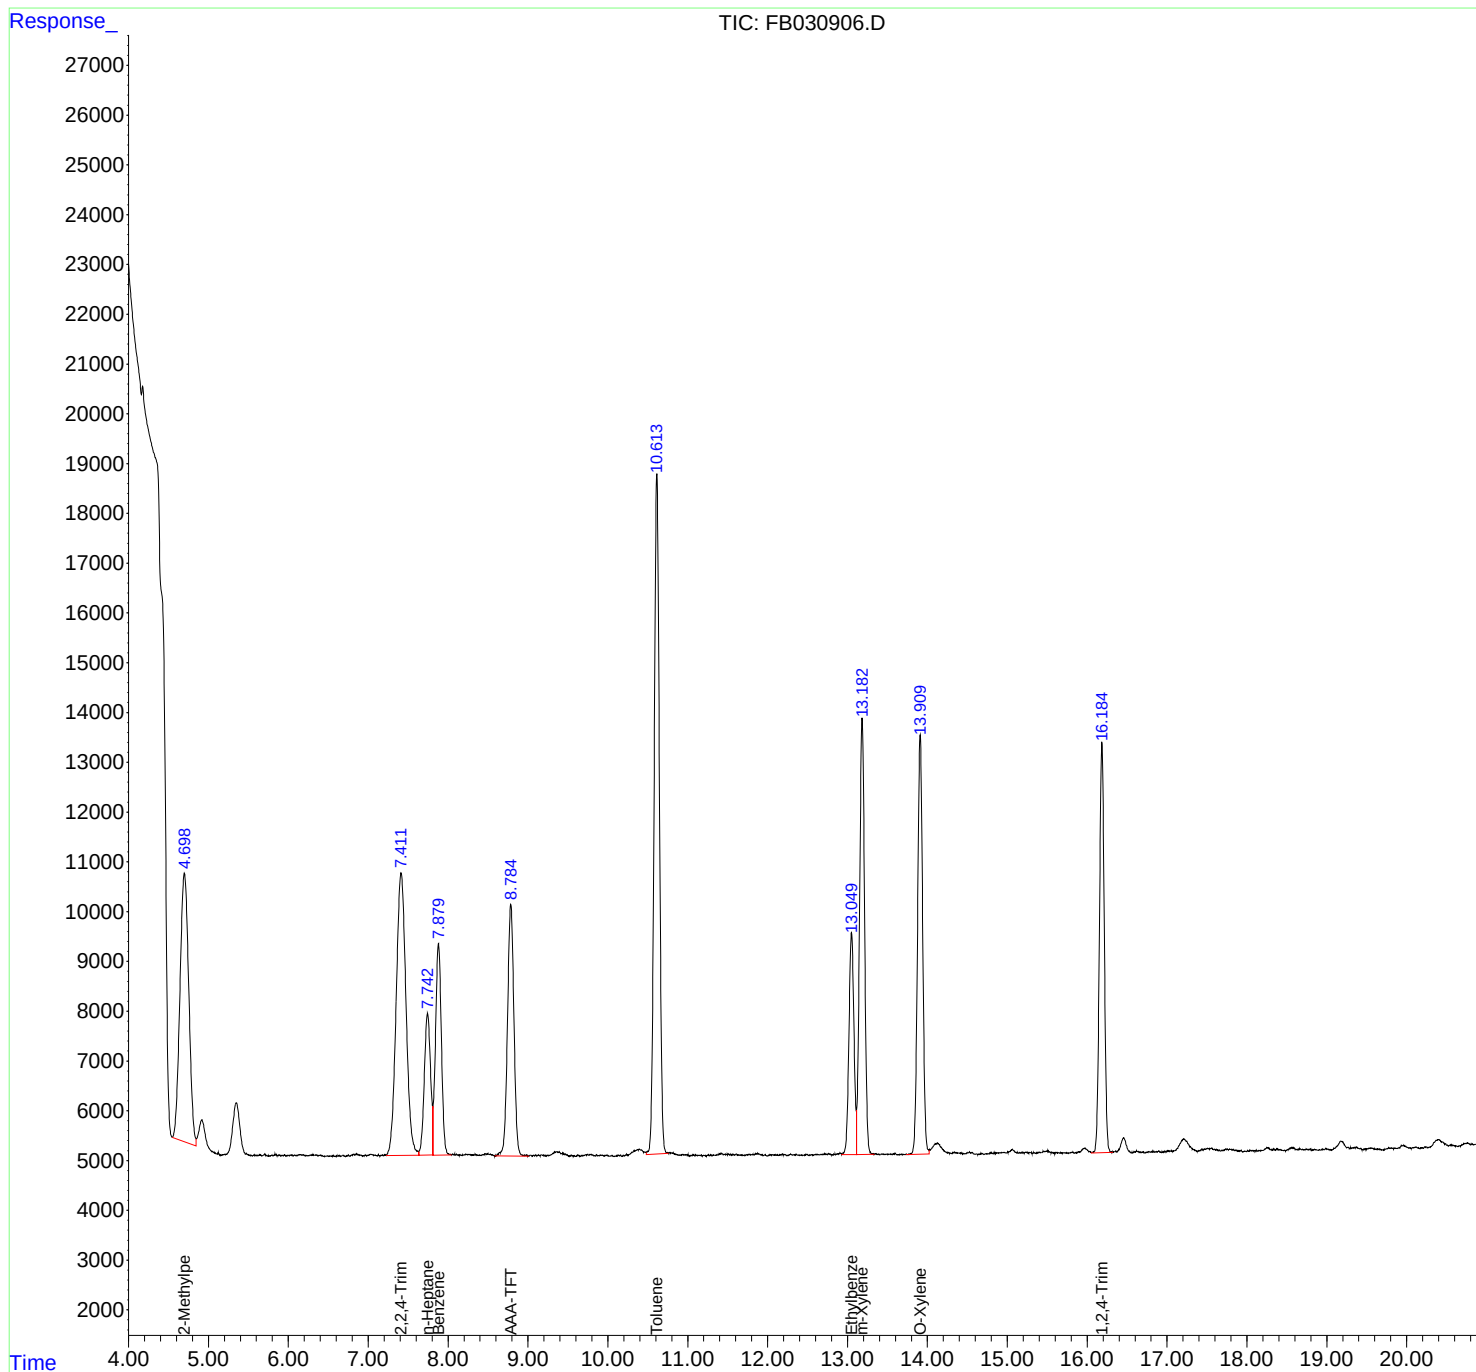


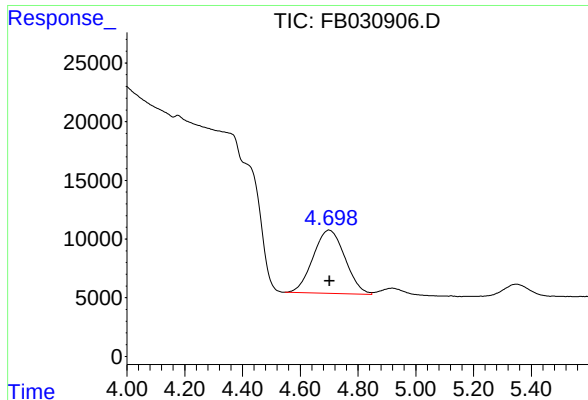

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.003 min
Response: 413855
Conc: 23.16 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MSD

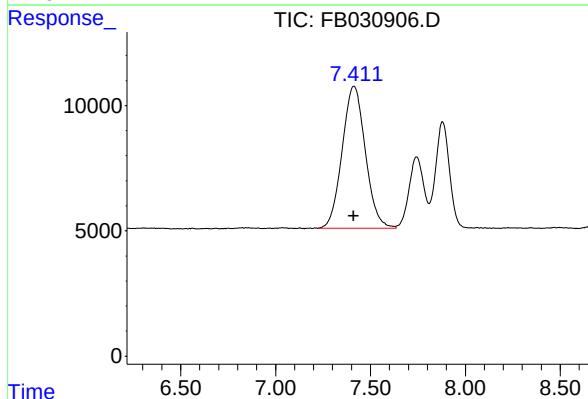


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.001 min
Response: 482090
Conc: 26.29 ng/ml

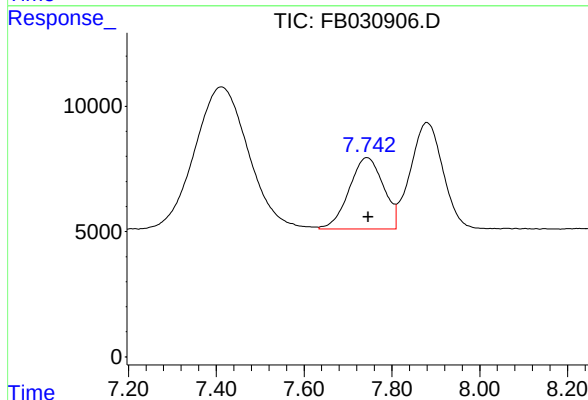


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.003 min
Response: 154231
Conc: 8.34 ng/ml

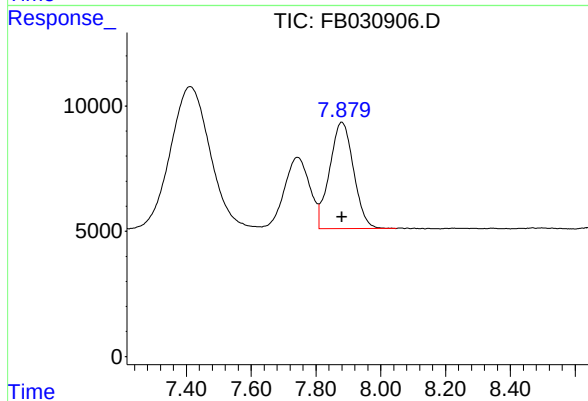

#4 Benzene


R.T.: 7.880 min
Delta R.T.: 0.000 min
Response: 217974
Conc: 9.65 ng/ml

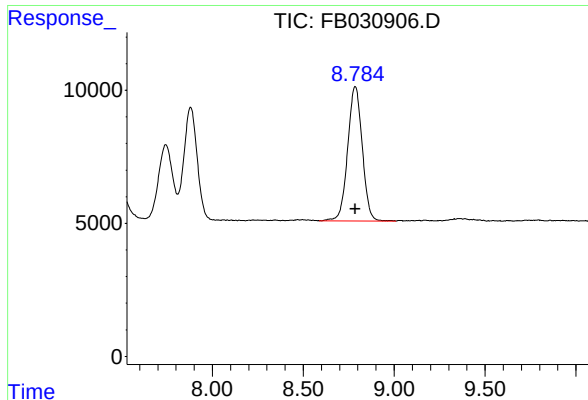

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 281686
Conc: 23.28 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MSD

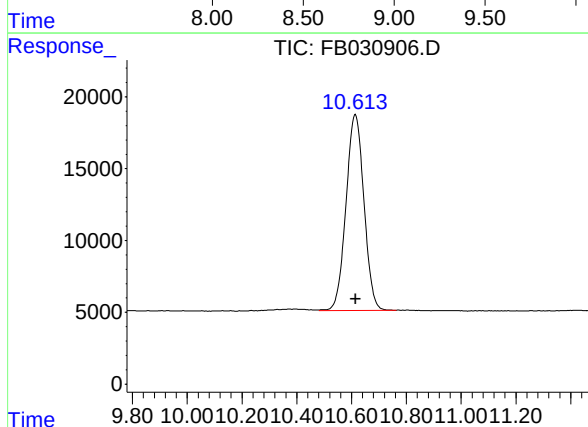


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 619560
Conc: 28.37 ng/ml

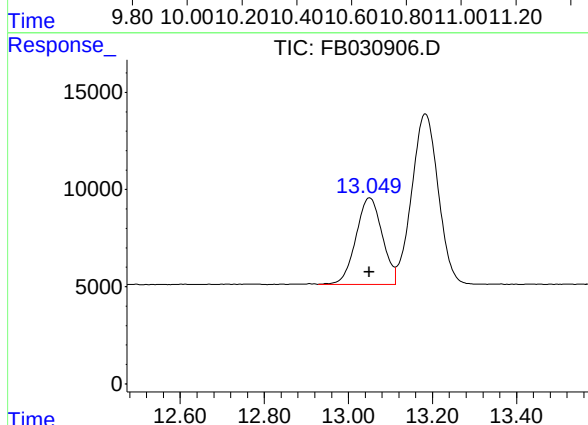


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.000 min
Response: 193452
Conc: 9.24 ng/ml

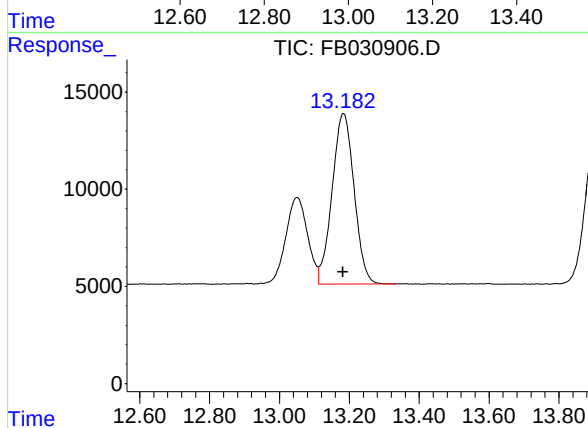

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.001 min
Response: 383508
Conc: 18.48 ng/ml

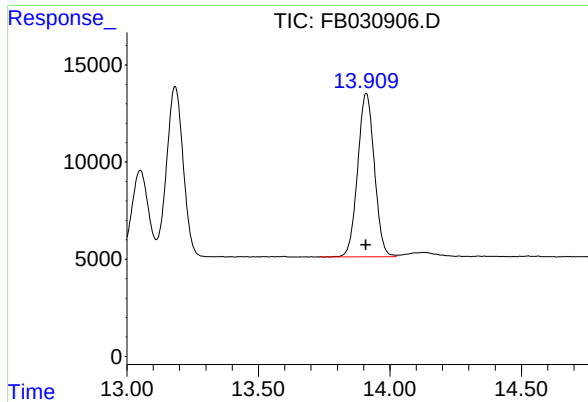

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.000 min
Response: 370609
Conc: 18.39 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-082824MSD

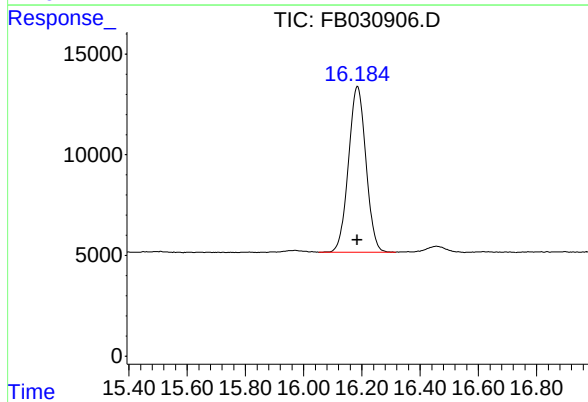

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.001 min
Response: 344272
Conc: 17.25 ng/ml