

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083018\
 Data File : FB017585.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2018 11:10
 Operator : MJ/SJ
 Sample : J4282-19MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 30 12:32:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.110	164785	19.987 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	338334	24.146 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	334359	23.727 ng/ml
3) t n-Heptane	8.065	95333	6.917 ng/ml
4) t Benzene	8.206	153858	8.727 ng/ml
6) t Toluene	10.960	380098	26.422 ng/ml
7) t Ethylbenzene	13.410	131177	8.895 ng/ml
8) t m-Xylene	13.542	276107	17.761 ng/ml
9) t O-Xylene	14.274	289733	17.650 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	329318	16.908 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083018\
Data File : FB017585.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2018 11:10
Operator : MJ/SJ
Sample : J4282-19MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 30 12:32:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

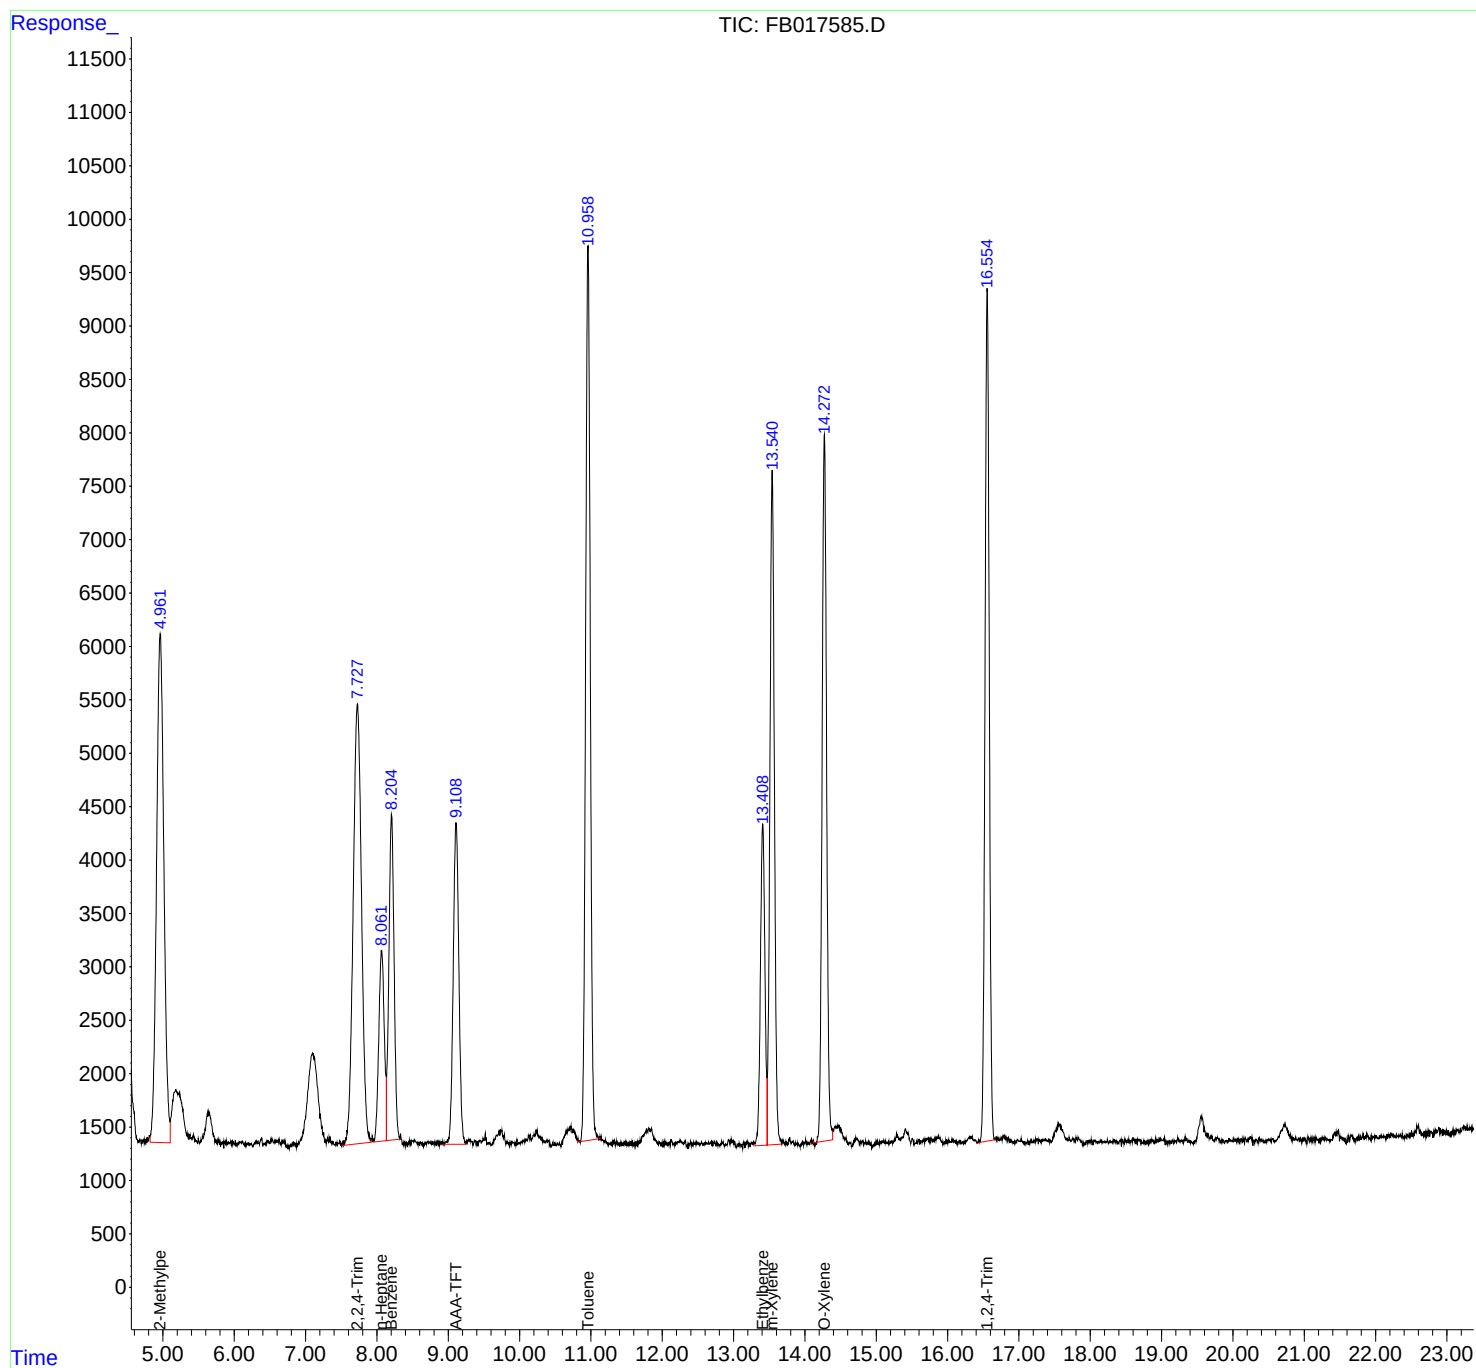

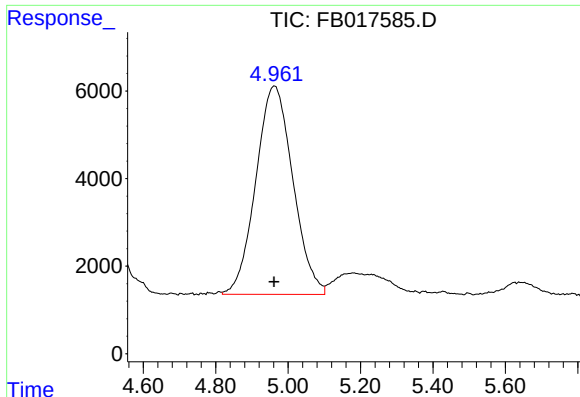


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: 0.002 min
Response: 338334
Conc: 24.15 ng/ml

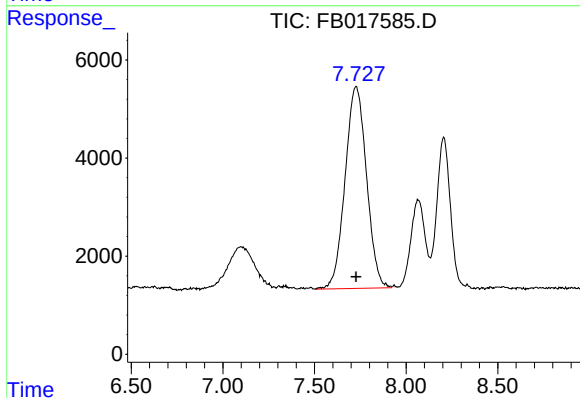


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 334359
Conc: 23.73 ng/ml

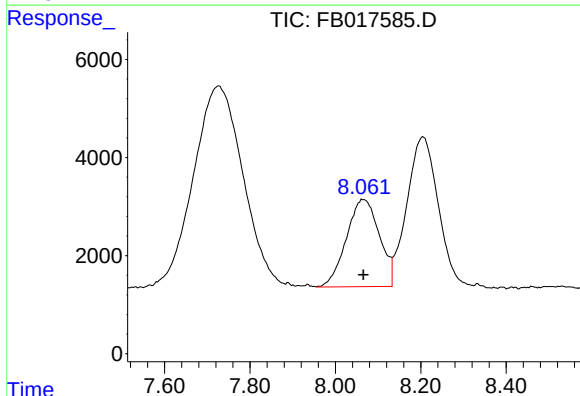


#3 n-Heptane

R.T.: 8.065 min
Delta R.T.: -0.001 min
Response: 95333
Conc: 6.92 ng/ml

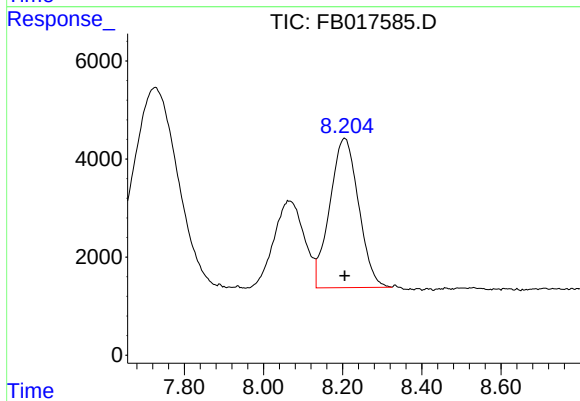


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 153858
Conc: 8.73 ng/ml

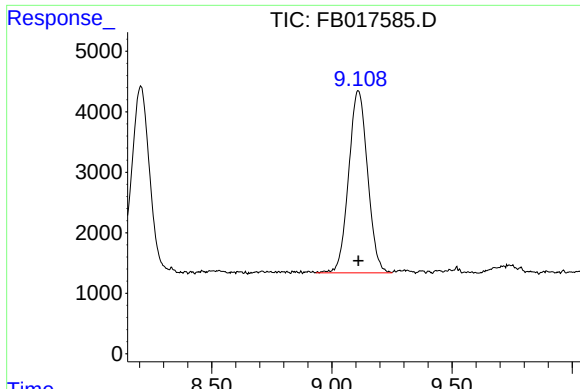


#5 AAA-TFT

R.T.: 9.110 min
Delta R.T.: -0.001 min
Response: 164785
Conc: 19.99 ng/ml

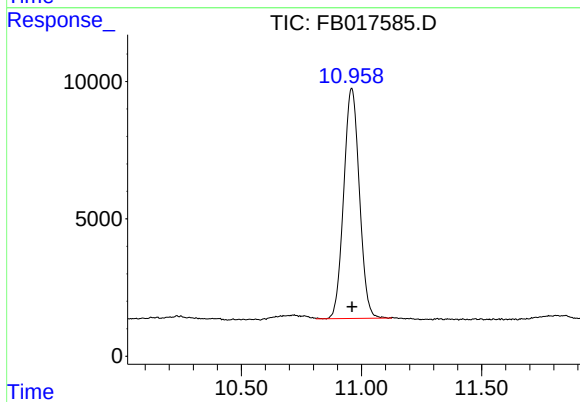


#6 Toluene

R.T.: 10.960 min
Delta R.T.: 0.000 min
Response: 380098
Conc: 26.42 ng/ml

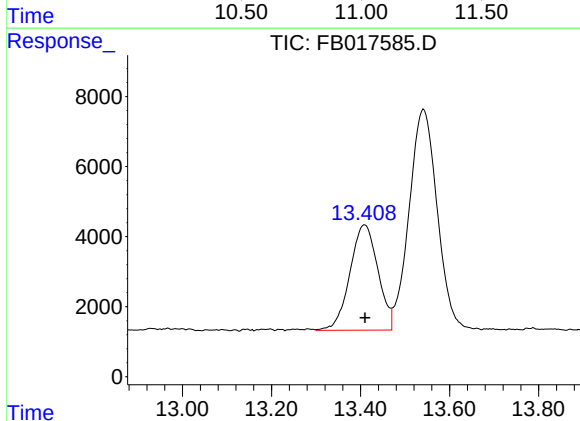


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 131177
Conc: 8.89 ng/ml

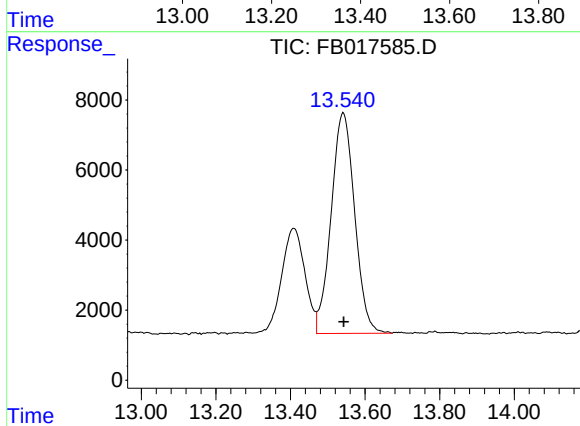


#8 m-Xylene

R.T.: 13.542 min
Delta R.T.: 0.000 min
Response: 276107
Conc: 17.76 ng/ml

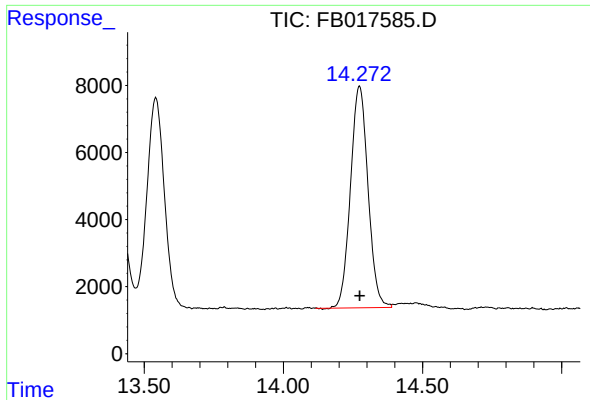

#9 O-Xylene

R.T.: 14.274 min
Delta R.T.: 0.000 min
Response: 289733
Conc: 17.65 ng/ml

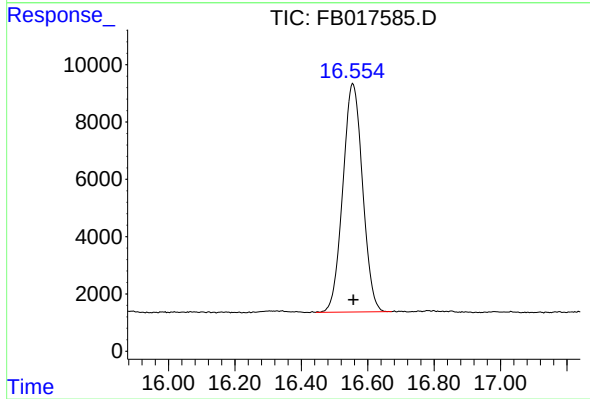

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.002 min
Response: 329318
Conc: 16.91 ng/ml